

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111519\
 Data File : FB023004.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2019 11:54
 Operator : DD/AJ
 Sample : BSF1115S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 15 22:04:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	504499	22.410 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	1000002	31.087 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1134556	32.140 ng/ml
3) t n-Heptane	7.756	366601	10.539 ng/ml
4) t Benzene	7.891	455588	10.518 ng/ml
6) t Toluene	10.629	1334612	30.958 ng/ml
7) t Ethylbenzene	13.070	420819	10.541 ng/ml
8) t m-Xylene	13.203	790288	20.925 ng/ml
9) t O-Xylene	13.931	743689	20.866 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	630595	22.236 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111519\
Data File : FB023004.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2019 11:54
Operator : DD/AJ
Sample : BSF1115S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 22:04:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

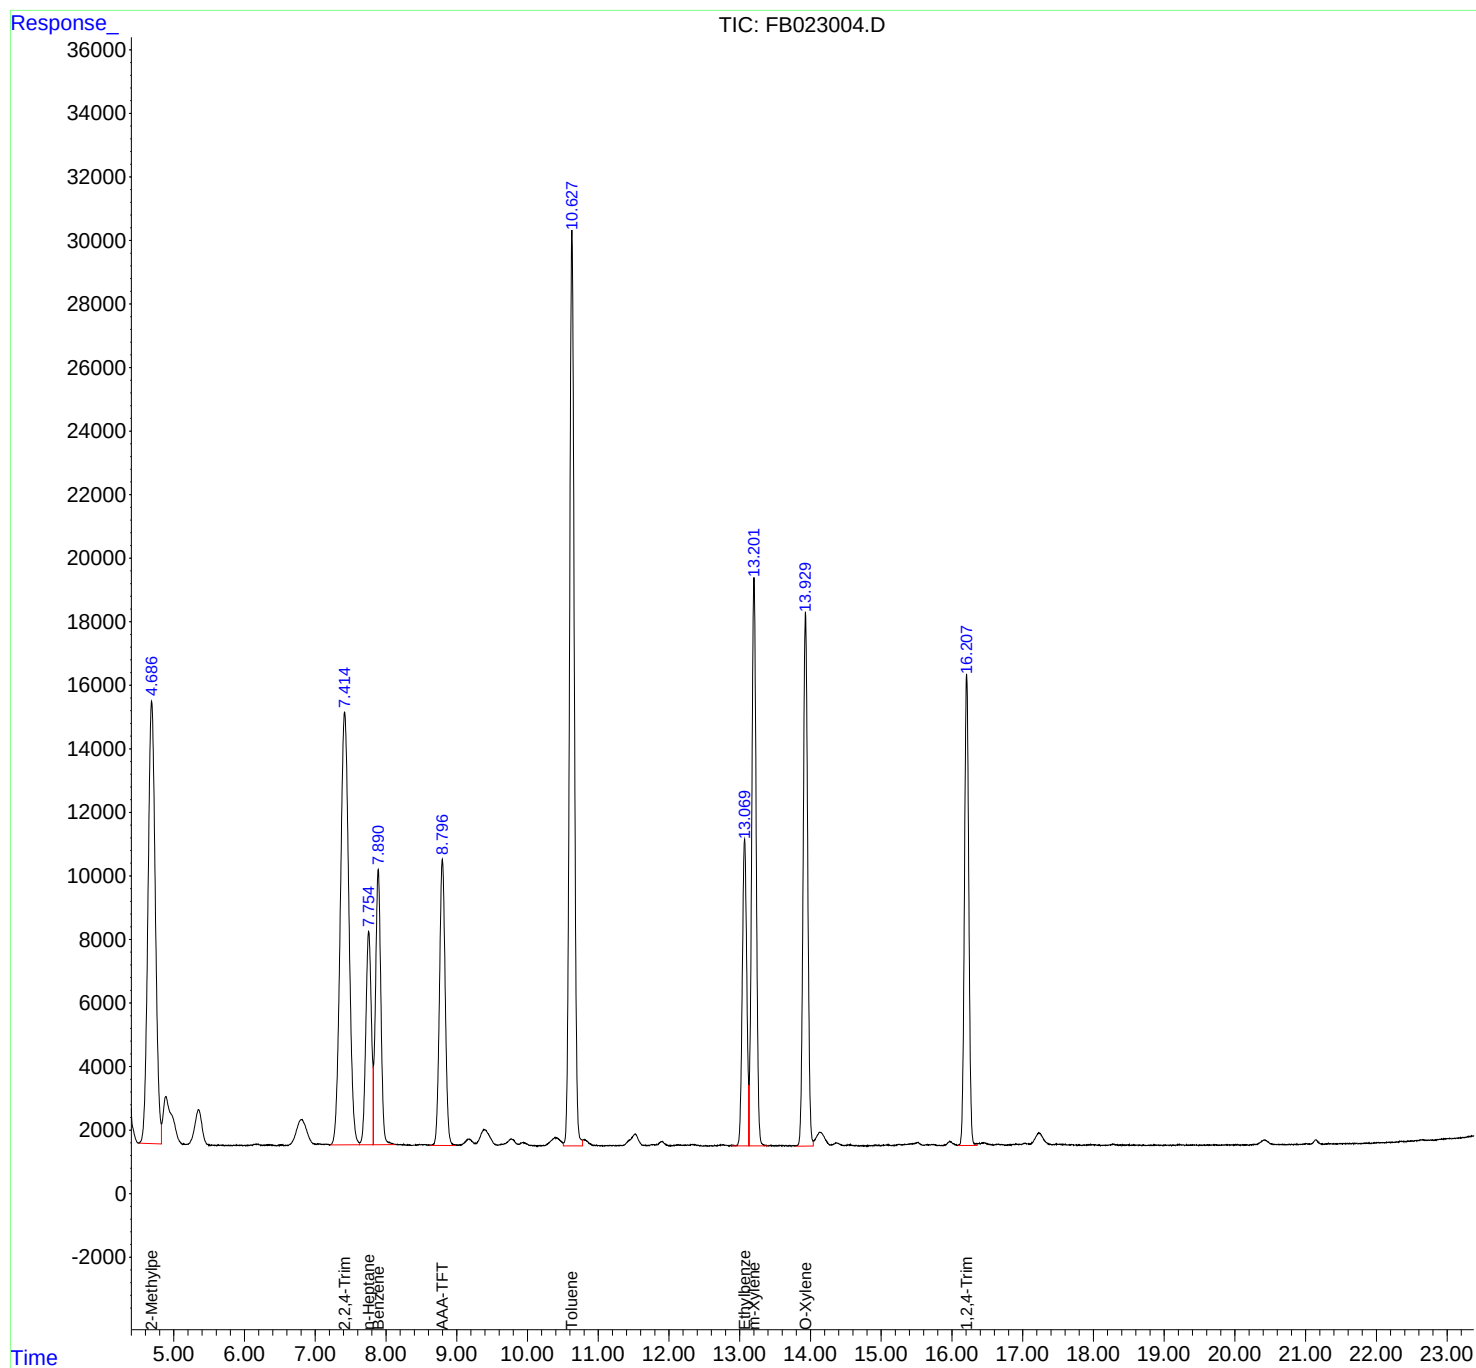

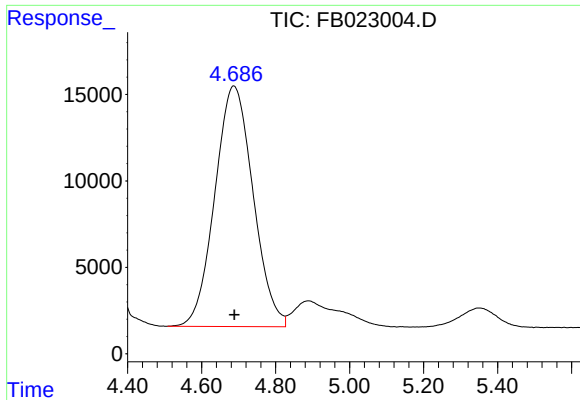


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.001 min
Response: 1000002
Conc: 31.09 ng/ml

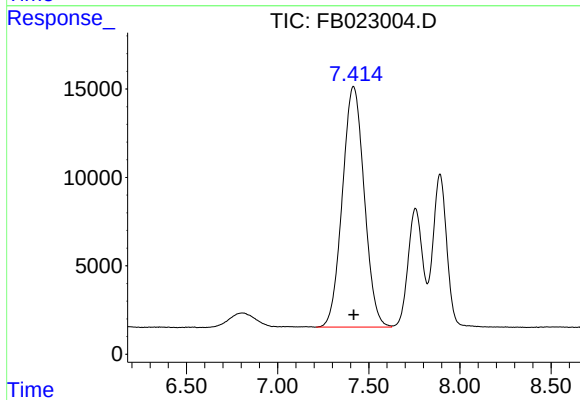


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 1134556
Conc: 32.14 ng/ml

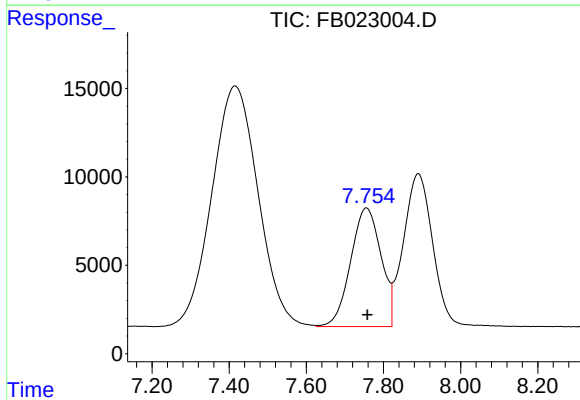


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 366601
Conc: 10.54 ng/ml

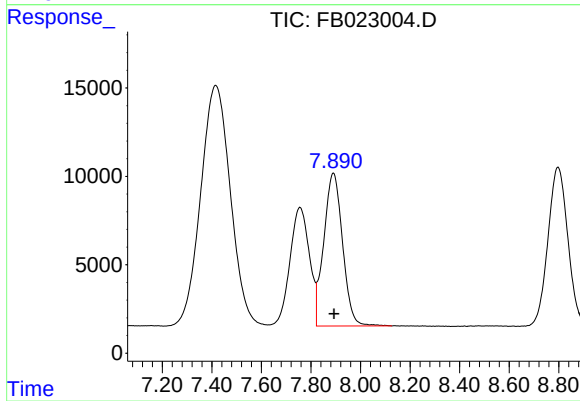


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 455588
Conc: 10.52 ng/ml

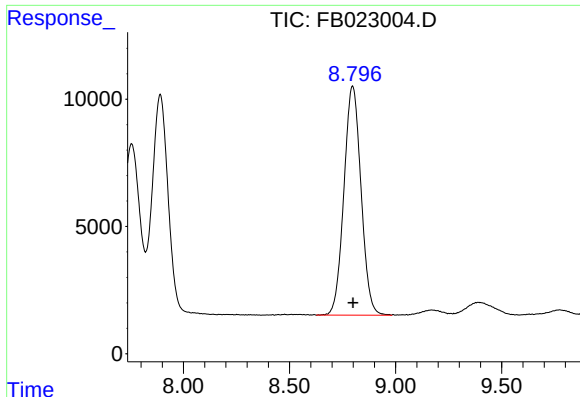


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 504499
Conc: 22.41 ng/ml

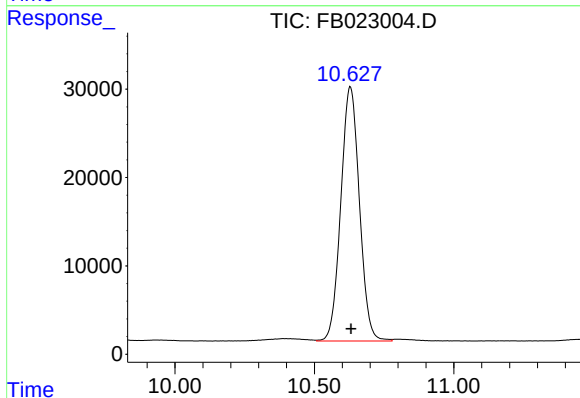


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 1334612
Conc: 30.96 ng/ml

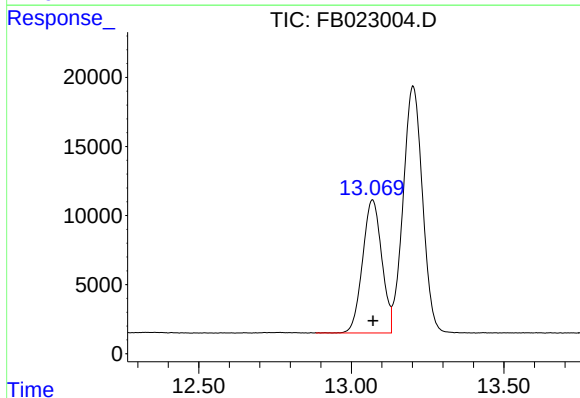


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.002 min
Response: 420819
Conc: 10.54 ng/ml

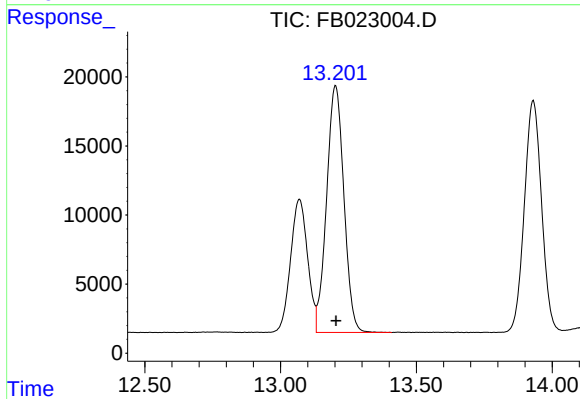


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.002 min
Response: 790288
Conc: 20.93 ng/ml

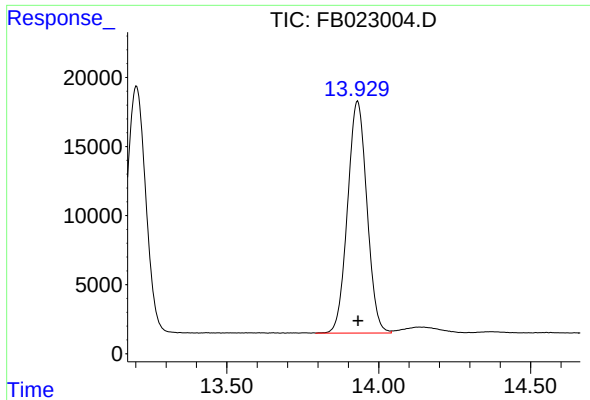

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.002 min
Response: 743689
Conc: 20.87 ng/ml

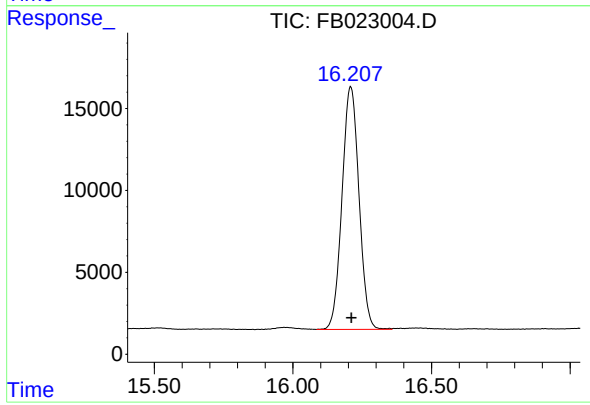

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 630595
Conc: 22.24 ng/ml