

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111519\
Data File : FB023005.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2019 12:46
Operator : DD/AJ
Sample : K5864-02
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 22:04:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	482693	21.442 ng/ml
Target Compounds				
6) t	Toluene	10.618	5358	0.124 ng/ml
8) t	m-Xylene	13.204	1857	0.049 ng/ml
9) t	O-Xylene	13.935	1368	0.038 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	2401	0.085 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111519\
Data File : FB023005.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2019 12:46
Operator : DD/AJ
Sample : K5864-02
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 22:04:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

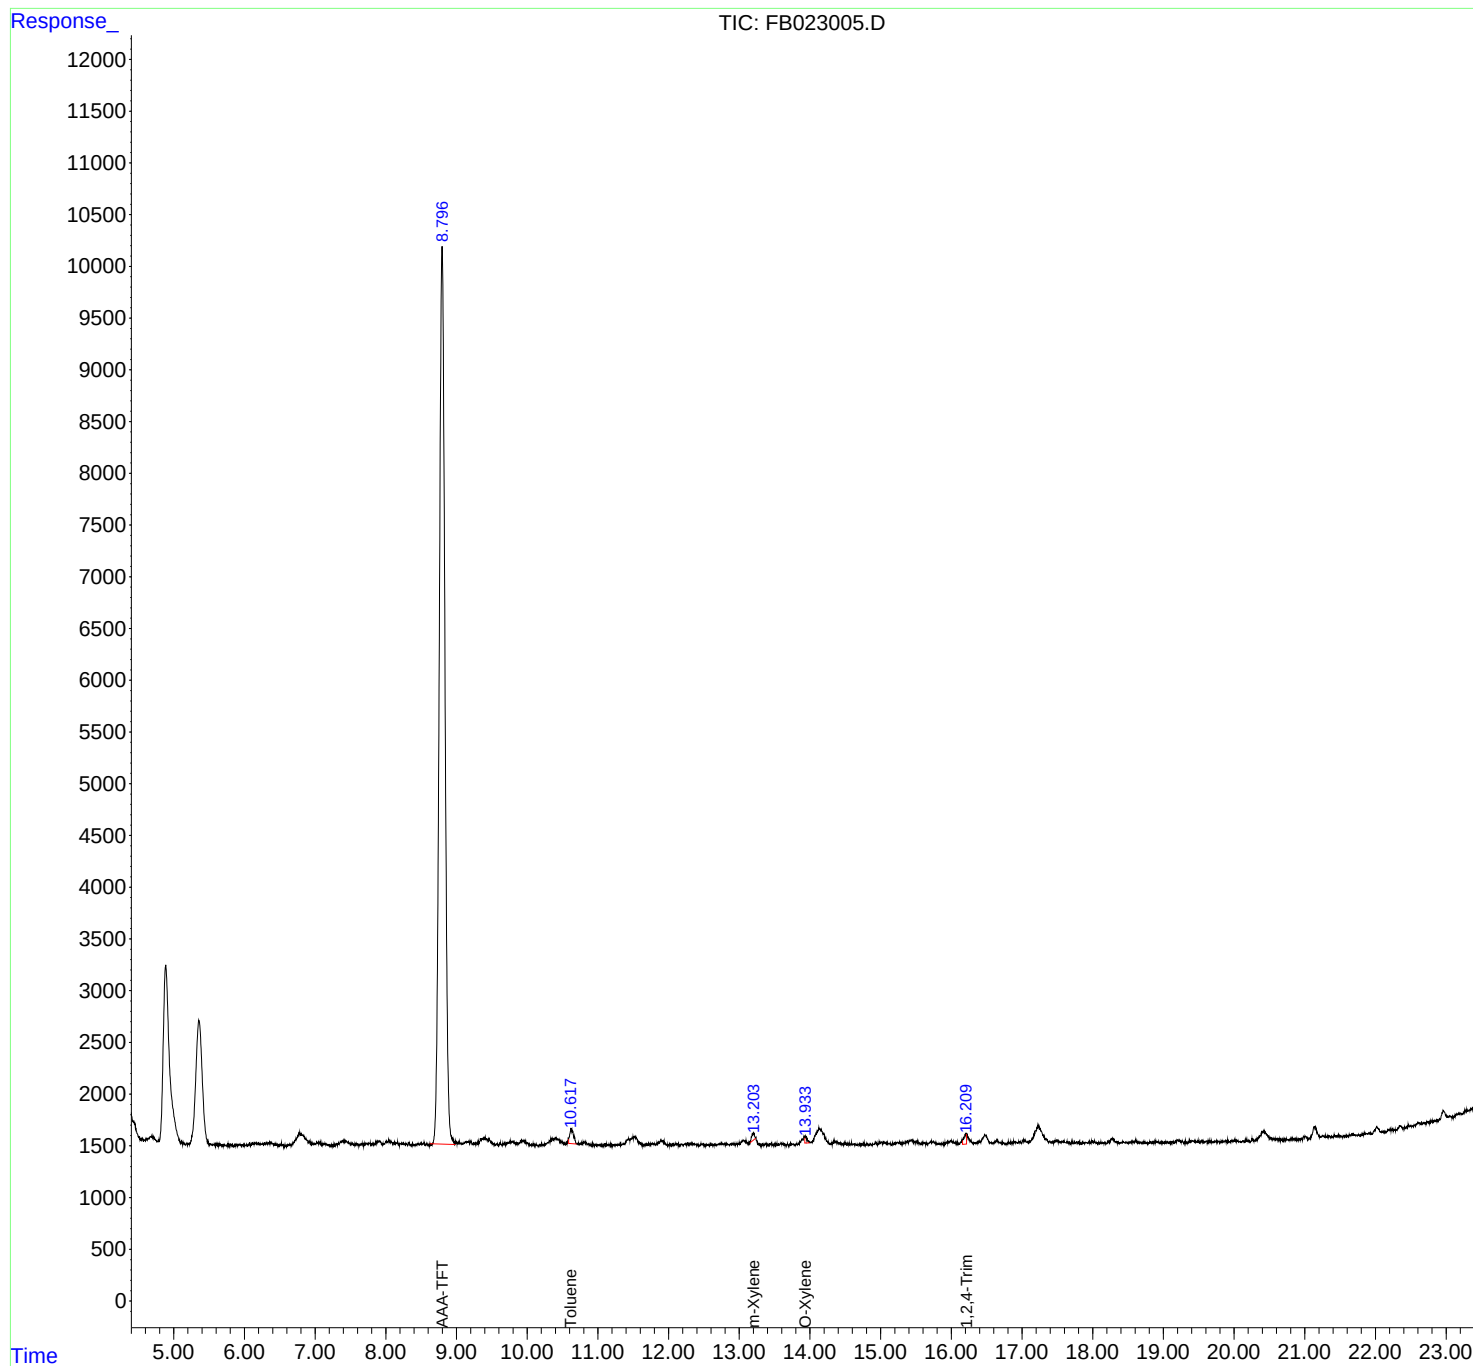

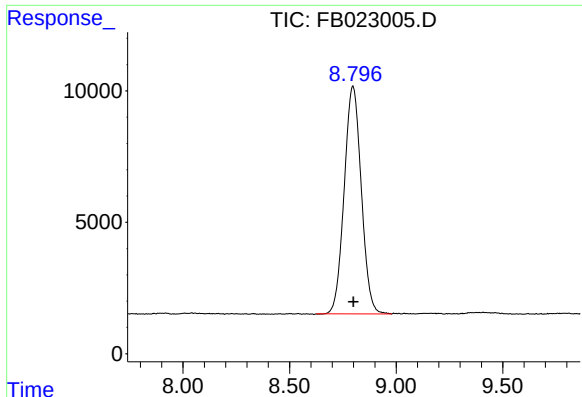


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 482693
Conc: 21.44 ng/ml

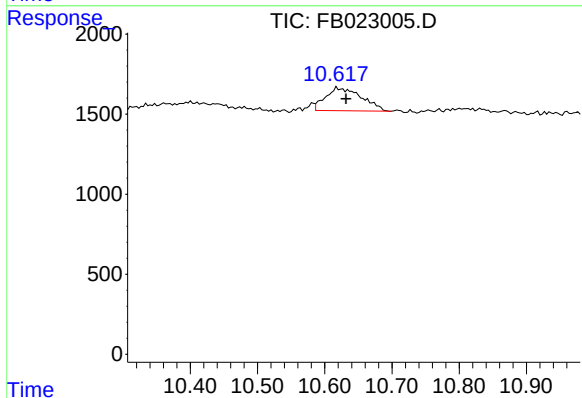


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.013 min
Response: 5358
Conc: 0.12 ng/ml

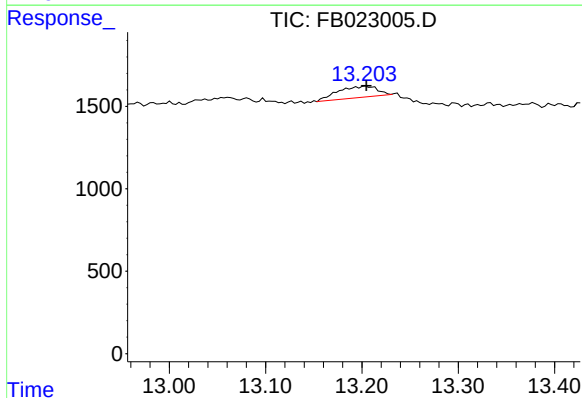


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 1857
Conc: 0.05 ng/ml

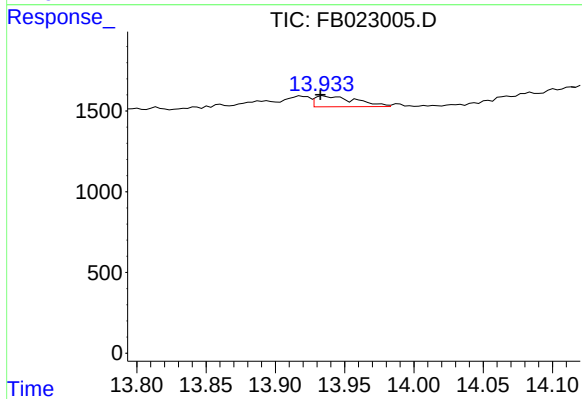

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.003 min
Response: 1368
Conc: 0.04 ng/ml

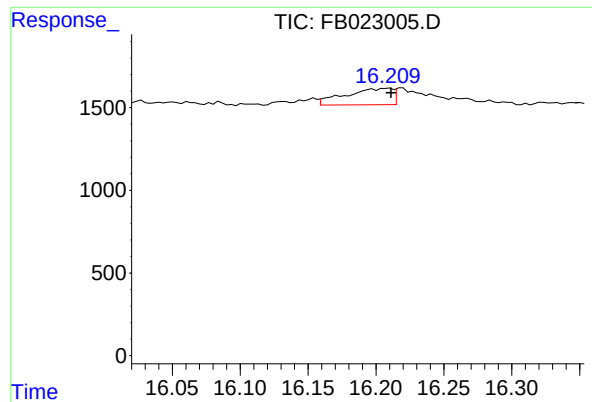

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 2401
Conc: 0.08 ng/ml