

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111519\
 Data File : FB023007.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2019 13:46
 Operator : DD/AJ
 Sample : K5864-02MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 15 22:04:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	423752	18.823 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	786302	24.444 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	901331	25.533 ng/ml
3) t n-Heptane	7.755	287759	8.272 ng/ml
4) t Benzene	7.890	394000	9.096 ng/ml
6) t Toluene	10.629	1165307	27.031 ng/ml
7) t Ethylbenzene	13.069	376493	9.431 ng/ml
8) t m-Xylene	13.202	727051	19.251 ng/ml
9) t O-Xylene	13.930	695420	19.512 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	579073	20.420 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111519\
Data File : FB023007.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2019 13:46
Operator : DD/AJ
Sample : K5864-02MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 15 22:04:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

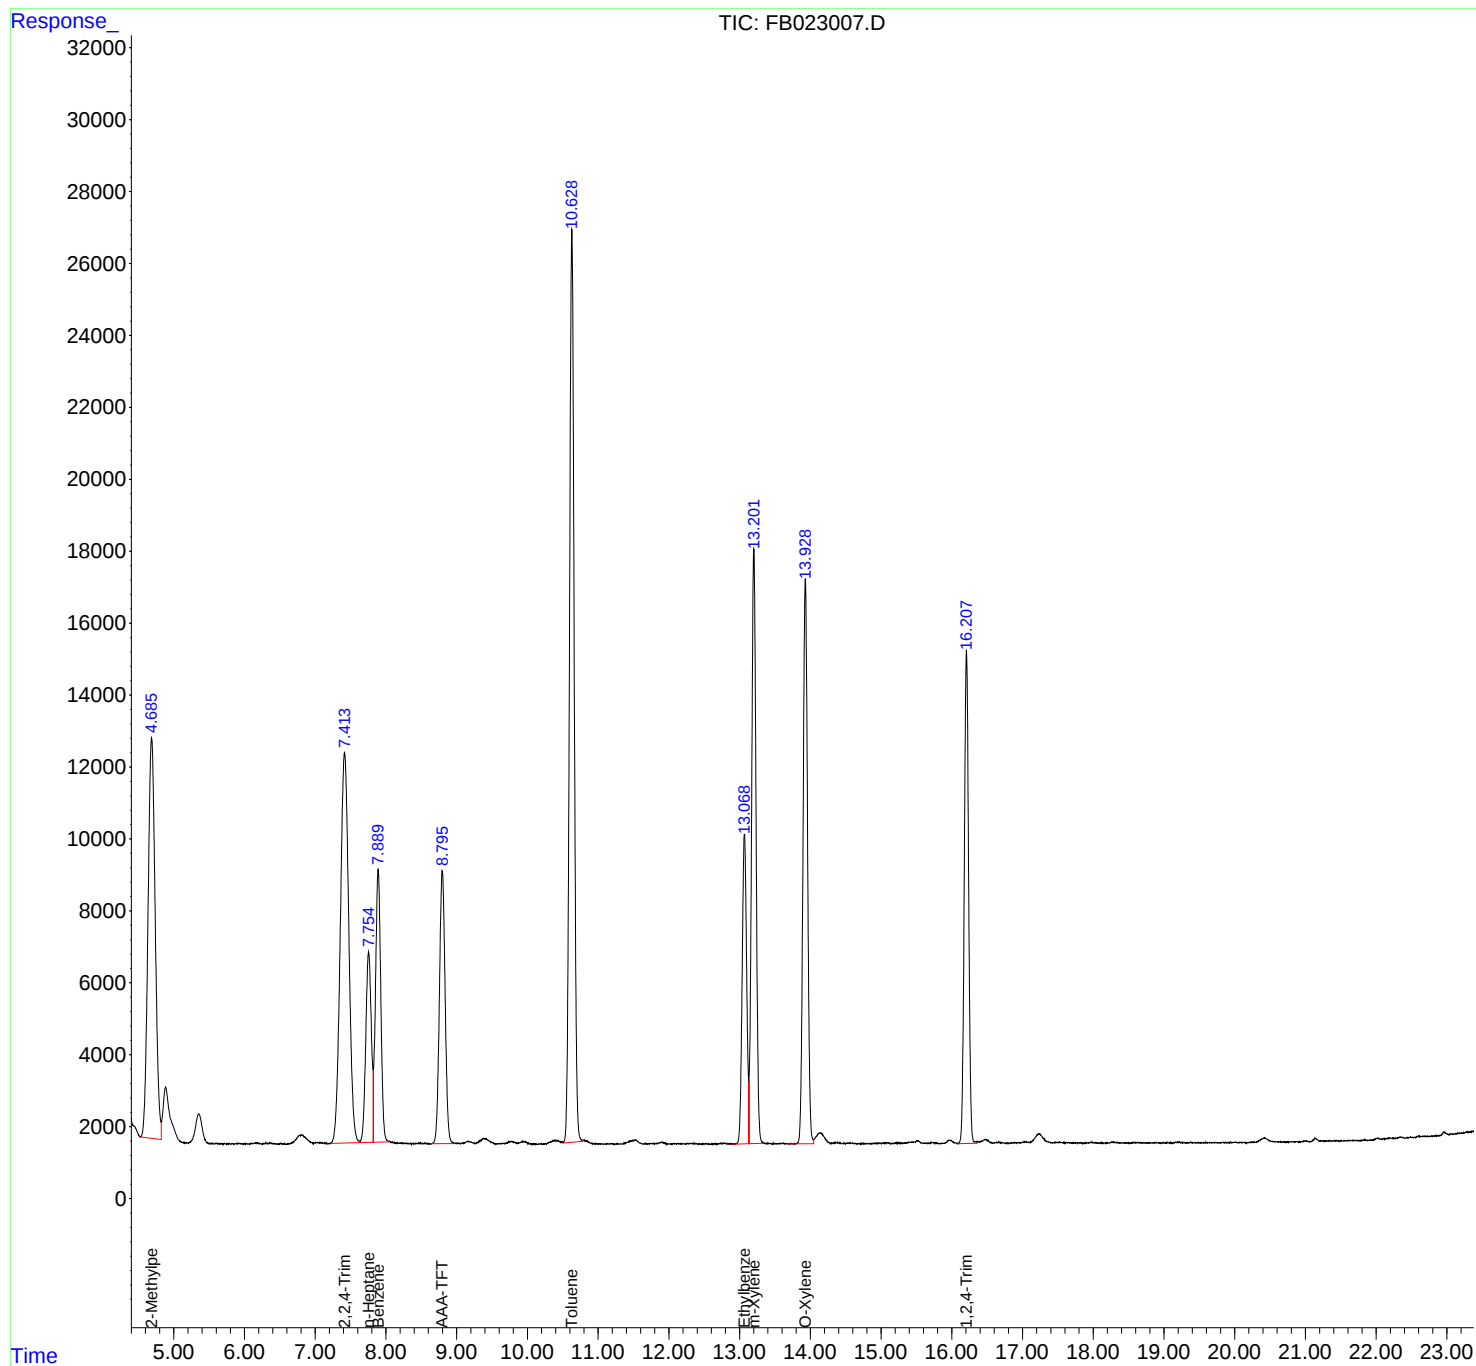

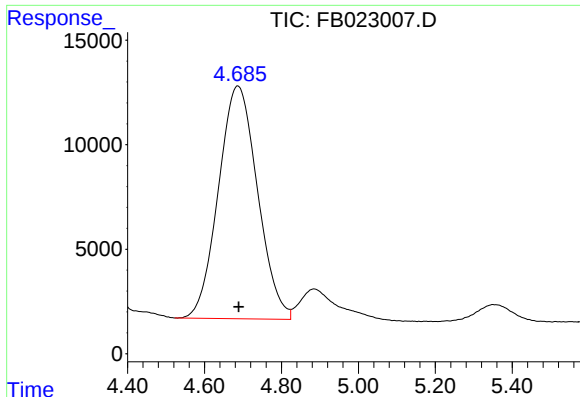


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 786302
Conc: 24.44 ng/ml

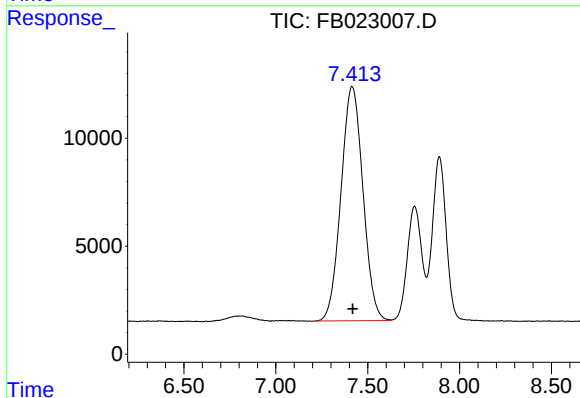


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 901331
Conc: 25.53 ng/ml

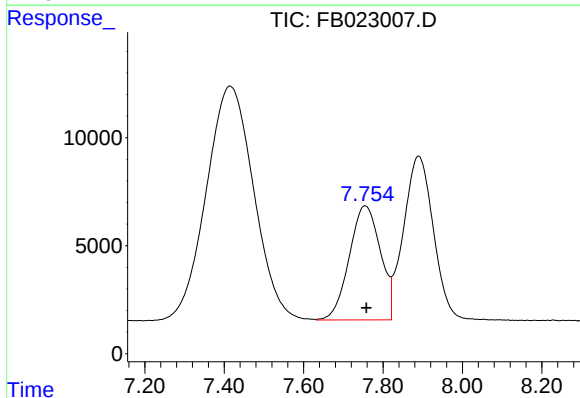


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 287759
Conc: 8.27 ng/ml

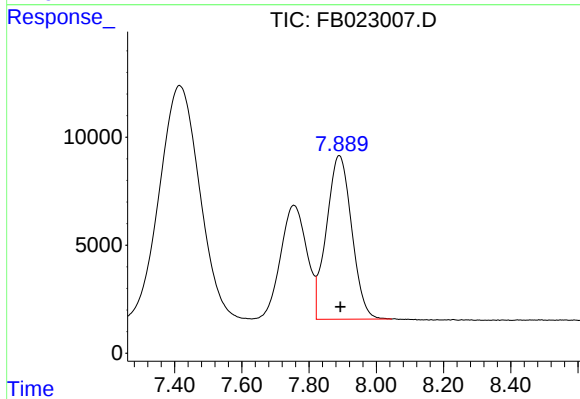


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 394000
Conc: 9.10 ng/ml

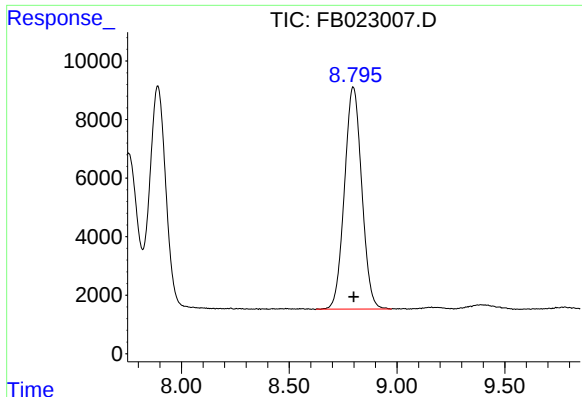


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 423752
Conc: 18.82 ng/ml

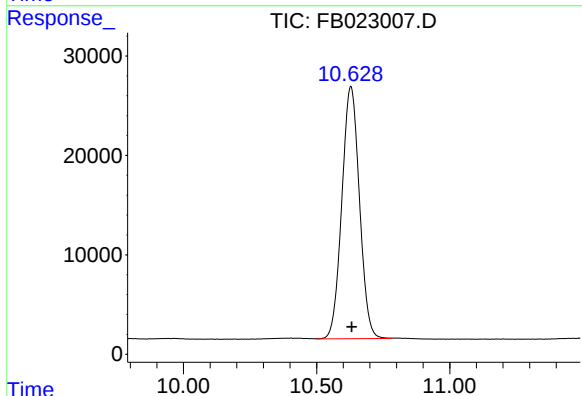


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 1165307
Conc: 27.03 ng/ml

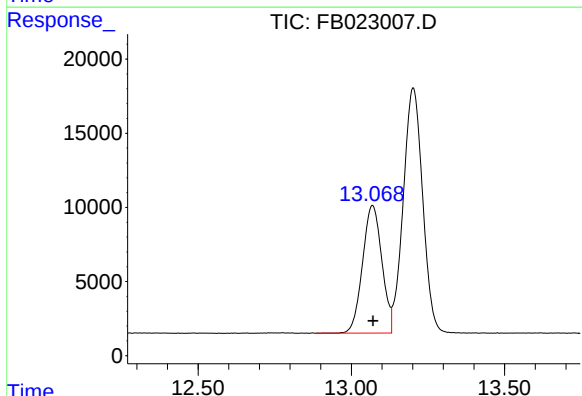


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 376493
Conc: 9.43 ng/ml

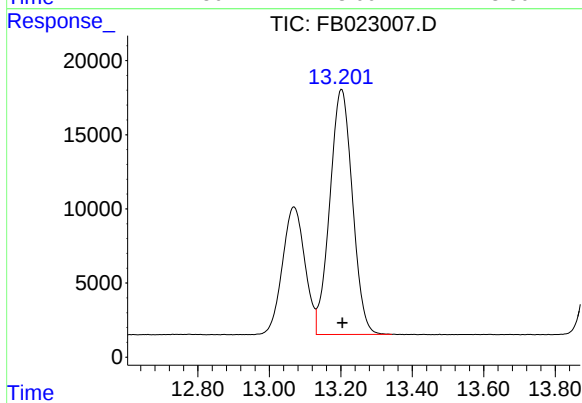


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 727051
Conc: 19.25 ng/ml

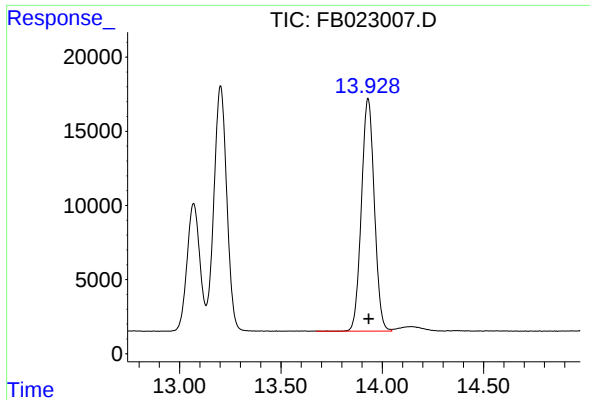

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 695420
Conc: 19.51 ng/ml

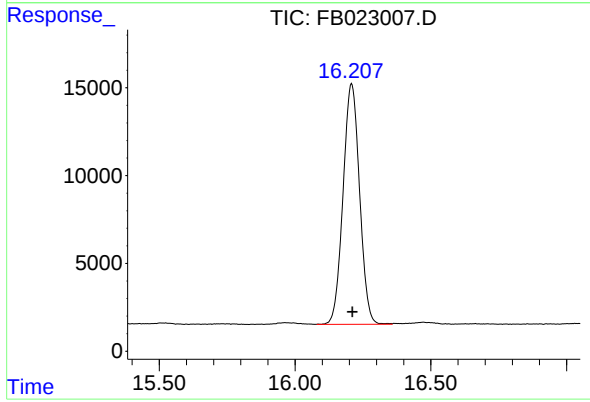

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 579073
Conc: 20.42 ng/ml