

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB111519\  
Data File : FB023012.D  
Signal(s) : FID2B.CH  
Acq On : 15 Nov 2019 16:19  
Operator : DD/AJ  
Sample : K5671-07  
Misc : 5.01g/5.00ml DI WATER  
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Nov 15 22:05:16 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB103119.M  
Quant Title :  
QLast Update : Thu Oct 31 14:57:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.797  | 434407   | 19.297 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.628 | 23956    | 0.556 ng/ml  |
| 7) t Ethylbenzene            | 13.076 | 5716     | 0.143 ng/ml  |
| 8) t m-Xylene                | 13.200 | 18012    | 0.477 ng/ml  |
| 9) t O-Xylene                | 13.933 | 8898     | 0.250 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.212 | 6171     | 0.218 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB111519\  
Data File : FB023012.D  
Signal(s) : FID2B.CH  
Acq On : 15 Nov 2019 16:19  
Operator : DD/AJ  
Sample : K5671-07  
Misc : 5.01g/5.00ml DI WATER  
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Nov 15 22:05:16 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB103119.M  
Quant Title :  
QLast Update : Thu Oct 31 14:57:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

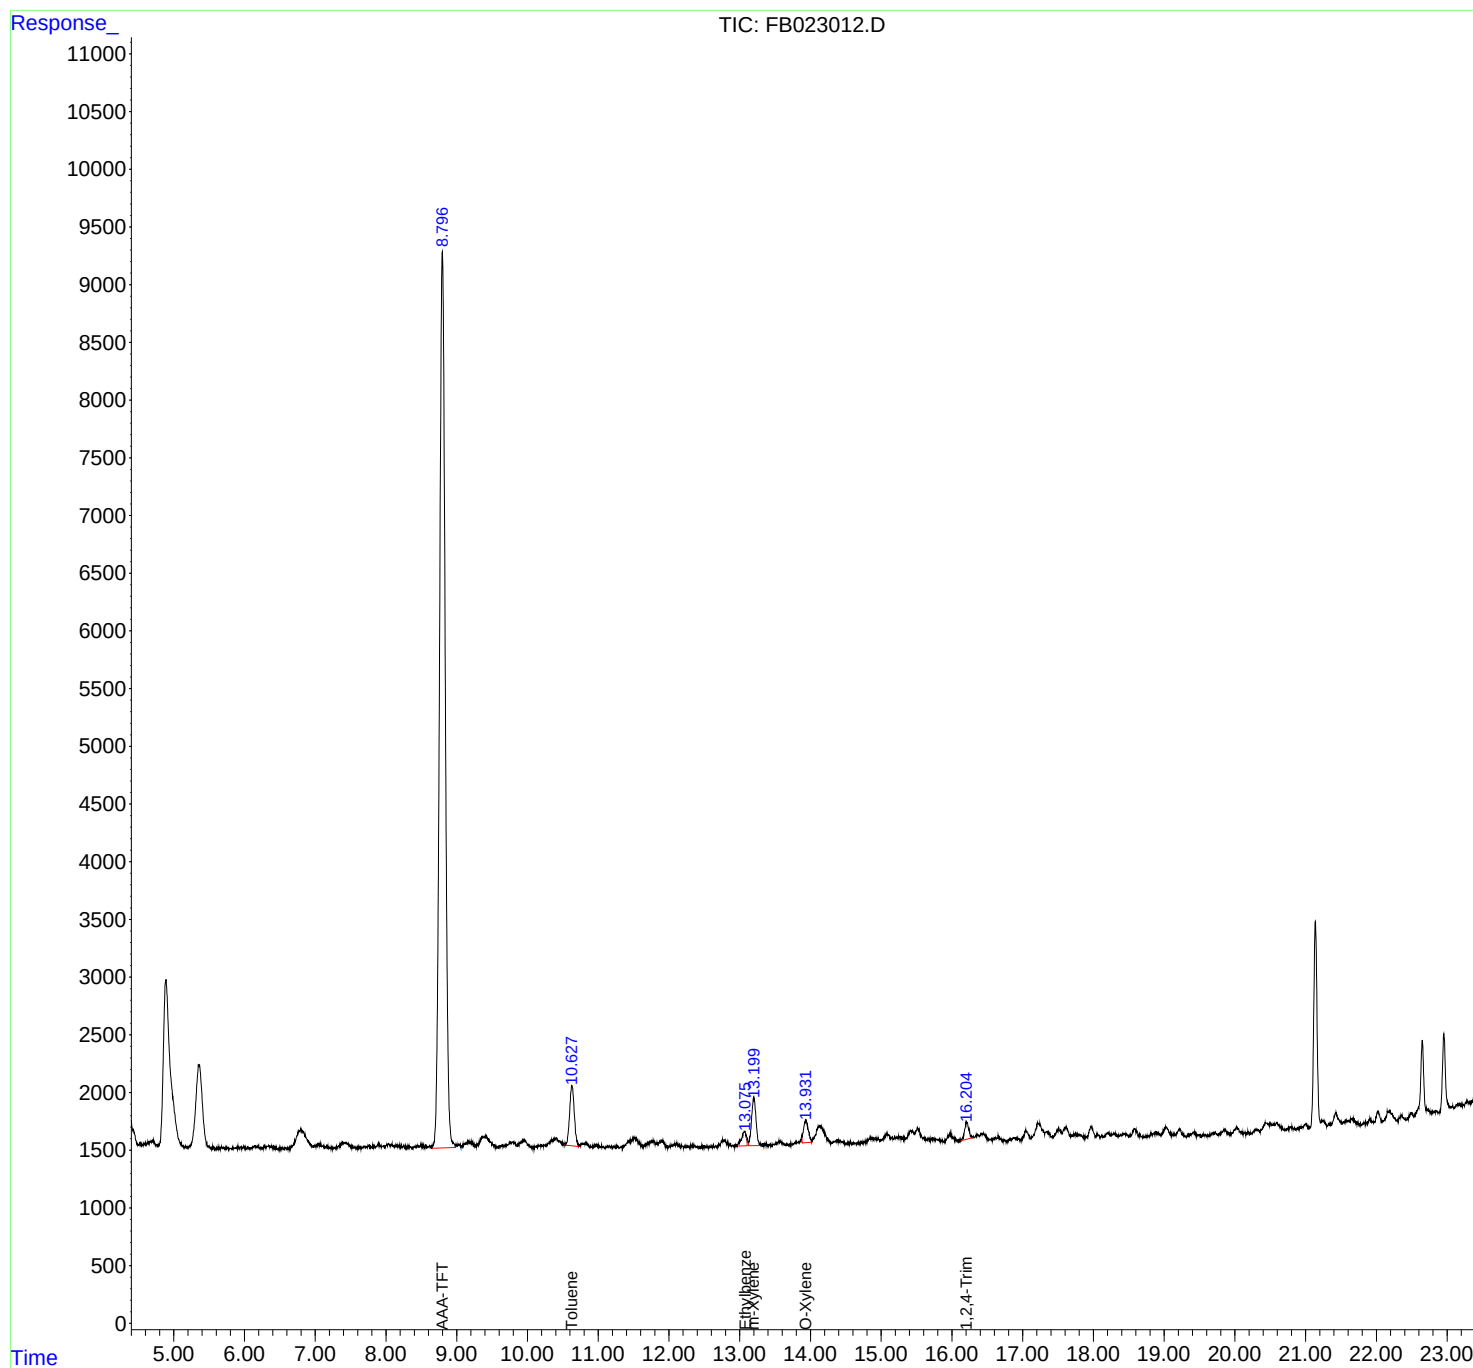

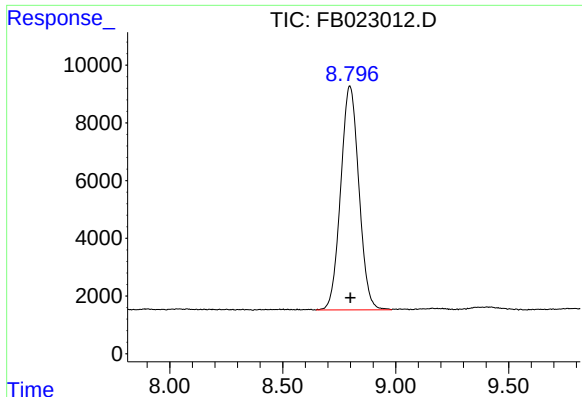


#5 AAA-TFT

R.T.: 8.797 min  
Delta R.T.: -0.003 min  
Response: 434407  
Conc: 19.30 ng/ml

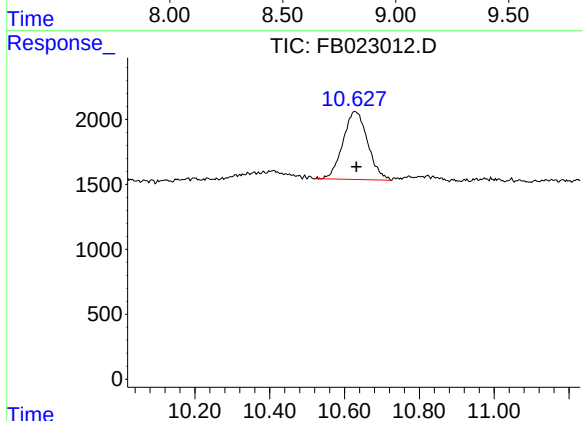


#6 Toluene

R.T.: 10.628 min  
Delta R.T.: -0.003 min  
Response: 23956  
Conc: 0.56 ng/ml

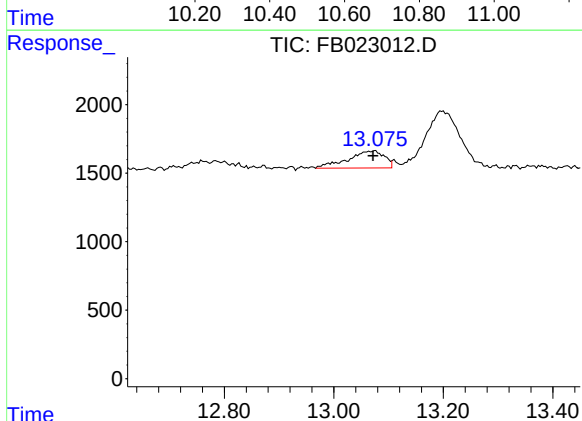


#7 Ethylbenzene

R.T.: 13.076 min  
Delta R.T.: 0.004 min  
Response: 5716  
Conc: 0.14 ng/ml

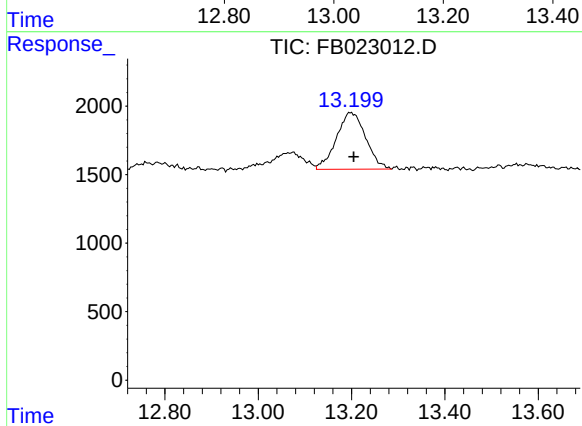


#8 m-Xylene

R.T.: 13.200 min  
Delta R.T.: -0.005 min  
Response: 18012  
Conc: 0.48 ng/ml

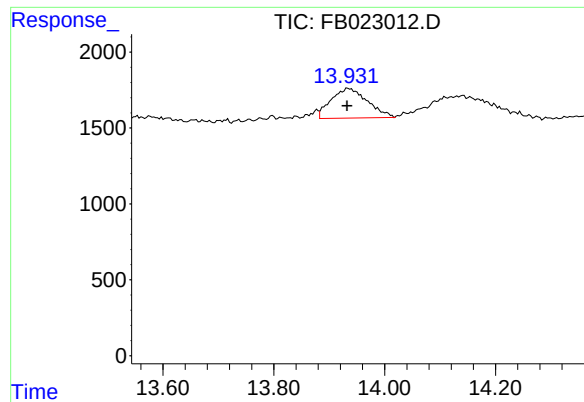

#9 O-Xylene

R.T.: 13.933 min  
Delta R.T.: 0.000 min  
Response: 8898  
Conc: 0.25 ng/ml

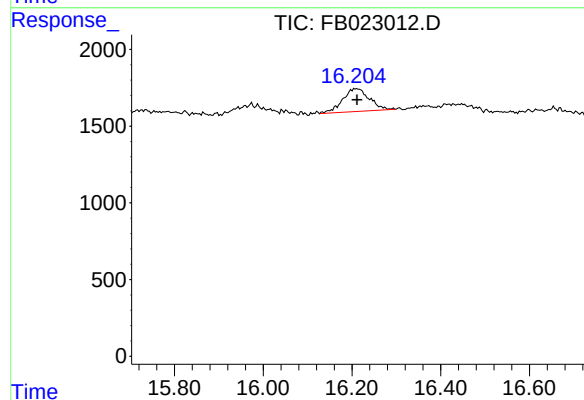

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min  
Delta R.T.: 0.000 min  
Response: 6171  
Conc: 0.22 ng/ml