

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111522\
 Data File : FB029044.D
 Signal(s) : FID2B.CH
 Acq On : 16 Nov 2022 3:55
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 16 05:30:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	303710	23.900 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	485727	29.800 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	537533	30.592 ng/ml
3) t n-Heptane	7.748	176833	10.057 ng/ml
4) t Benzene	7.884	231555	11.292 ng/ml
6) t Toluene	10.617	672552	33.438 ng/ml
7) t Ethylbenzene	13.054	206780	10.903 ng/ml
8) t m-Xylene	13.186	405394	21.549 ng/ml
9) t O-Xylene	13.913	393363	21.442 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	382094	20.741 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111522\
Data File : FB029044.D
Signal(s) : FID2B.CH
Acq On : 16 Nov 2022 3:55
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 16 05:30:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

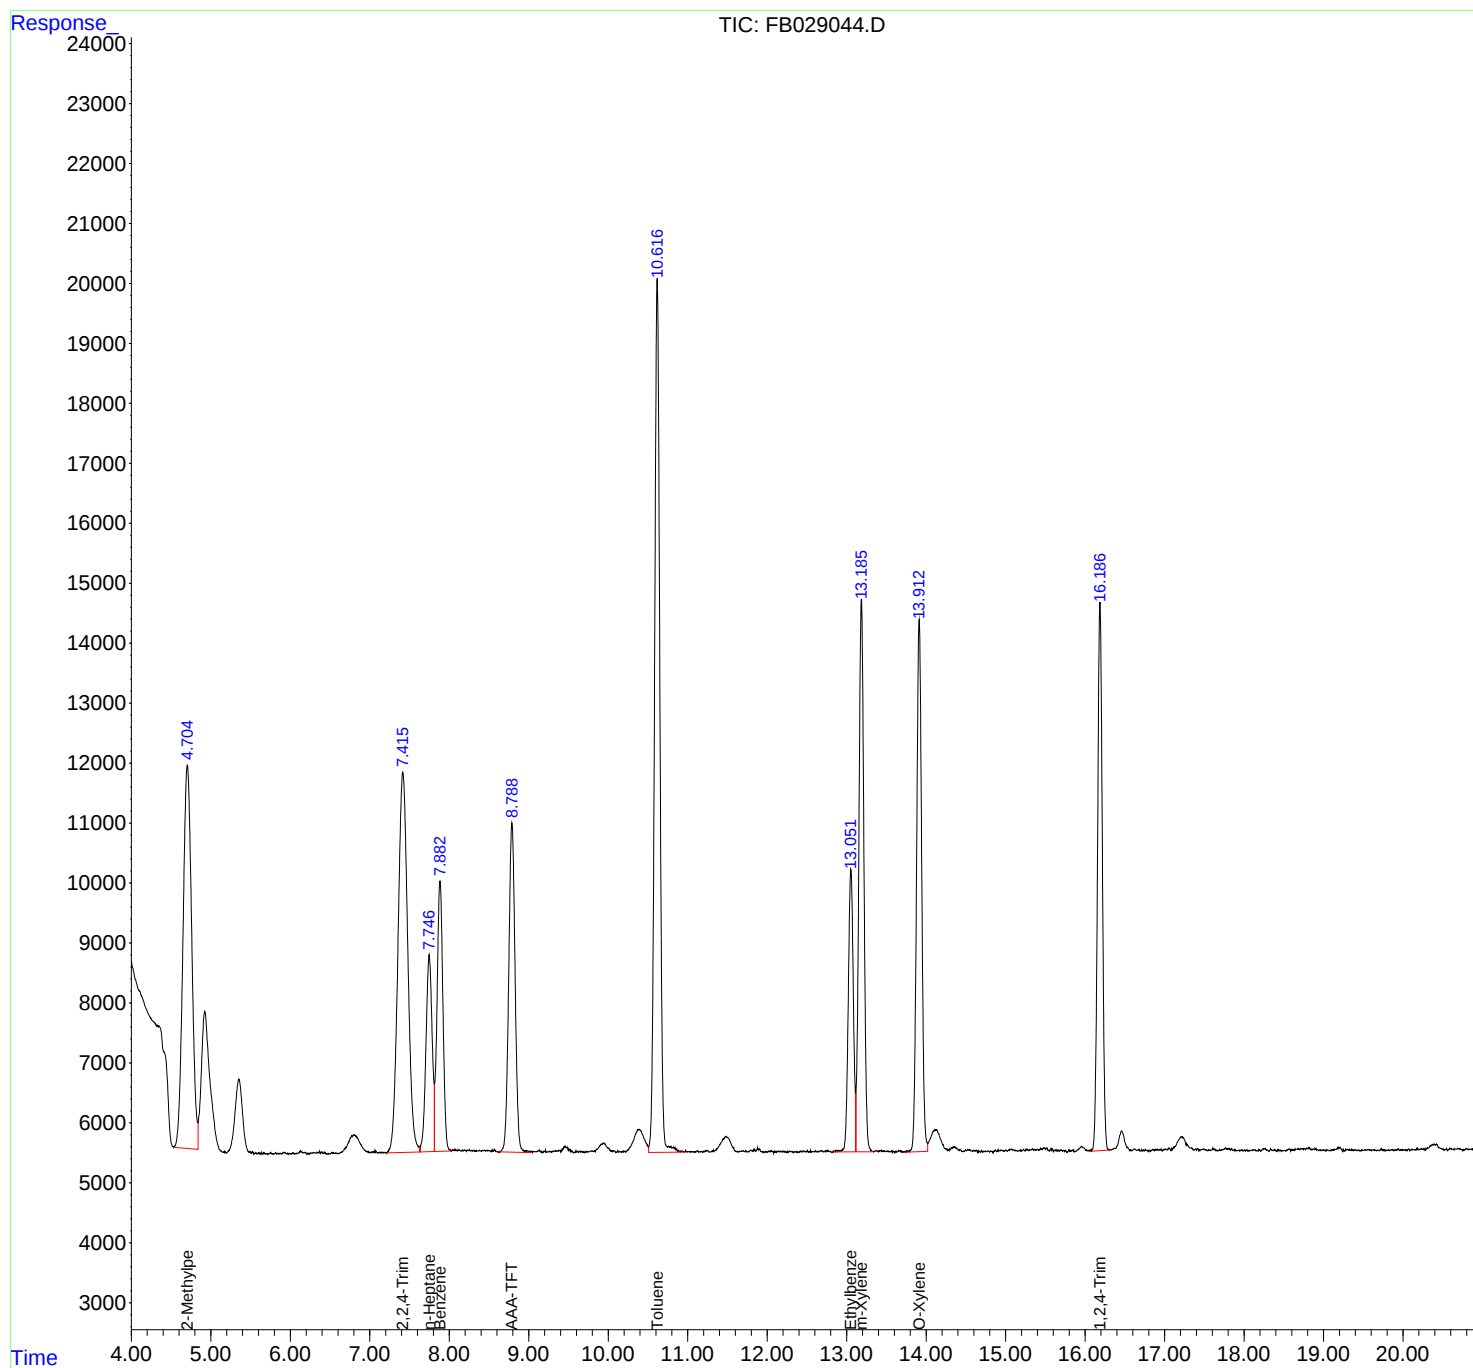


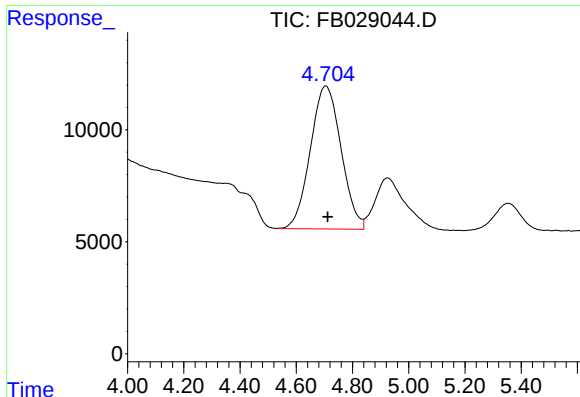

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.006 min
Response: 485727
Conc: 29.80 ng/ml

Instrument :
FID_B
ClientSampleId :

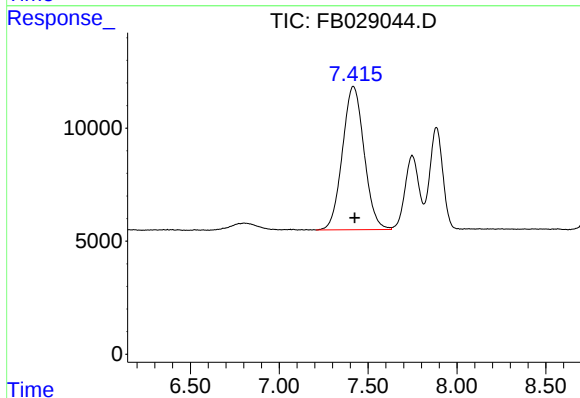


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.009 min
Response: 537533
Conc: 30.59 ng/ml

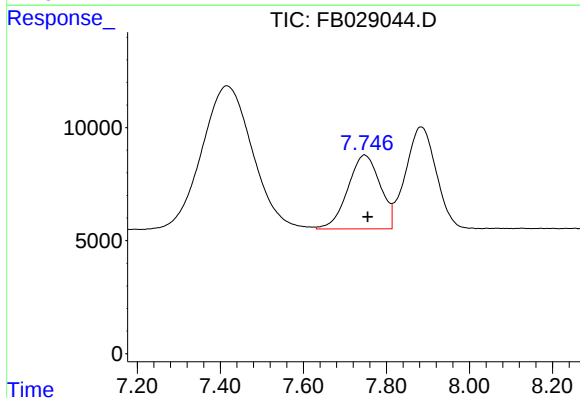


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.007 min
Response: 176833
Conc: 10.06 ng/ml

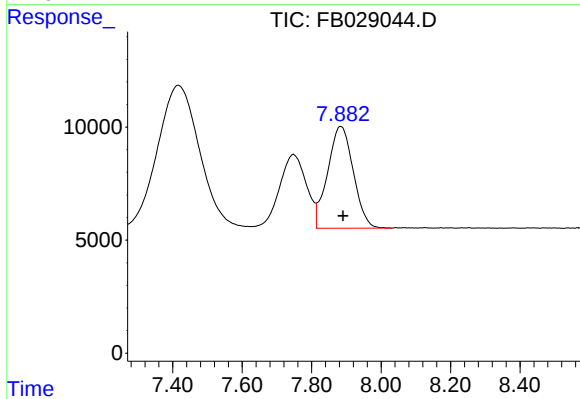

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.007 min
Response: 231555
Conc: 11.29 ng/ml

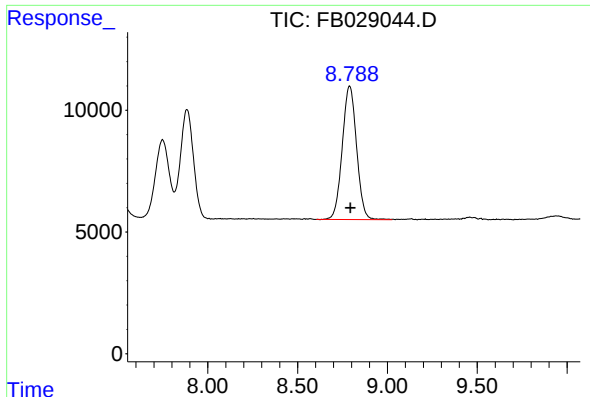

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.005 min
Response: 303710
Conc: 23.90 ng/ml

Instrument :
FID_B
ClientSampleId :

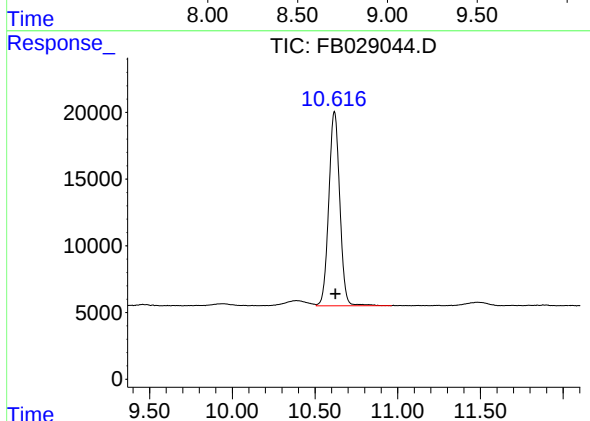


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.005 min
Response: 672552
Conc: 33.44 ng/ml

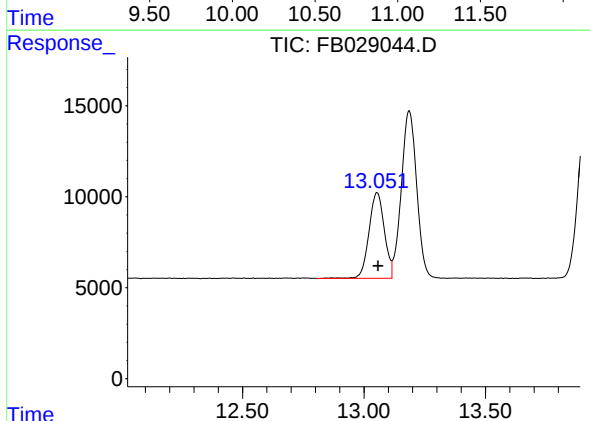


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 206780
Conc: 10.90 ng/ml

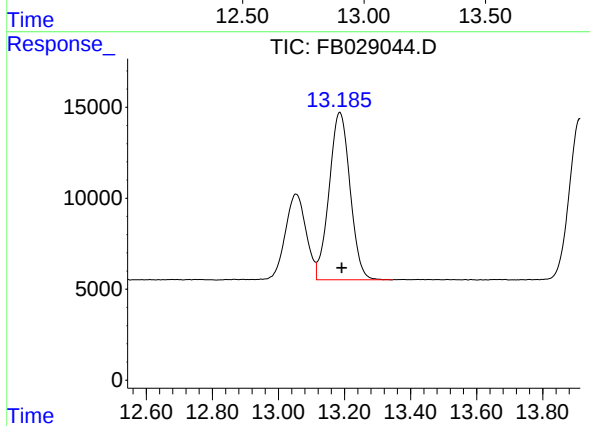

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 405394
Conc: 21.55 ng/ml

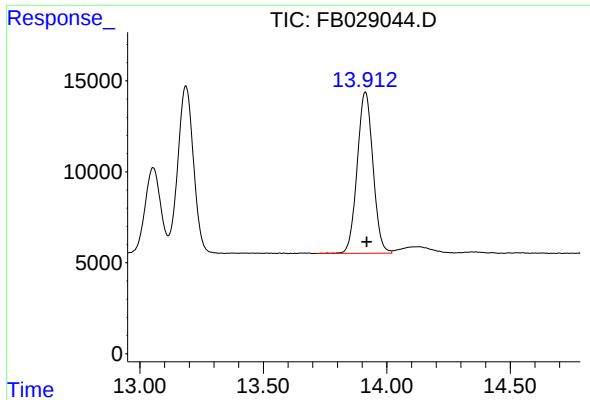

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 393363
Conc: 21.44 ng/ml

Instrument :
FID_B
ClientSampleId :

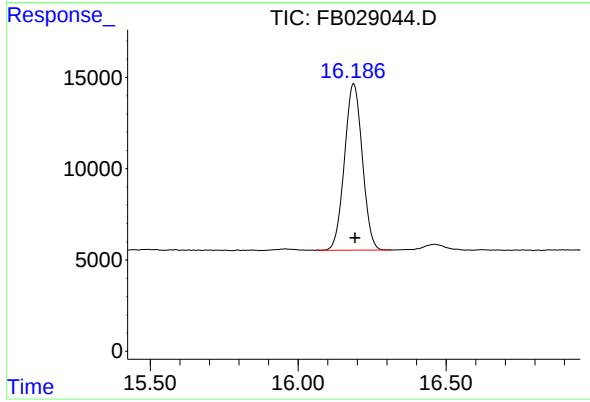

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.005 min
Response: 382094
Conc: 20.74 ng/ml