

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
 Data File : FB031201.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2024 7:51
 Operator : YP/AJ
 Sample : VBF1115S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 18 02:29:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	526091	19.059 ng/ml
Target Compounds			
6) t Toluene	10.618	6112	0.122 ng/ml
8) t m-Xylene	13.184	3223	0.066 ng/ml
9) t O-Xylene	13.920	7492	0.164 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	16000	0.430 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
Data File : FB031201.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2024 7:51
Operator : YP/AJ
Sample : VBF1115S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 18 02:29:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

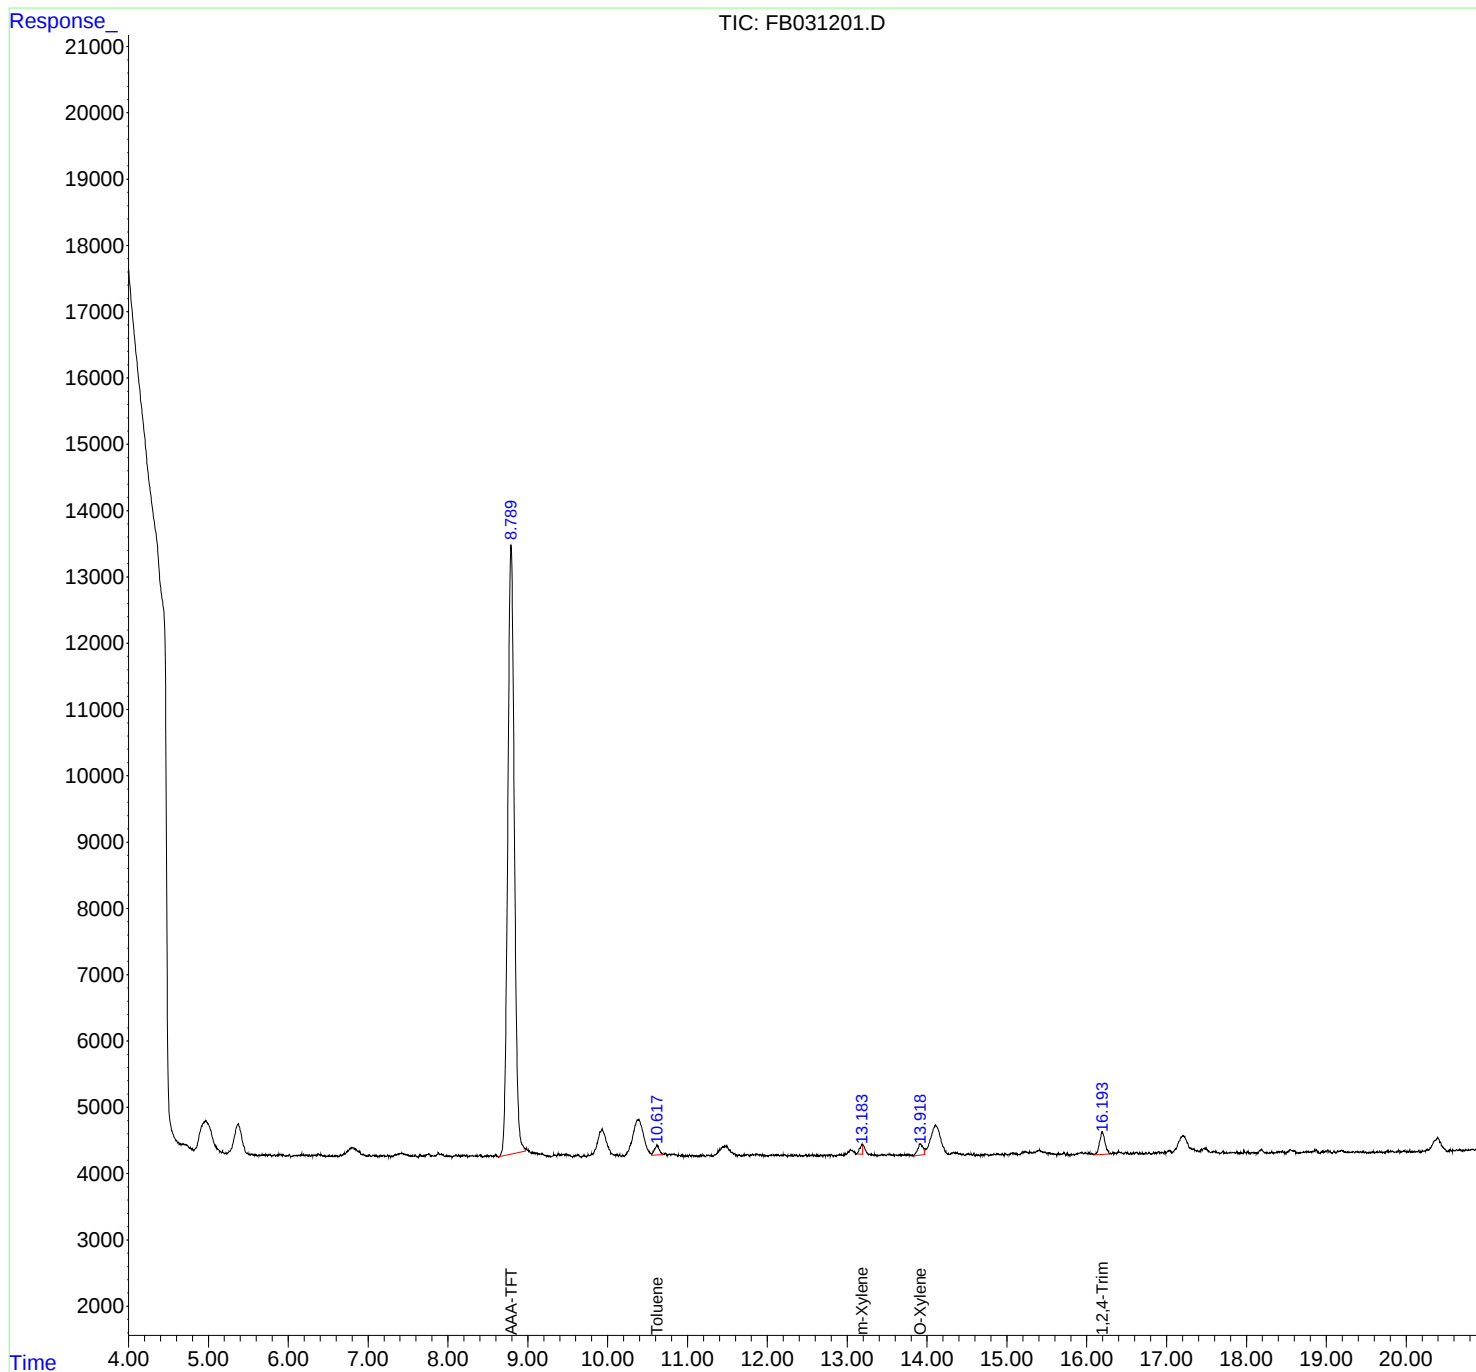


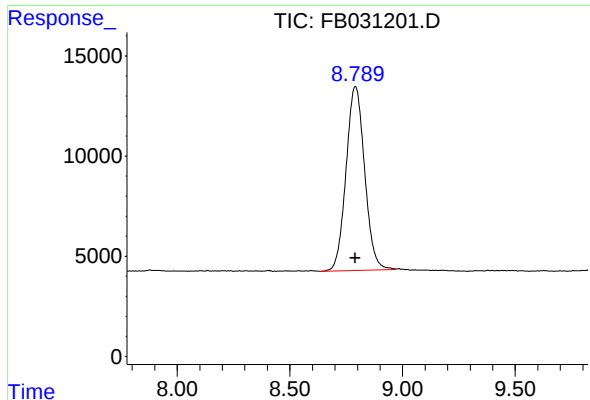

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 526091
Conc: 19.06 ng/ml

Instrument :
FID_B
ClientSampleId :

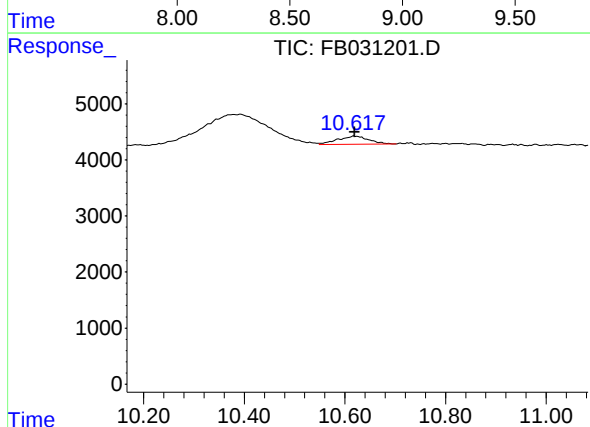


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 6112
Conc: 0.12 ng/ml

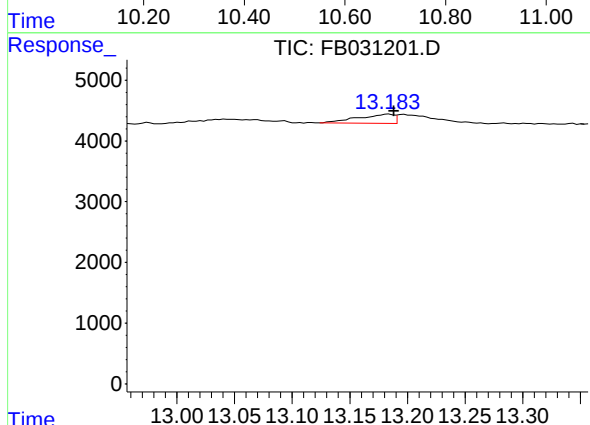


#8 m-Xylene

R.T.: 13.184 min
Delta R.T.: -0.004 min
Response: 3223
Conc: 0.07 ng/ml

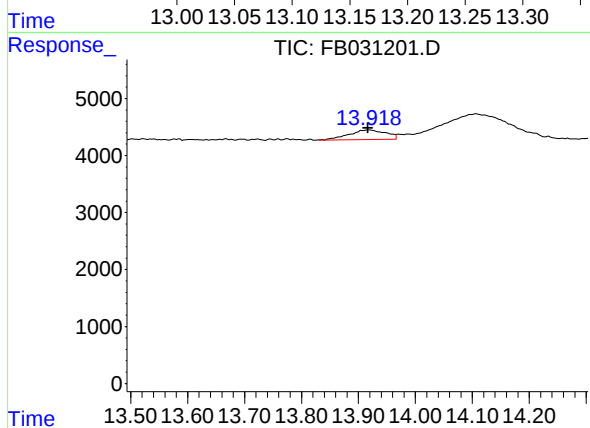

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.003 min
Response: 7492
Conc: 0.16 ng/ml

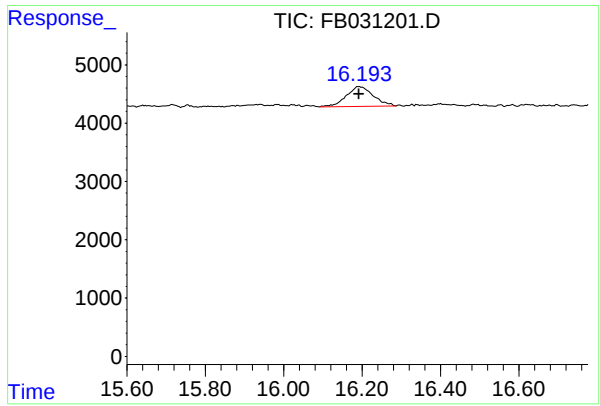

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min

Delta R.T.: -0.003 min

Response: 16000

Conc: 0.43 ng/ml

Instrument :

FID_B

ClientSampleId :