

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
 Data File : FB031215.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2024 15:34
 Operator : YP/AJ
 Sample : P4839-20
 Misc : 7.32G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 18 02:30:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	561812	20.353 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	89315	2.274 ng/ml
2) t 2,2,4-Trimethylpentane	7.403	119135	2.544 ng/ml
3) t n-Heptane	7.808	51535	1.137 ng/ml
6) t Toluene	10.641	4997	0.100 ng/ml
7) t Ethylbenzene	13.024	83825	1.873 ng/ml
9) t O-Xylene	13.926	14740	0.323 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	8637	0.232 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
Data File : FB031215.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2024 15:34
Operator : YP/AJ
Sample : P4839-20
Misc : 7.32G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 18 02:30:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

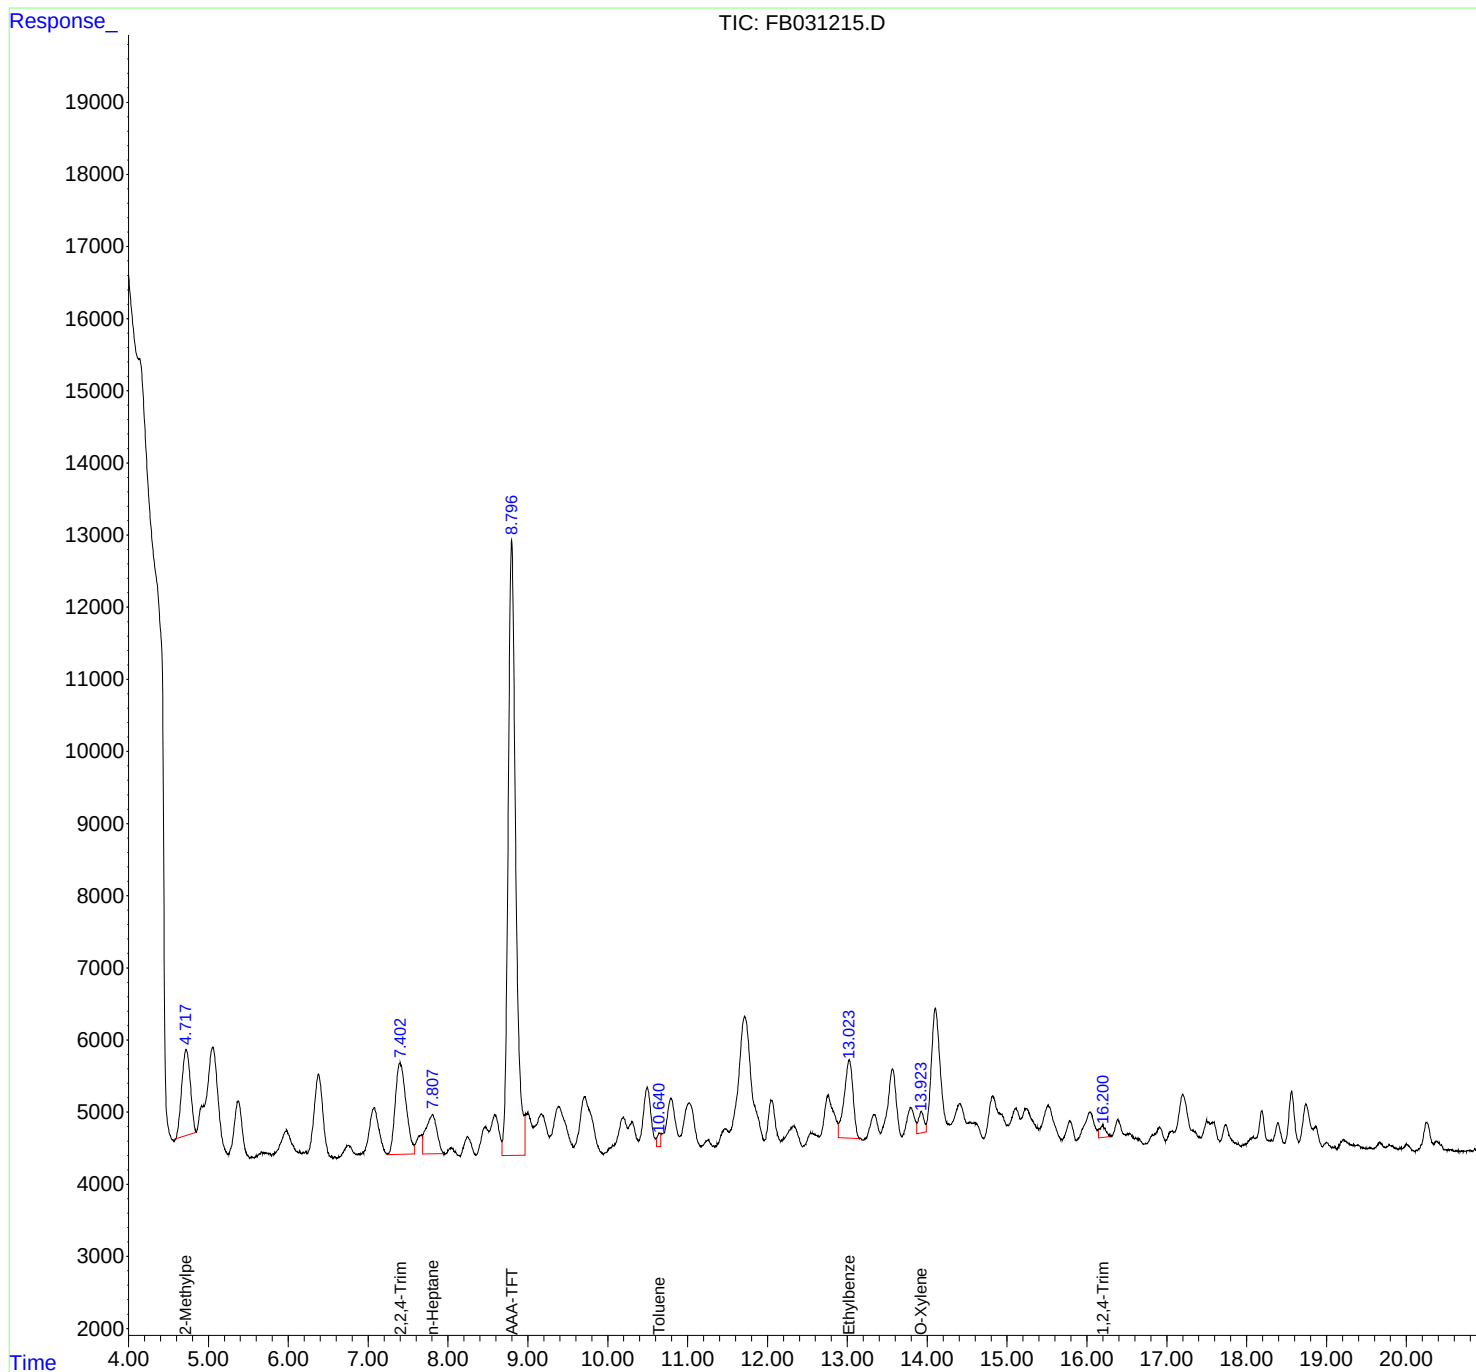


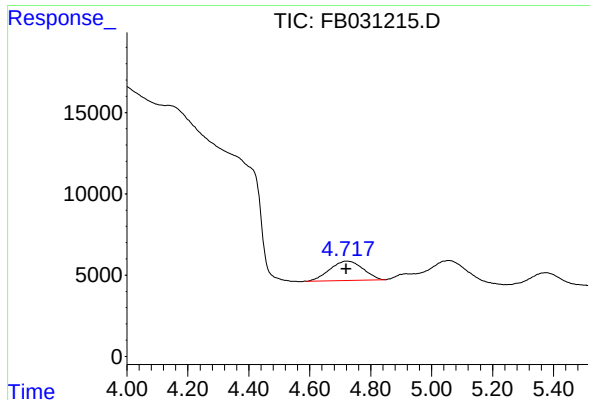

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: -0.001 min
Response: 89315
Conc: 2.27 ng/ml

Instrument :
FID_B
ClientSampleId :

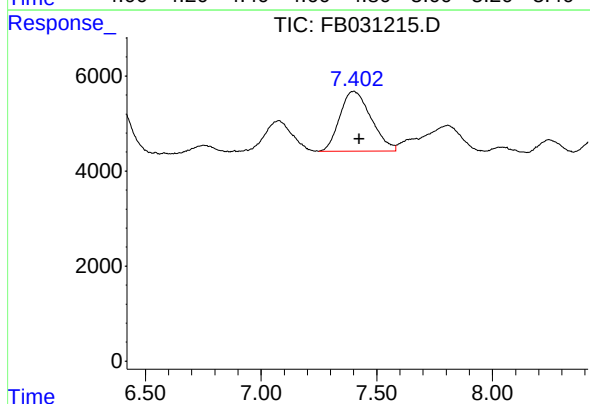


#2 2,2,4-Trimethylpentane

R.T.: 7.403 min
Delta R.T.: -0.022 min
Response: 119135
Conc: 2.54 ng/ml

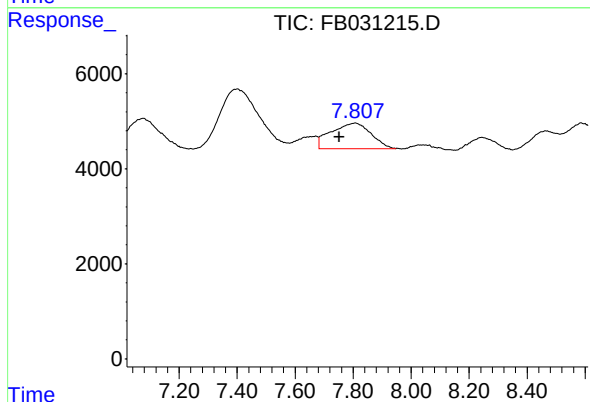


#3 n-Heptane

R.T.: 7.808 min
Delta R.T.: 0.055 min
Response: 51535
Conc: 1.14 ng/ml

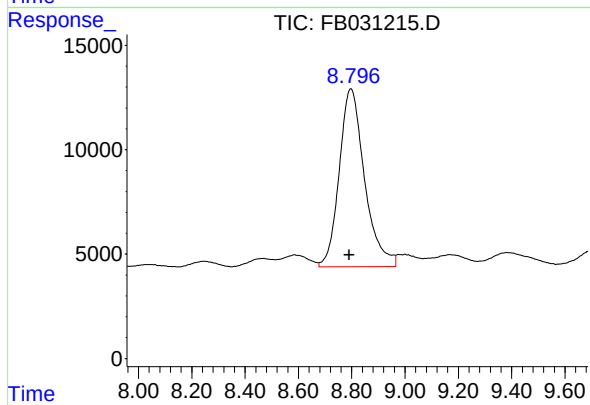

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.007 min
Response: 561812
Conc: 20.35 ng/ml

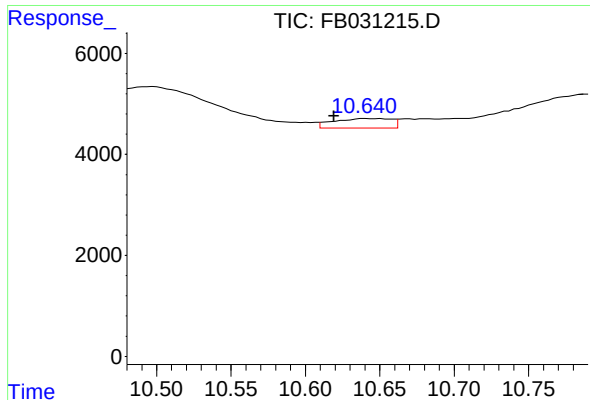

#6 Toluene


R.T.: 10.641 min
Delta R.T.: 0.022 min
Response: 4997
Conc: 0.10 ng/ml

Instrument :
FID_B
ClientSampleId :

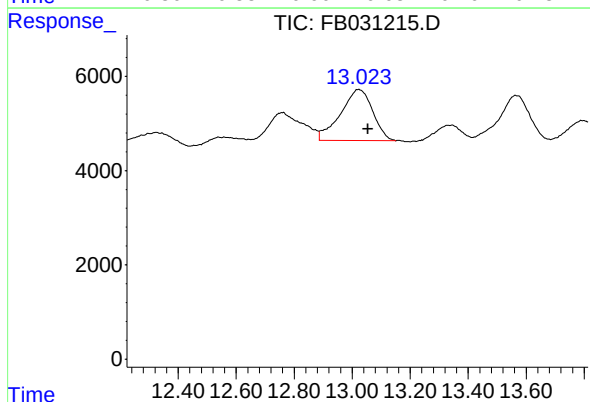


#7 Ethylbenzene

R.T.: 13.024 min
Delta R.T.: -0.031 min
Response: 83825
Conc: 1.87 ng/ml

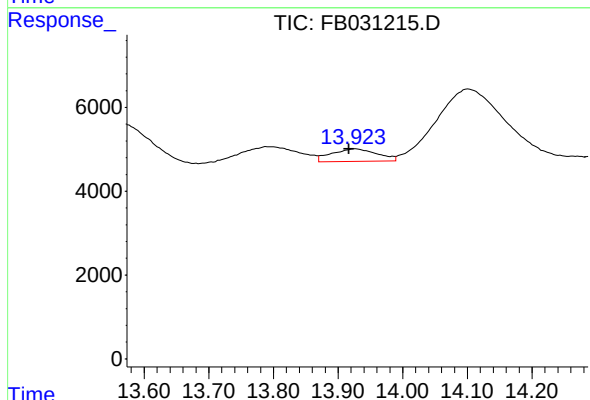

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.010 min
Response: 14740
Conc: 0.32 ng/ml

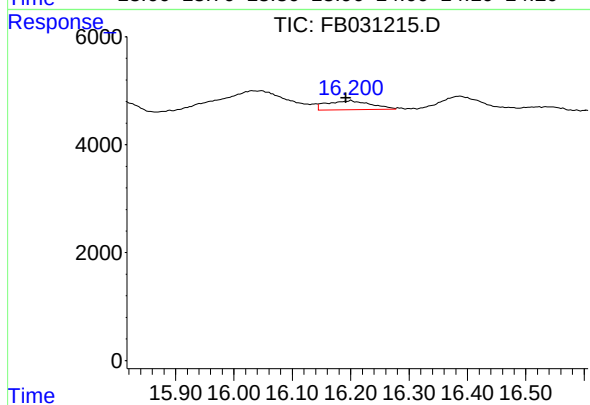

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.009 min
Response: 8637
Conc: 0.23 ng/ml