

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
 Data File : FB031217.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2024 16:28
 Operator : YP/AJ
 Sample : P4839-07 250X
 Misc : 7.53G/5.00 ML MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 18 02:30:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	723246	26.202 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	300625	7.654 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	849428	18.136 ng/ml
3) t n-Heptane	7.739	202289	4.464 ng/ml
7) t Ethylbenzene	13.019	115241	2.574 ng/ml
8) t m-Xylene	13.119	77040	1.584 ng/ml
9) t O-Xylene	13.917	15312	0.336 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
Data File : FB031217.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2024 16:28
Operator : YP/AJ
Sample : P4839-07 250X
Misc : 7.53G/5.00 ML MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 18 02:30:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

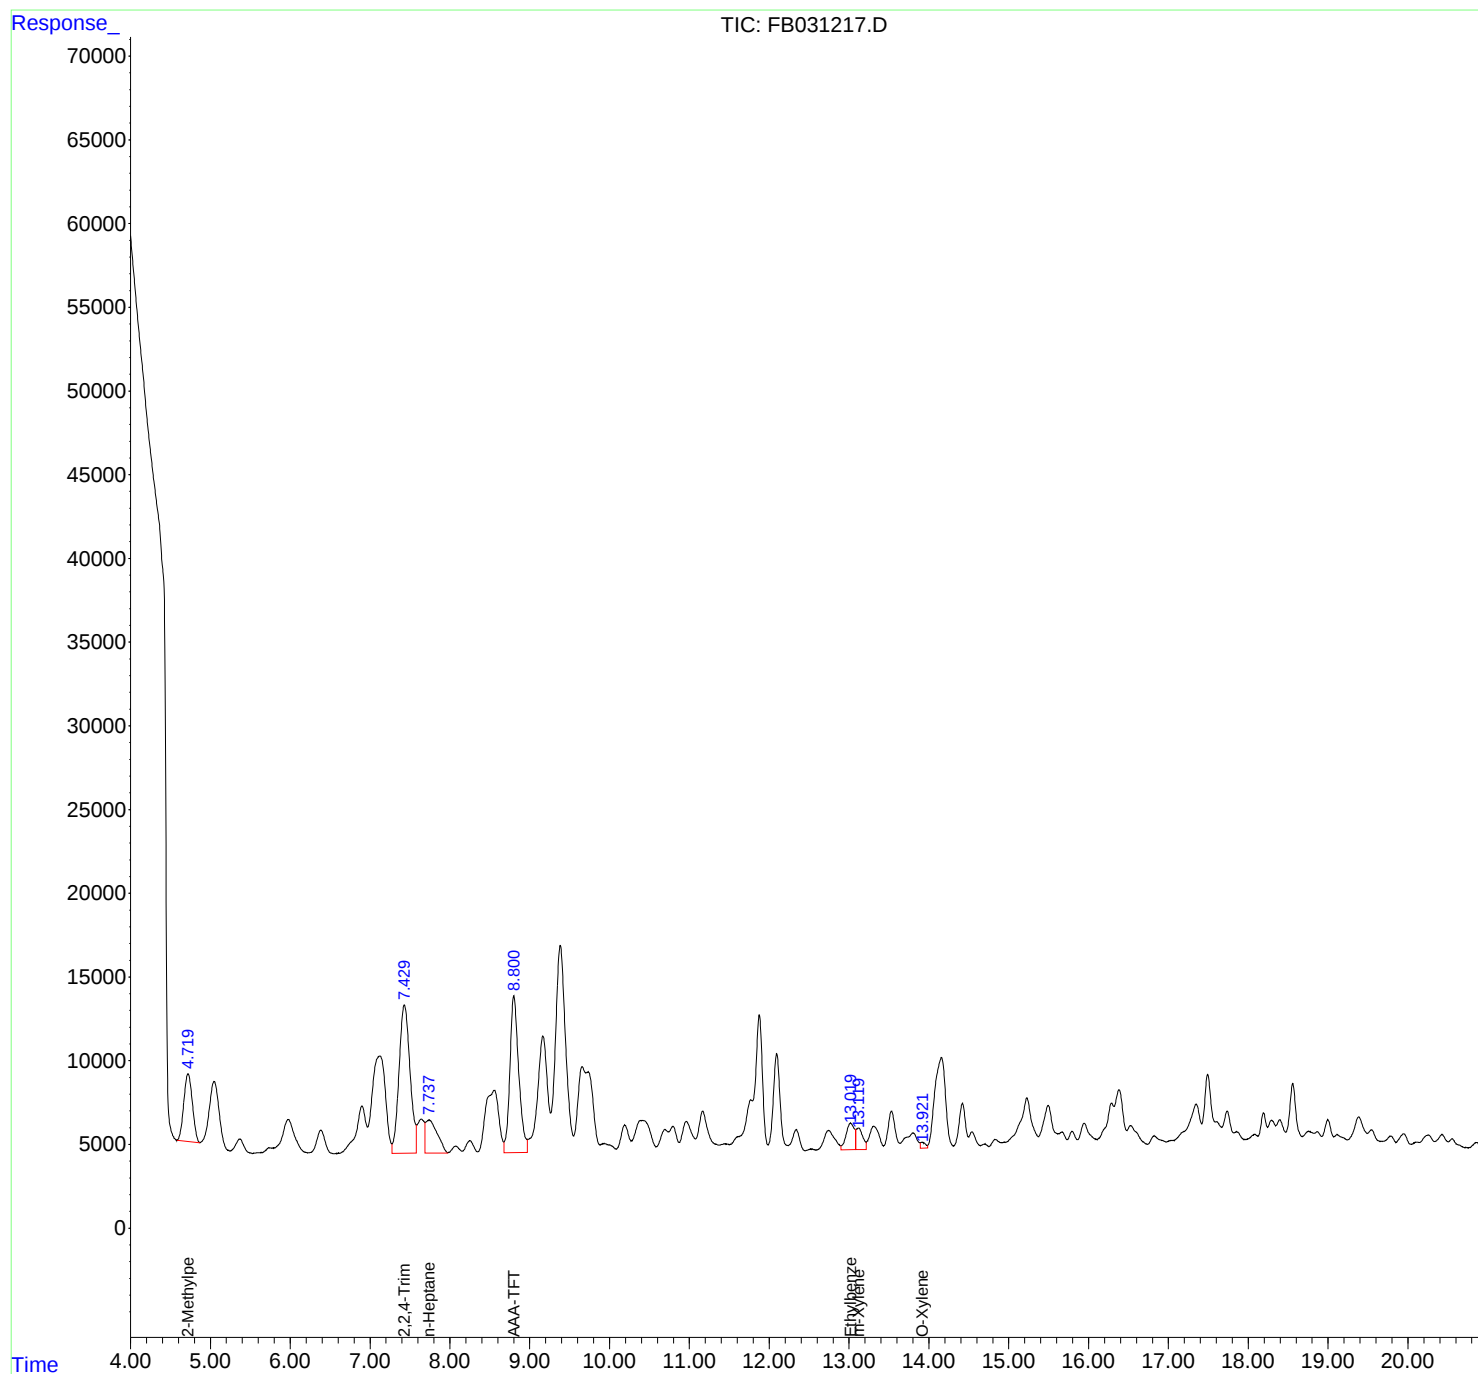


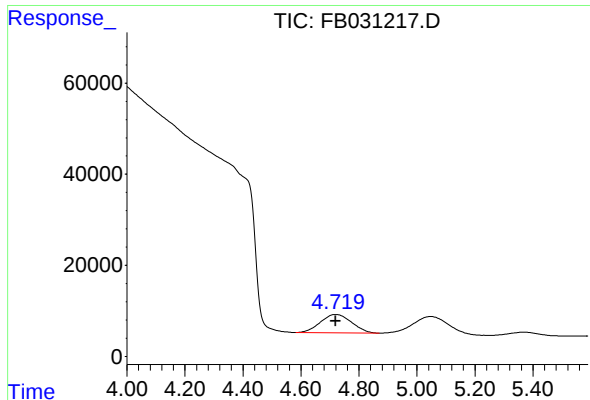

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 300625
Conc: 7.65 ng/ml

Instrument :
FID_B
ClientSampleId :

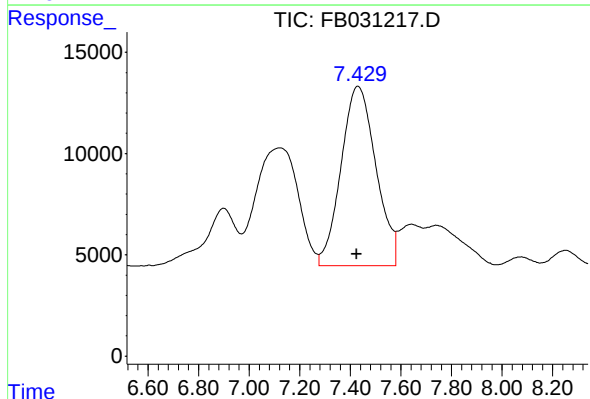


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.005 min
Response: 849428
Conc: 18.14 ng/ml

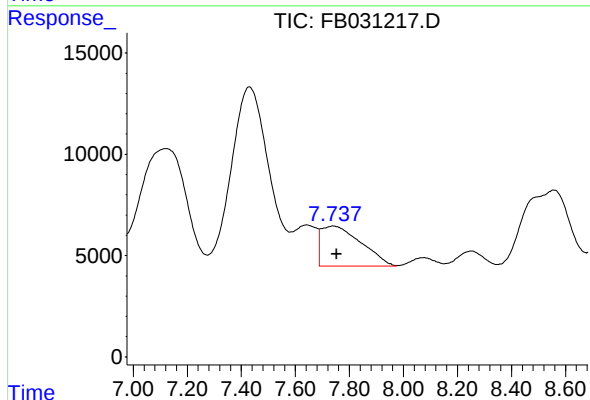


#3 n-Heptane

R.T.: 7.739 min
Delta R.T.: -0.014 min
Response: 202289
Conc: 4.46 ng/ml

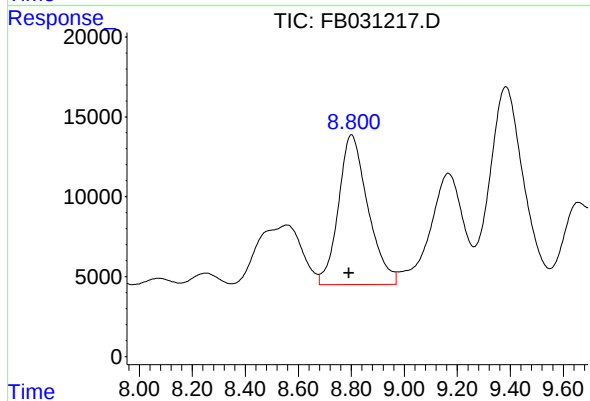

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.010 min
Response: 723246
Conc: 26.20 ng/ml

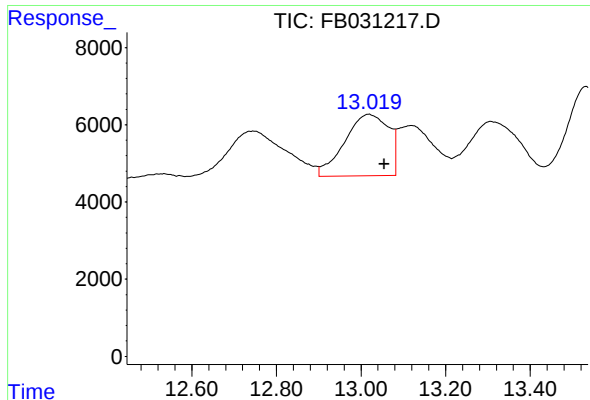

#7 Ethylbenzene


R.T.: 13.019 min
Delta R.T.: -0.036 min
Response: 115241
Conc: 2.57 ng/ml

Instrument :
FID_B
ClientSampleId :

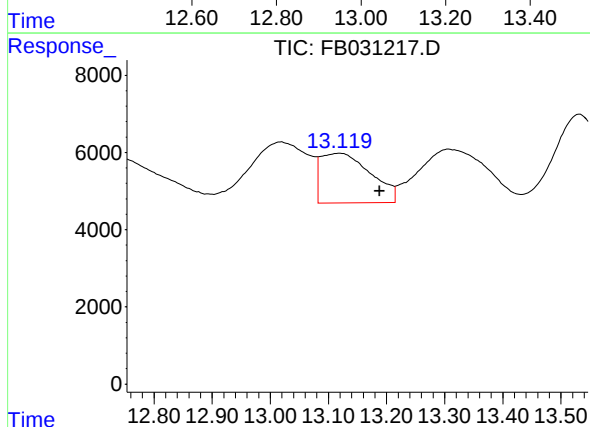

#8 m-Xylene

R.T.: 13.119 min
Delta R.T.: -0.069 min
Response: 77040
Conc: 1.58 ng/ml

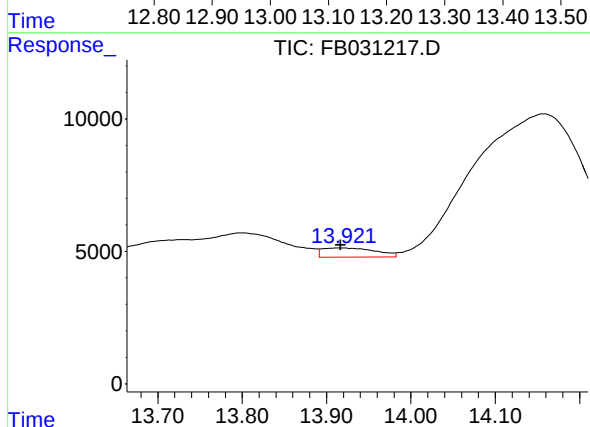

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 15312
Conc: 0.34 ng/ml