

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
 Data File : FB031225.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2024 21:23
 Operator : YP/AJ
 Sample : P4839-15 250X
 Misc : 7.59G/5.00 ML MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 18 02:31:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	857287	31.058 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	13982	0.356 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	1851511	39.532 ng/ml
3) t n-Heptane	7.730	90119	1.989 ng/ml
4) t Benzene	7.872	39858	0.746 ng/ml
7) t Ethylbenzene	13.016	566408	12.654 ng/ml
9) t O-Xylene	13.925	51519	1.130 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
Data File : FB031225.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2024 21:23
Operator : YP/AJ
Sample : P4839-15 250X
Misc : 7.59G/5.00 ML MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 18 02:31:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

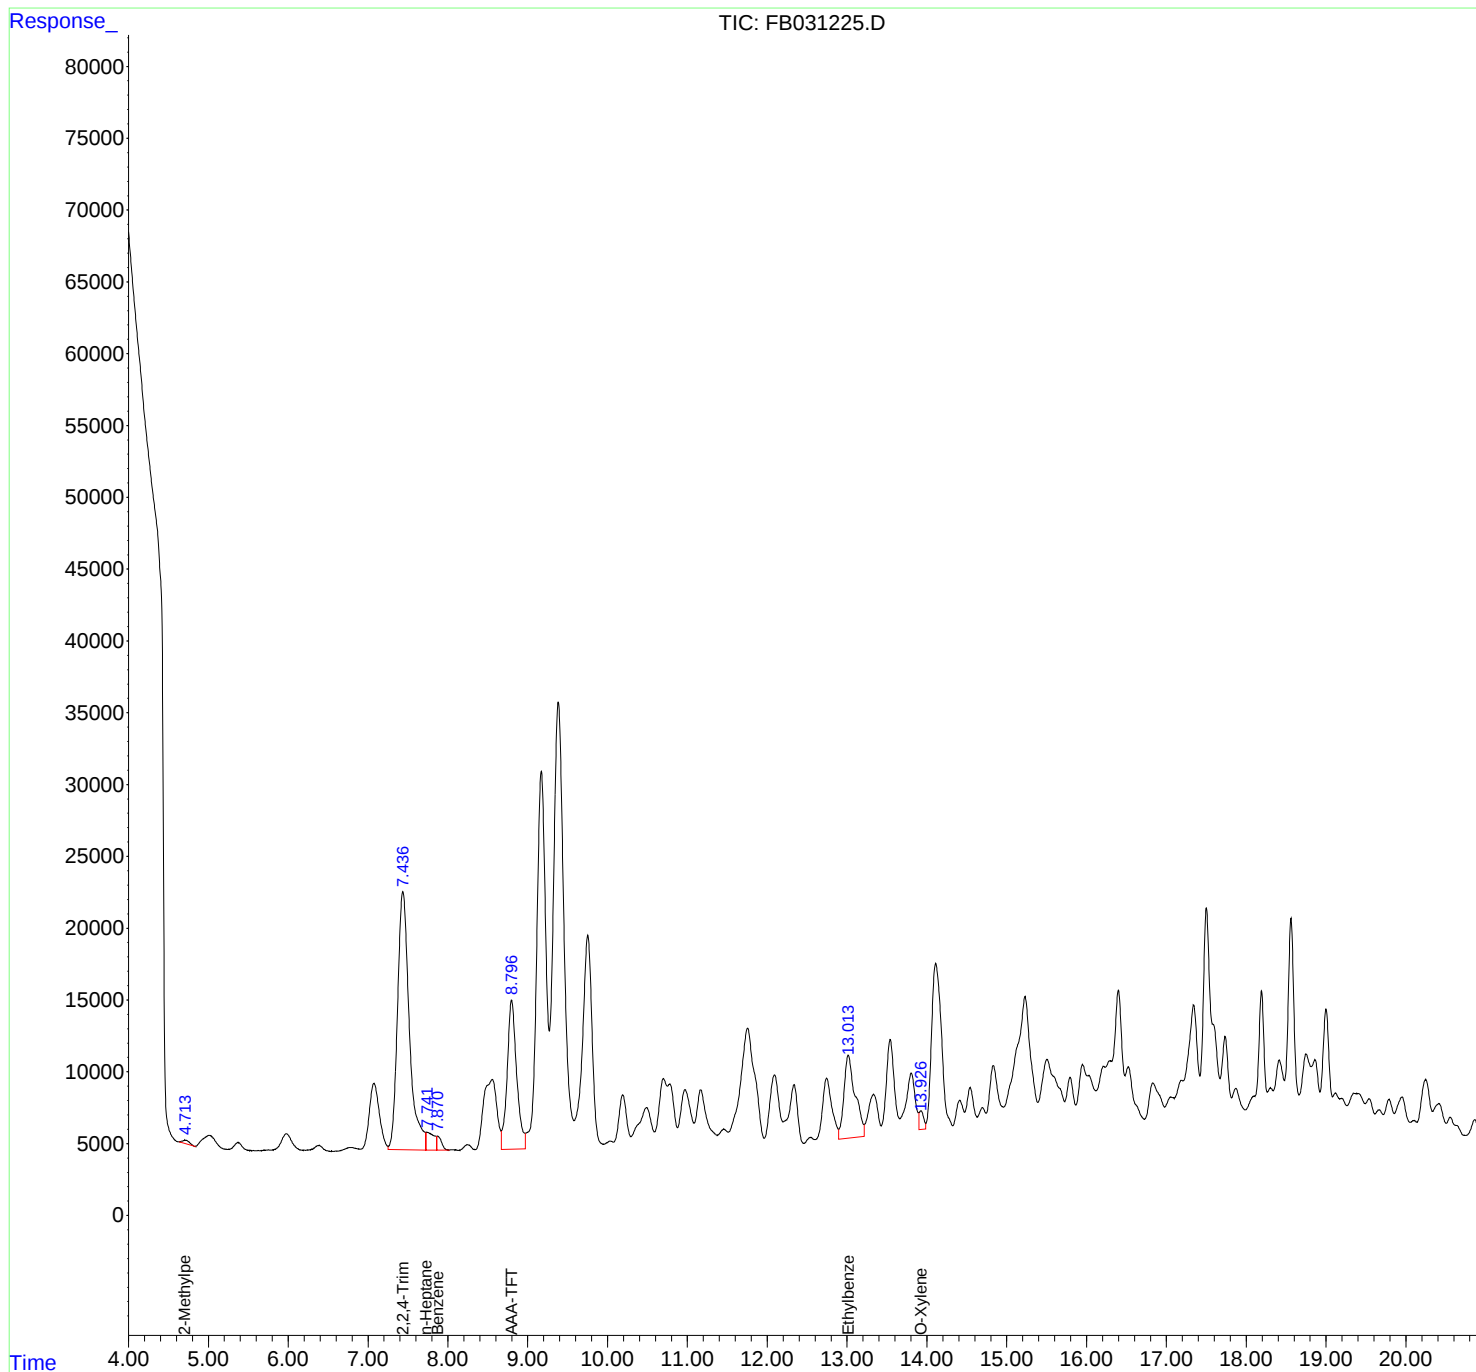

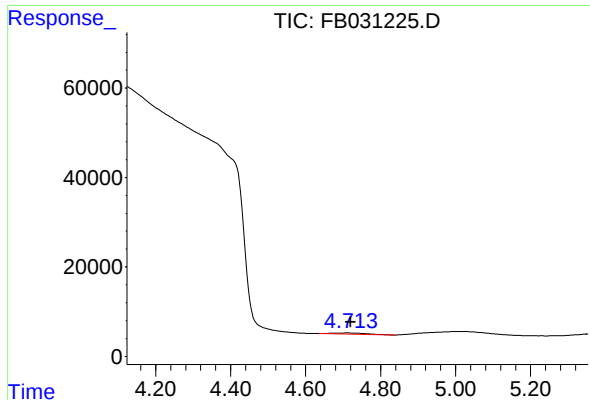


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.014 min
Response: 13982
Conc: 0.36 ng/ml

Instrument :


FID_B

ClientSampleId :

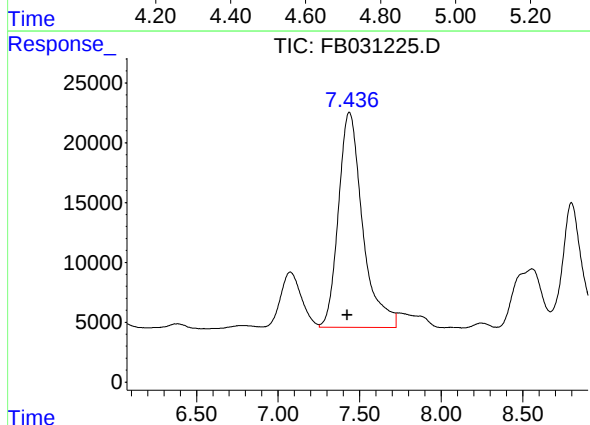


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.012 min
Response: 1851511
Conc: 39.53 ng/ml

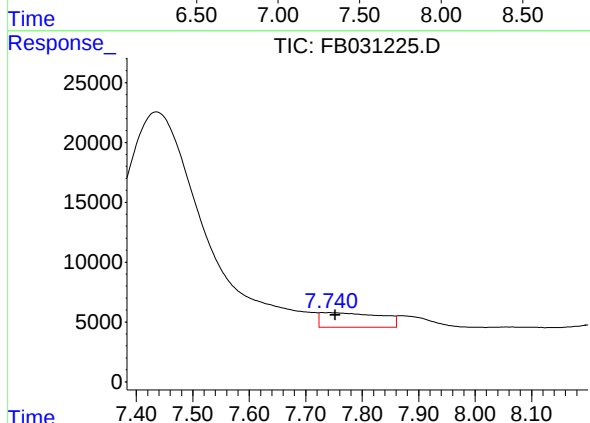


#3 n-Heptane

R.T.: 7.730 min
Delta R.T.: -0.023 min
Response: 90119
Conc: 1.99 ng/ml

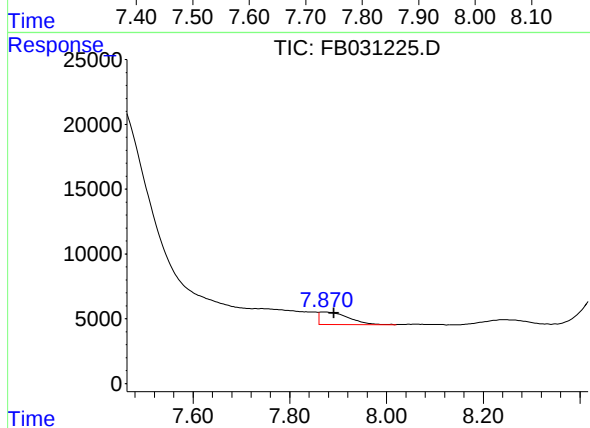

#4 Benzene


R.T.: 7.872 min
Delta R.T.: -0.020 min
Response: 39858
Conc: 0.75 ng/ml

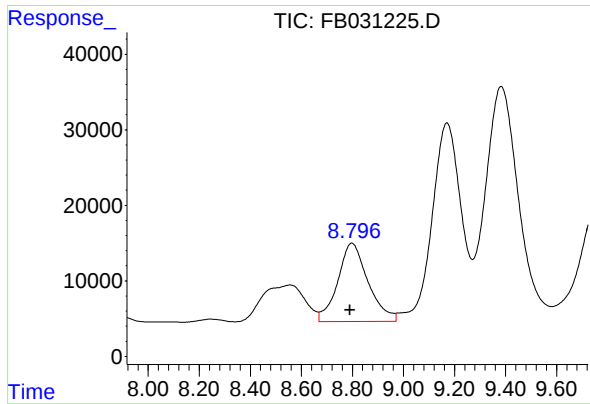

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.007 min
Response: 857287
Conc: 31.06 ng/ml

Instrument :
FID_B
ClientSampleId :

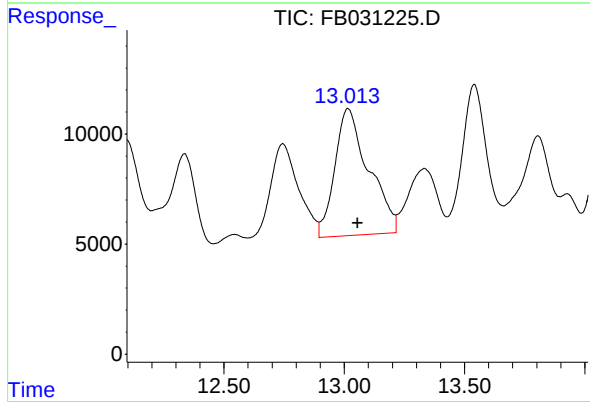

#7 Ethylbenzene

R.T.: 13.016 min
Delta R.T.: -0.039 min
Response: 566408
Conc: 12.65 ng/ml

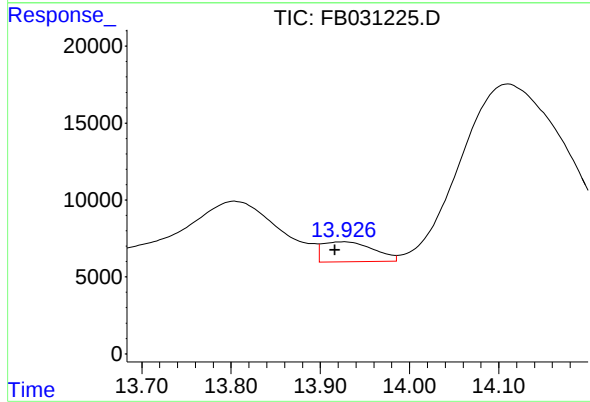

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.008 min
Response: 51519
Conc: 1.13 ng/ml