

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111524\
 Data File : FG014792.D
 Signal(s) : FID1A.ch
 Acq On : 15 Nov 2024 10:56
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 18 01:08:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111324.M
 Quant Title :
 QLast Update : Wed Nov 13 13:49:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.741	3048276	23.470 ug/ml
12) N-OCTACOSANE	17.220	2625107	22.328 ug/ml
13) N-TRIACONTANE	18.105	46460	0.403 ug/ml
14) N-DOTRIACONTANE	18.940	65988	0.600 ug/ml
15) N-TETRATRIACONTANE	19.722	63408	0.686 ug/ml
16) N-HEXATRIACONTANE	20.465	49521	0.699 ug/ml
17) N-OCTATRIACONTANE	21.213	79186	1.358 ug/ml
18) N-TETRACONTANE	22.150	140491	2.761 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111524\
Data File : FG014792.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2024 10:56
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 18 01:08:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111324.M
Quant Title :
QLast Update : Wed Nov 13 13:49:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

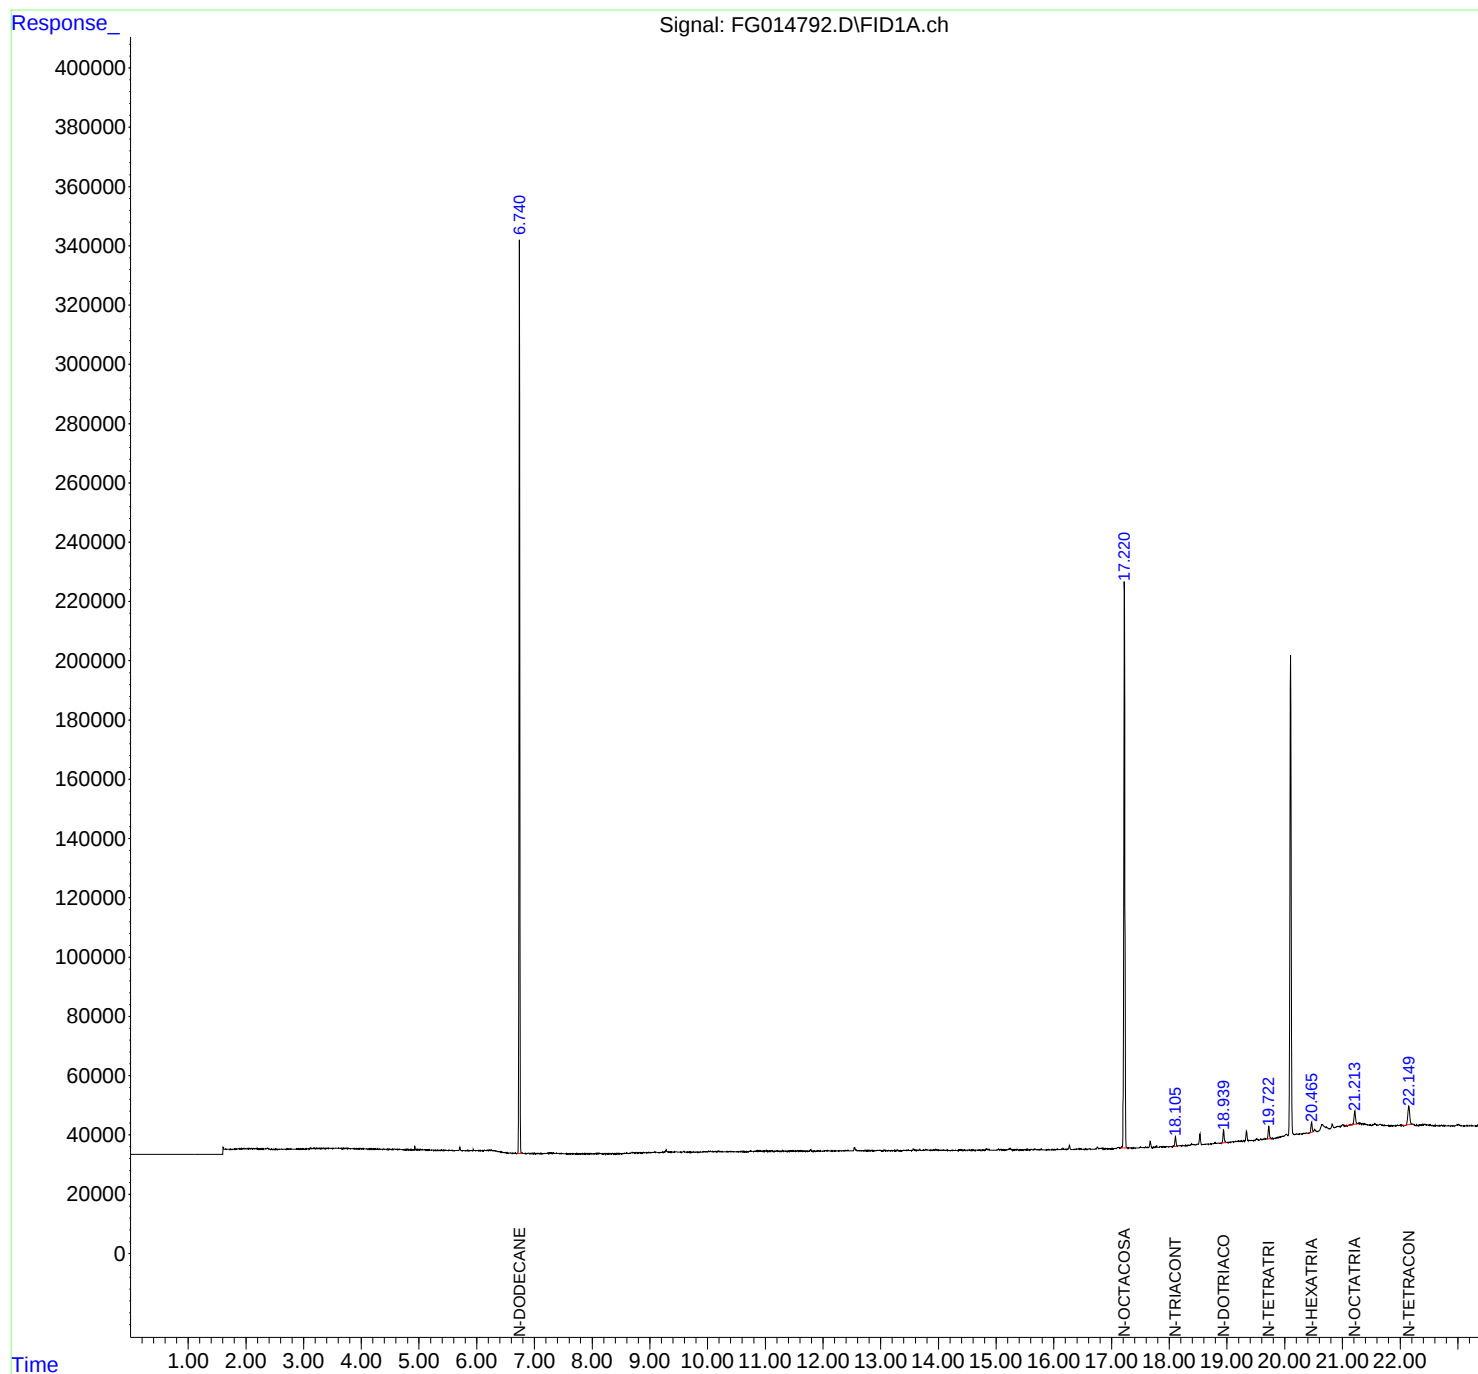


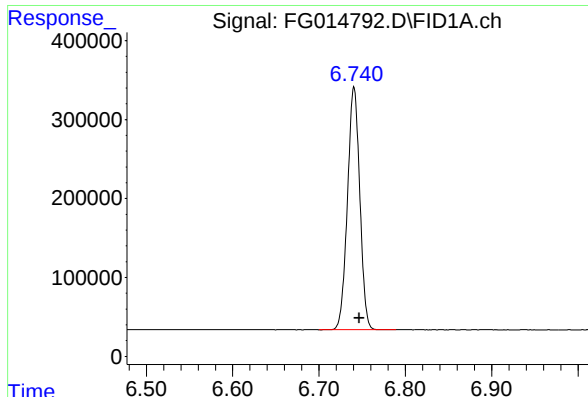

#3 N-DODECANE


R.T.: 6.741 min
Delta R.T.: -0.006 min
Response: 3048276
Conc: 23.47 ug/ml

Instrument :
FID_B
ClientSampleId :

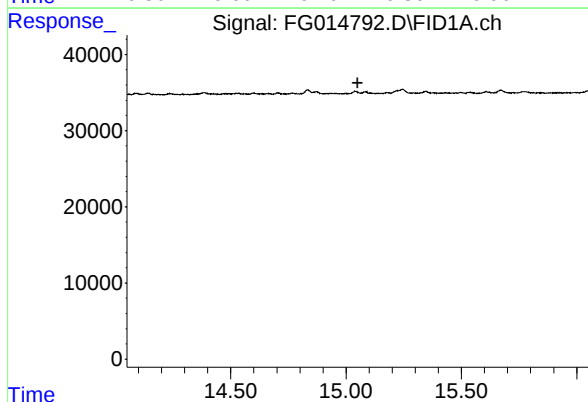


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.050 min
Response: 0
Conc: N.D.

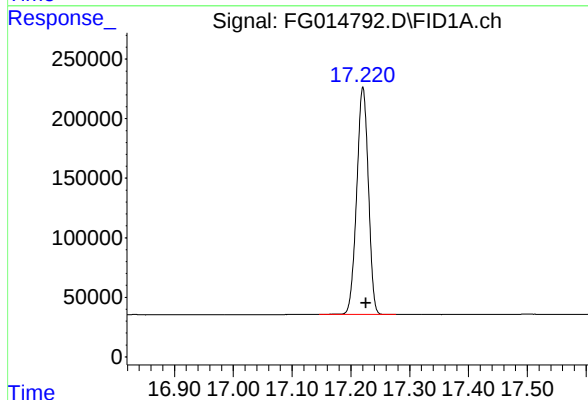


#12 N-OCTACOSANE

R.T.: 17.220 min
Delta R.T.: -0.006 min
Response: 2625107
Conc: 22.33 ug/ml

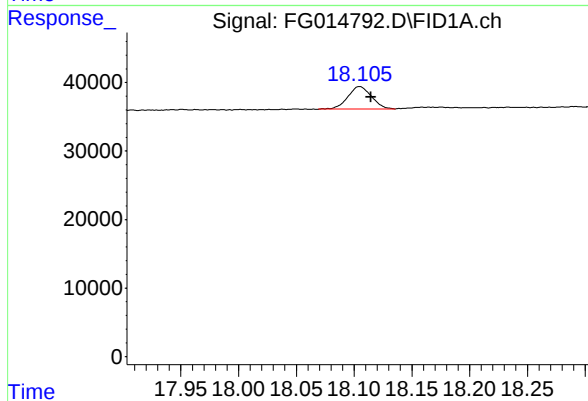

#13 N-TRIACONTANE


R.T.: 18.105 min
Delta R.T.: -0.010 min
Response: 46460
Conc: 0.40 ug/ml

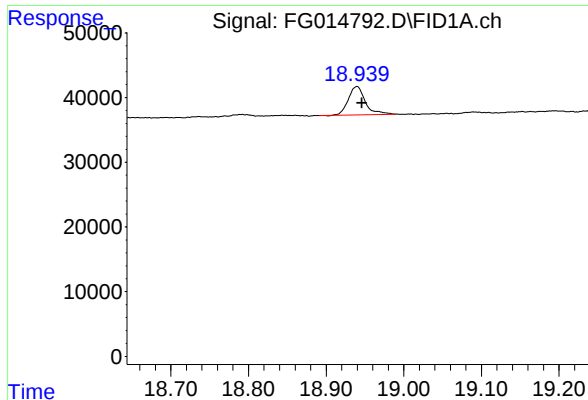

#14 N-DOTRIACONTANE


R.T.: 18.940 min
Delta R.T.: -0.006 min
Response: 65988
Conc: 0.60 ug/ml

Instrument :
FID_B
ClientSampleId :

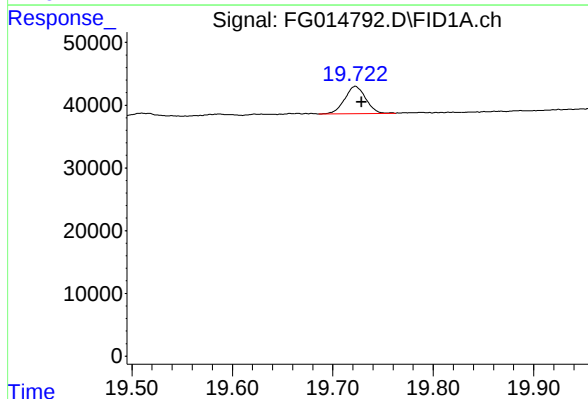


#15 N-TETRATRIACONTANE

R.T.: 19.722 min
Delta R.T.: -0.006 min
Response: 63408
Conc: 0.69 ug/ml

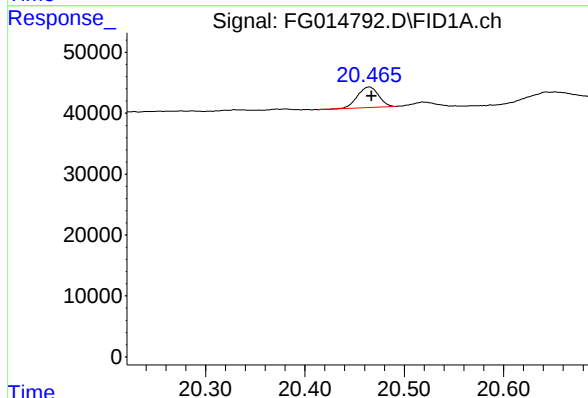


#16 N-HEXATRIACONTANE

R.T.: 20.465 min
Delta R.T.: -0.002 min
Response: 49521
Conc: 0.70 ug/ml

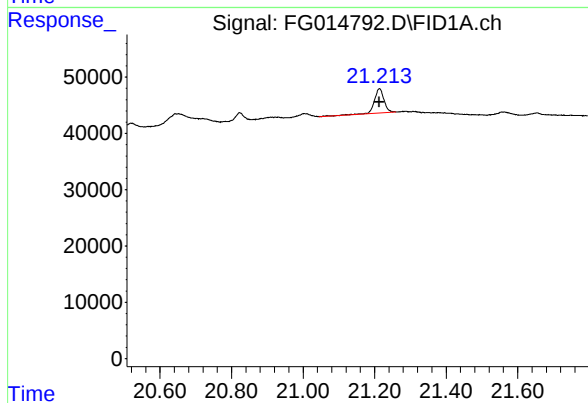

#17 N-OCTATRIACONTANE

R.T.: 21.213 min
Delta R.T.: 0.000 min
Response: 79186
Conc: 1.36 ug/ml

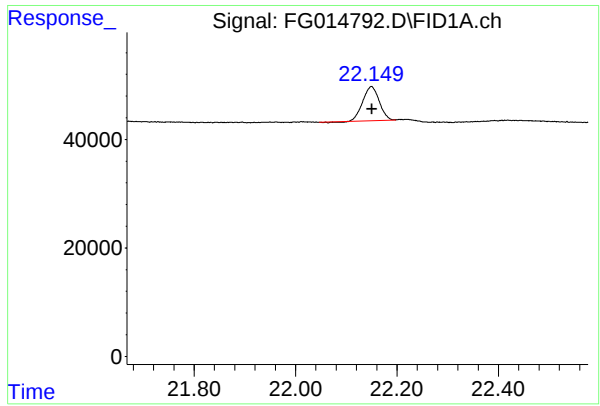

#18 N-TETRACONTANE

R.T.: 22.150 min
Delta R.T.: 0.000 min
Response: 140491
Conc: 2.76 ug/ml

Instrument :
FID_B
ClientSampleId :