

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG111524\  
 Data File : FG014793.D  
 Signal(s) : FID1A.ch  
 Acq On : 15 Nov 2024 11:24  
 Operator : YP\AJ  
 Sample : PB164989BL  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Nov 18 01:08:19 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG111324.M  
 Quant Title :  
 QLast Update : Wed Nov 13 13:49:18 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.041 | 1777058  | 15.843 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.938 | 32545    | 0.296 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.722 | 31576    | 0.342 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.462 | 22733    | 0.321 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG111524\  
Data File : FG014793.D  
Signal(s) : FID1A.ch  
Acq On : 15 Nov 2024 11:24  
Operator : YP\AJ  
Sample : PB164989BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 18 01:08:19 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG111324.M  
Quant Title :  
QLast Update : Wed Nov 13 13:49:18 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

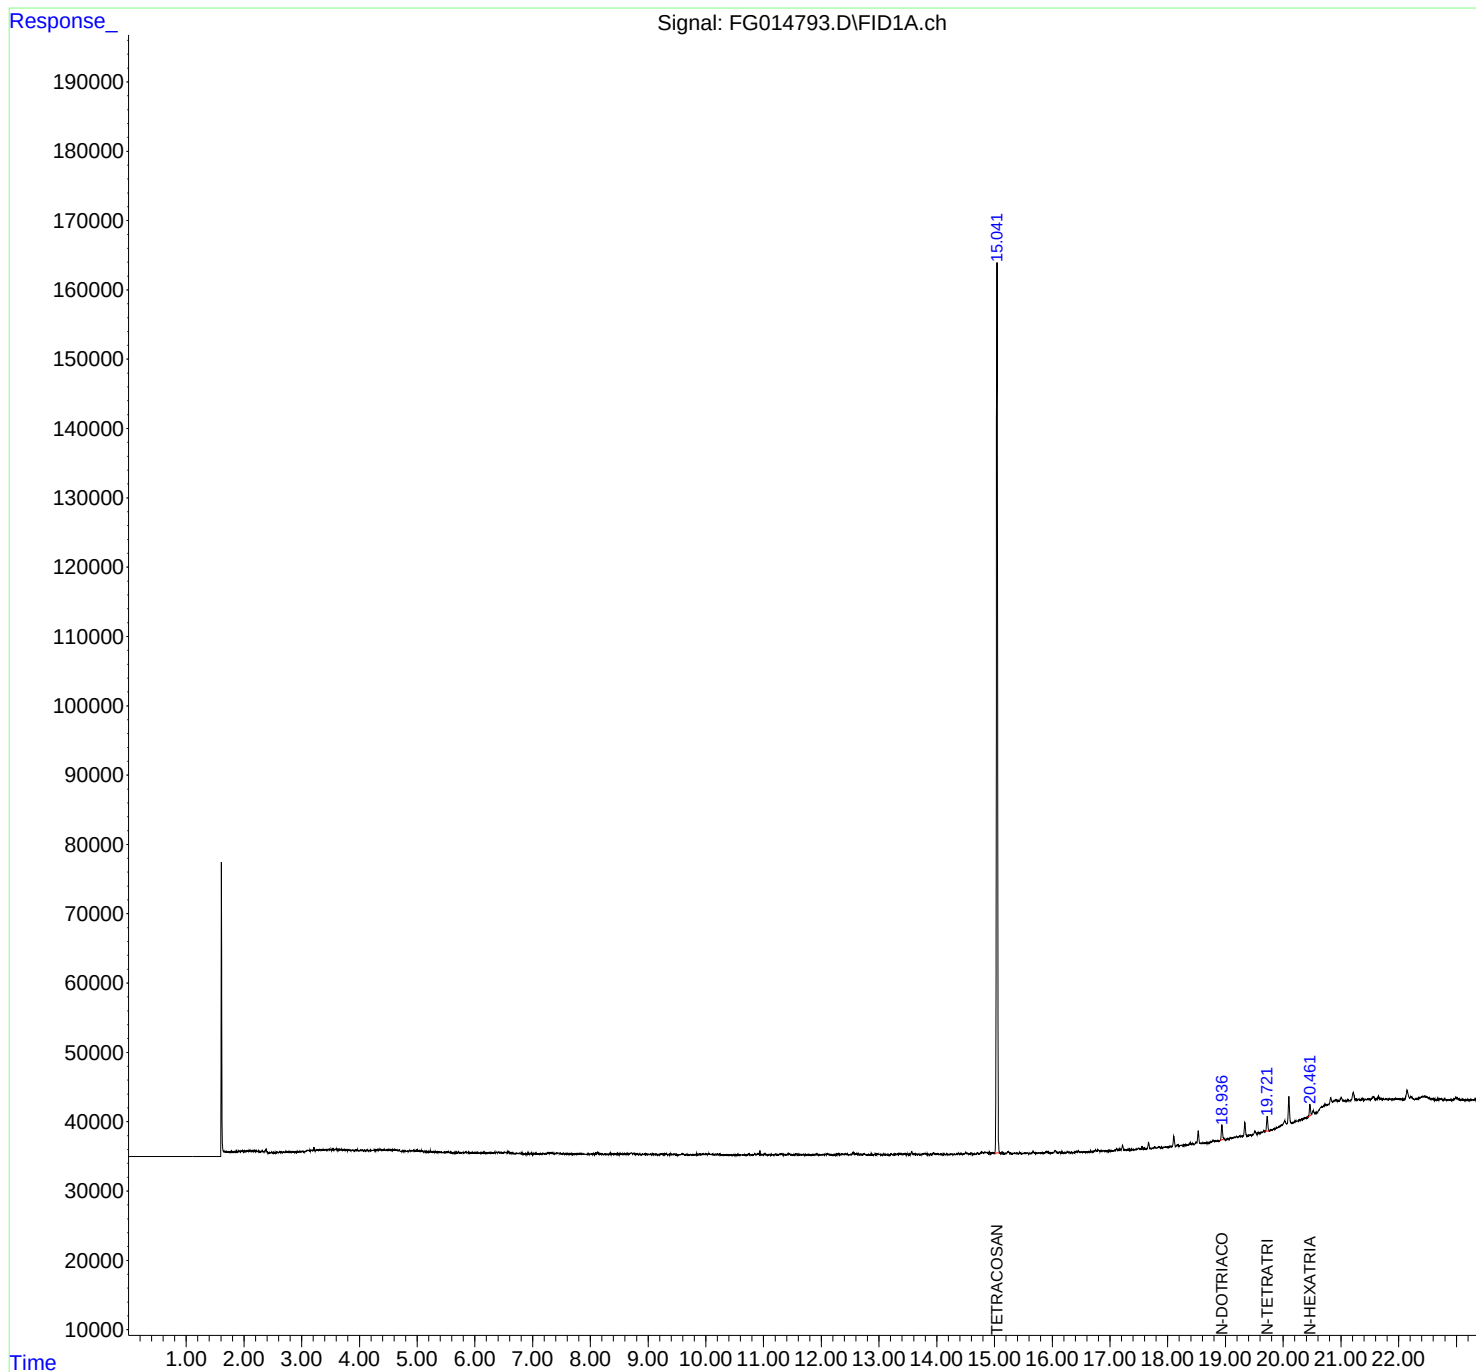


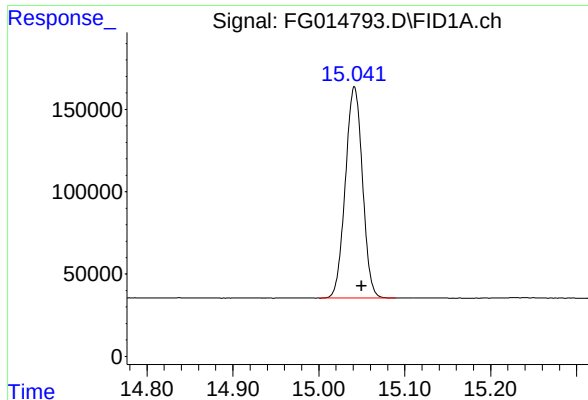

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.041 min  
Delta R.T.: -0.008 min  
Response: 1777058  
Conc: 15.84 ug/ml

Instrument :  
FID\_B  
ClientSampleId :

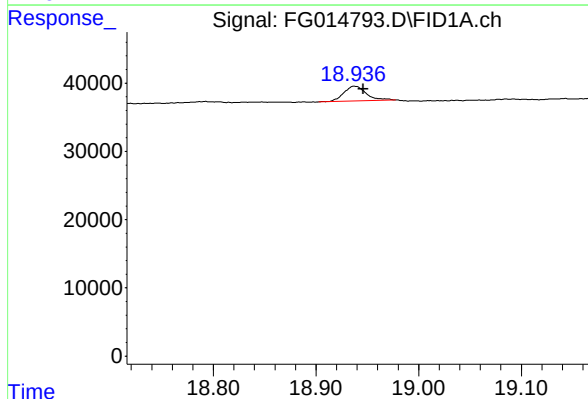


#14 N-DOTRIACONTANE

R.T.: 18.938 min  
Delta R.T.: -0.009 min  
Response: 32545  
Conc: 0.30 ug/ml

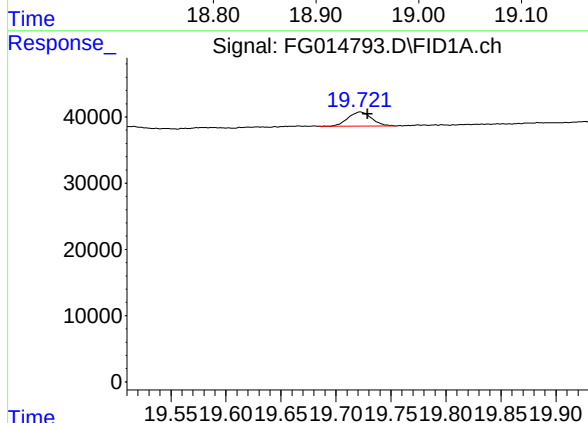

#15 N-TETRATRIACONTANE

R.T.: 19.722 min  
Delta R.T.: -0.007 min  
Response: 31576  
Conc: 0.34 ug/ml

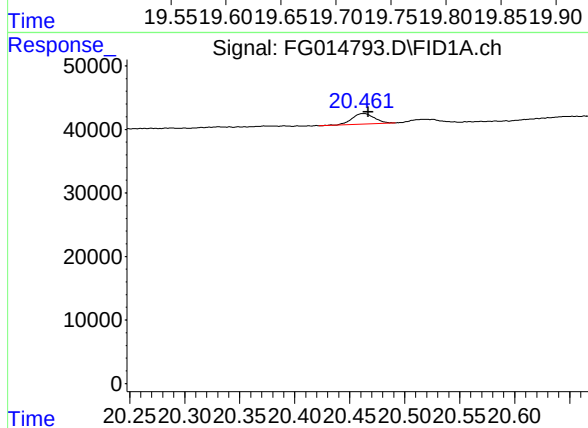

#16 N-HEXATRIACONTANE

R.T.: 20.462 min  
Delta R.T.: -0.005 min  
Response: 22733  
Conc: 0.32 ug/ml