

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111524\
Data File : FG014800.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2024 15:11
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 18 01:09:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111324.M
Quant Title :
QLast Update : Wed Nov 13 13:49:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.043	1994087	17.777 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.106	39296	0.341 ug/ml
14) N-DOTRIACONTANE	18.939	41834	0.381 ug/ml
15) N-TETRATRIACONTANE	19.723	53386	0.578 ug/ml
16) N-HEXATRIACONTANE	20.464	28133	0.397 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111524\
Data File : FG014800.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2024 15:11
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 18 01:09:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111324.M
Quant Title :
QLast Update : Wed Nov 13 13:49:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

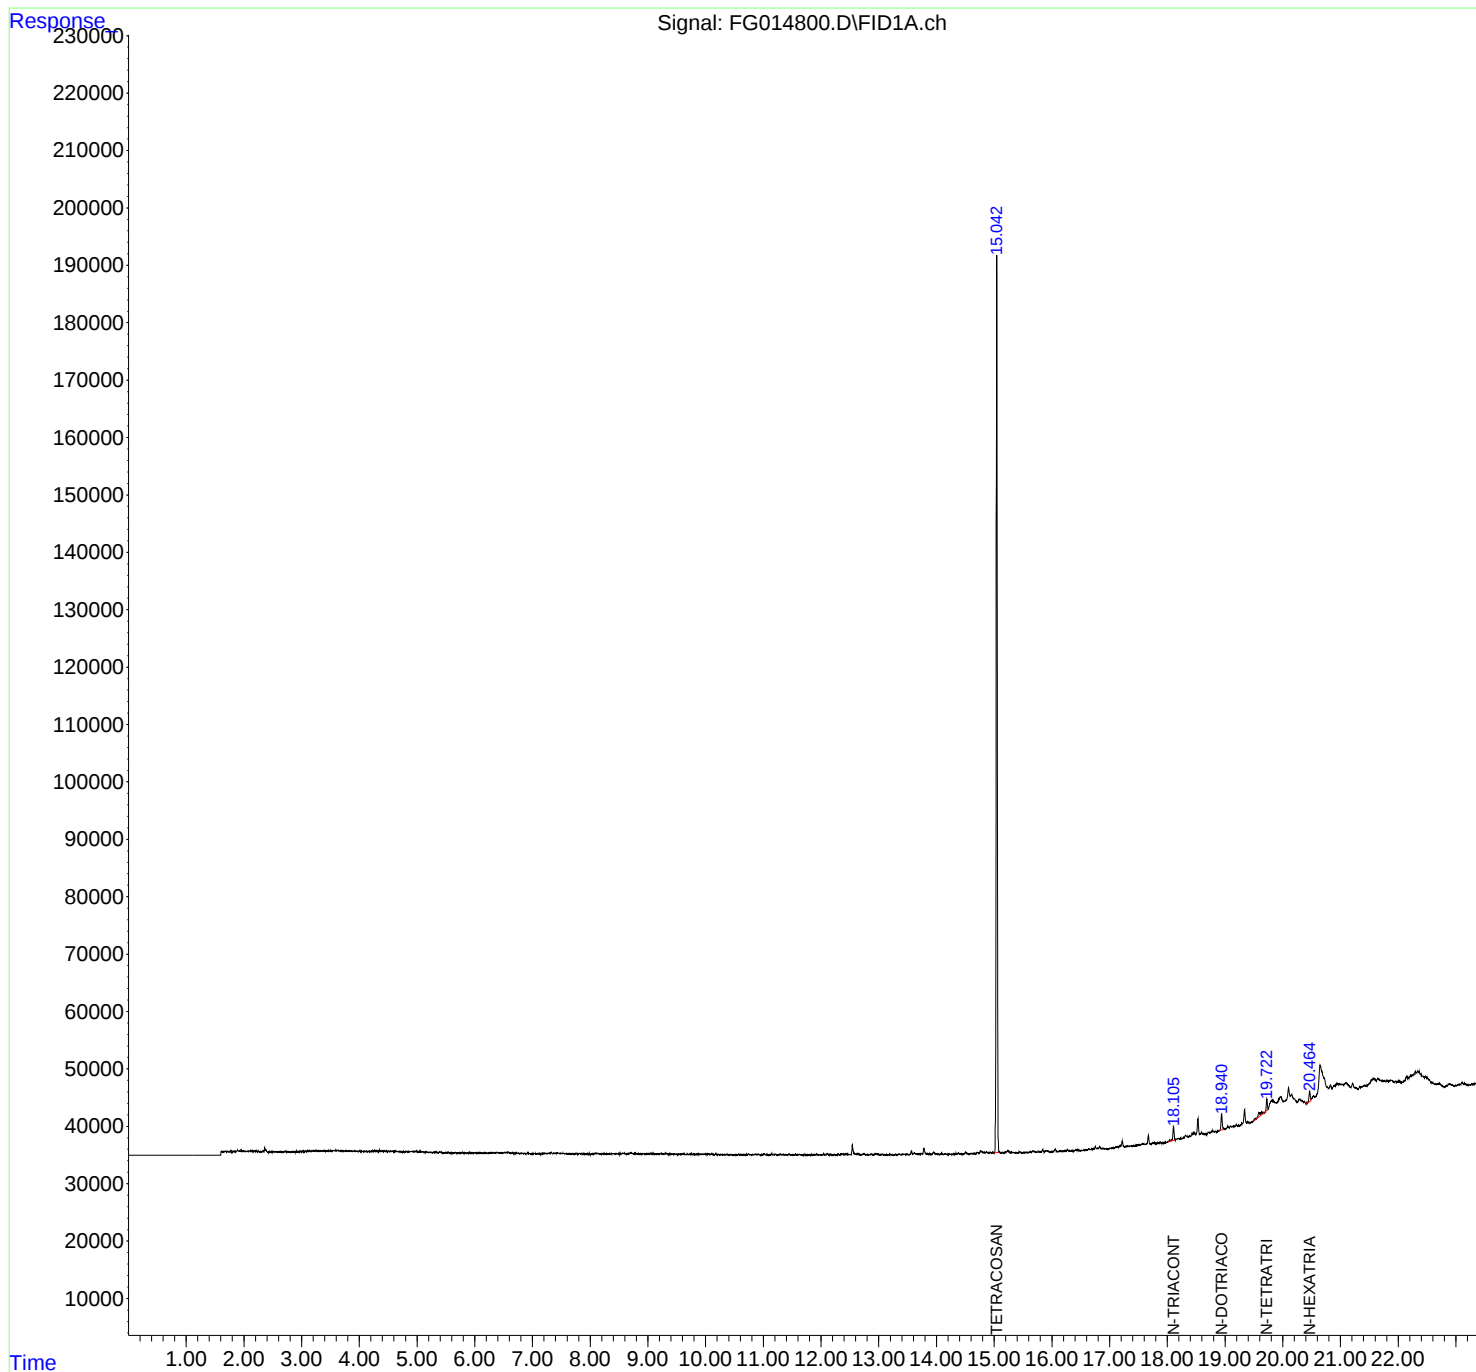


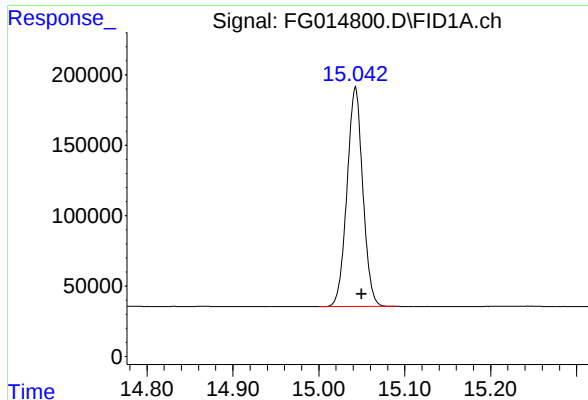

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.043 min
Delta R.T.: -0.007 min
Response: 1994087
Conc: 17.78 ug/ml

Instrument :
FID_B
ClientSampleId :

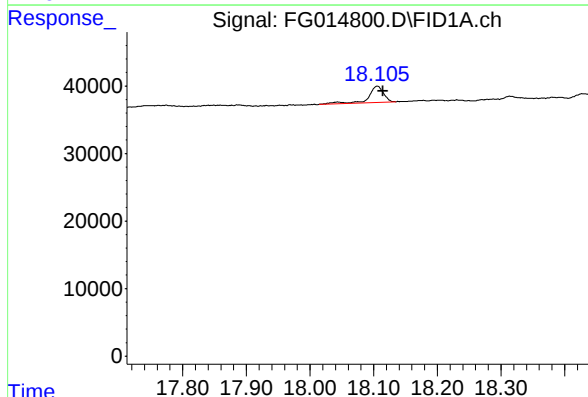


#13 N-TRIACONTANE

R.T.: 18.106 min
Delta R.T.: -0.009 min
Response: 39296
Conc: 0.34 ug/ml

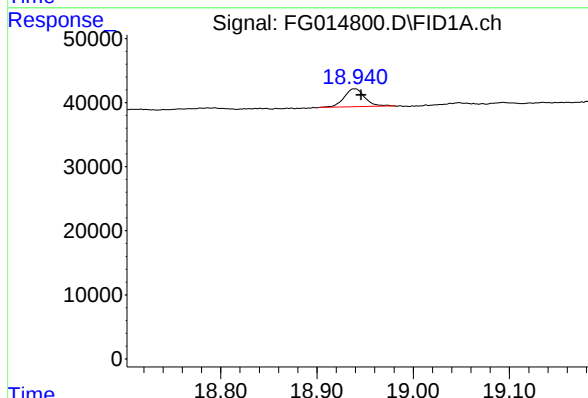


#14 N-DOTRIACONTANE

R.T.: 18.939 min
Delta R.T.: -0.007 min
Response: 41834
Conc: 0.38 ug/ml

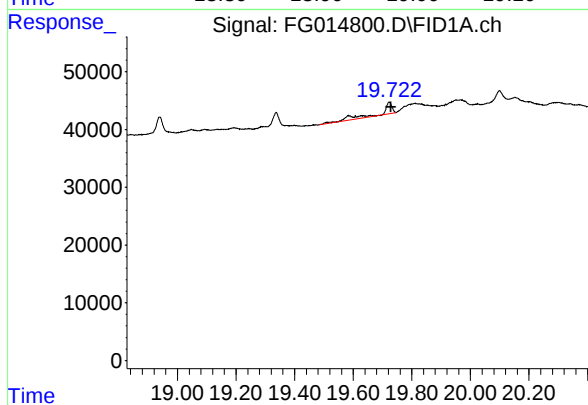

#15 N-TETRATRIACONTANE

R.T.: 19.723 min
Delta R.T.: -0.006 min
Response: 53386
Conc: 0.58 ug/ml

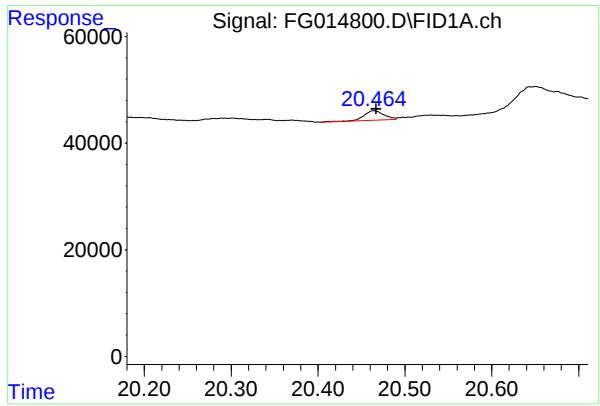

#16 N-HEXATRIACONTANE

R.T.: 20.464 min
Delta R.T.: -0.003 min
Response: 28133
Conc: 0.40 ug/ml

Instrument :

FID_B

ClientSampleId :