

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
 Data File : FB031203.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2024 8:44
 Operator : YP/AJ
 Sample : BSF1115S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1115S1

Integration File: Calibration.e
 Quant Time: Nov 18 02:29:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	451447	16.355 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	1044283	26.589 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1301814	27.795 ng/ml
3) t n-Heptane	7.753	380972	8.406 ng/ml
4) t Benzene	7.890	491740	9.199 ng/ml
6) t Toluene	10.619	1329745	26.629 ng/ml
7) t Ethylbenzene	13.056	387833	8.664 ng/ml
8) t m-Xylene	13.190	826401	16.991 ng/ml
9) t O-Xylene	13.918	773638	16.972 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	594560	15.979 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
Data File : FB031203.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2024 8:44
Operator : YP/AJ
Sample : BSF1115S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1115S1

Integration File: Calibration.e
Quant Time: Nov 18 02:29:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

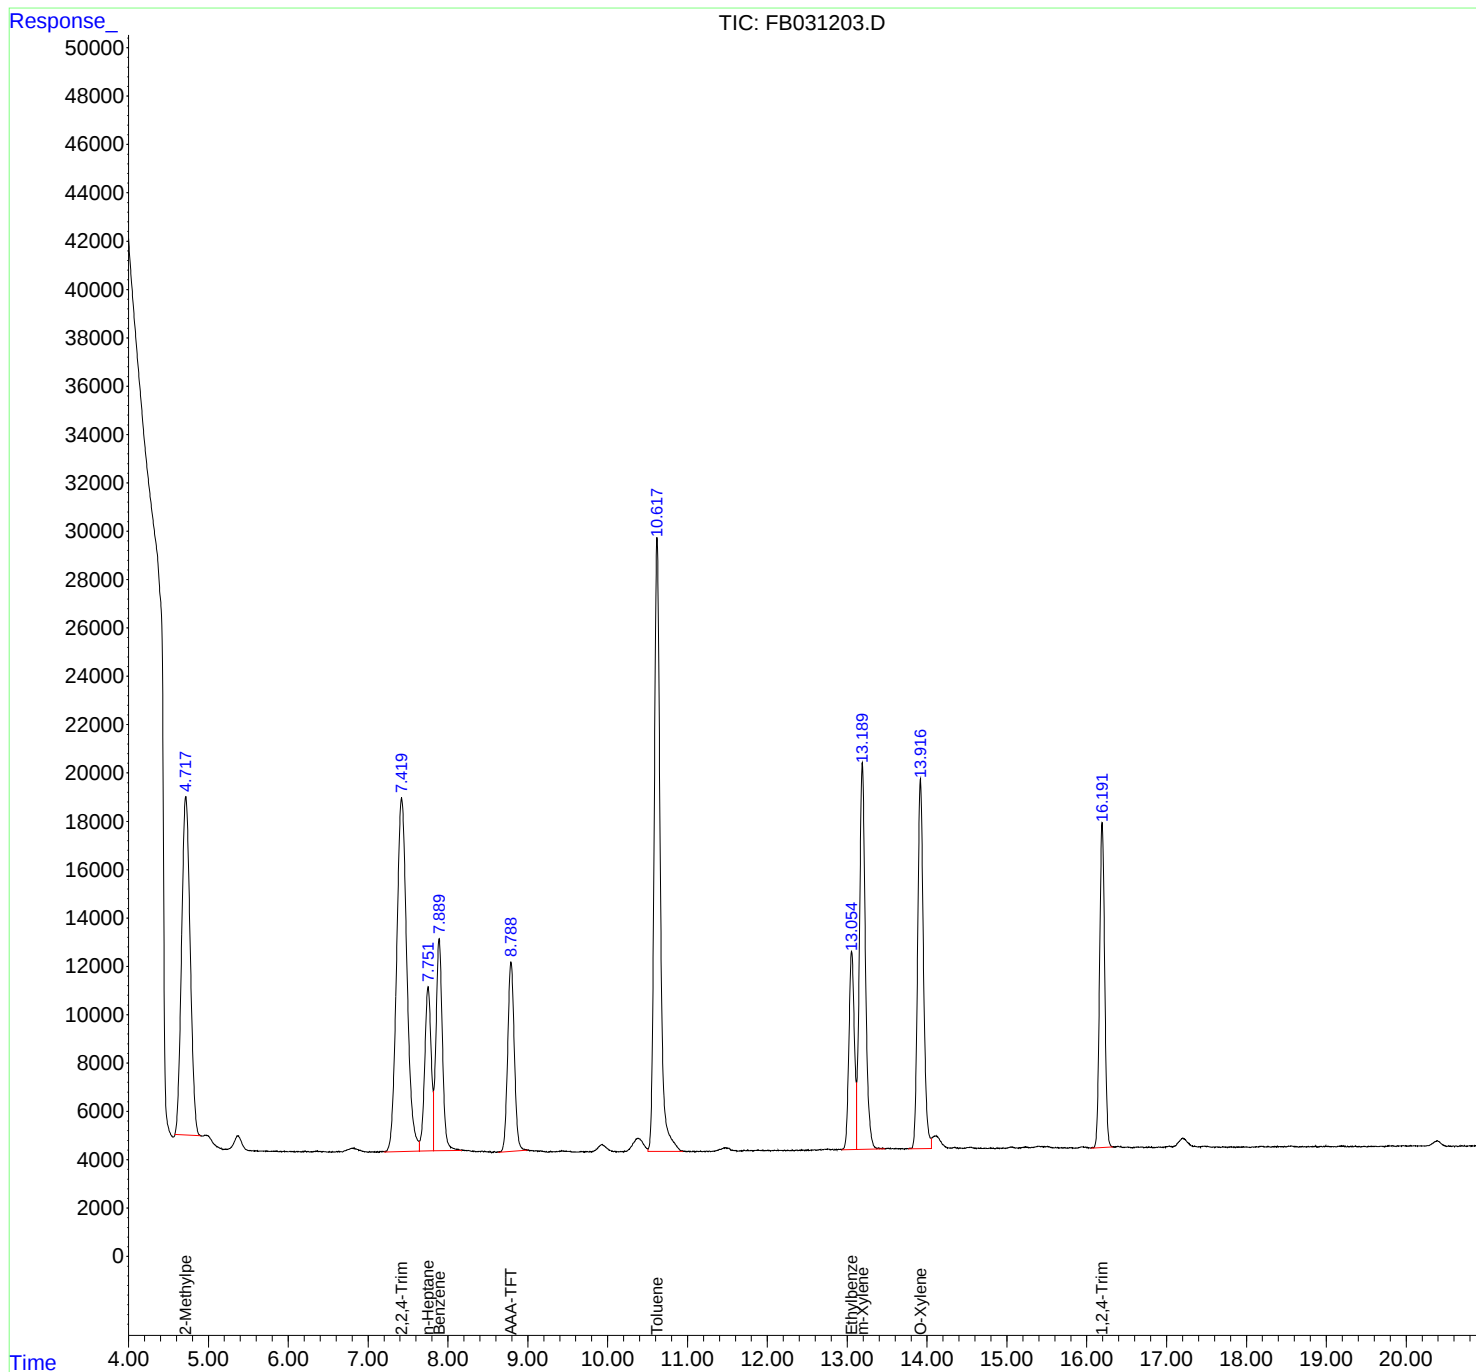


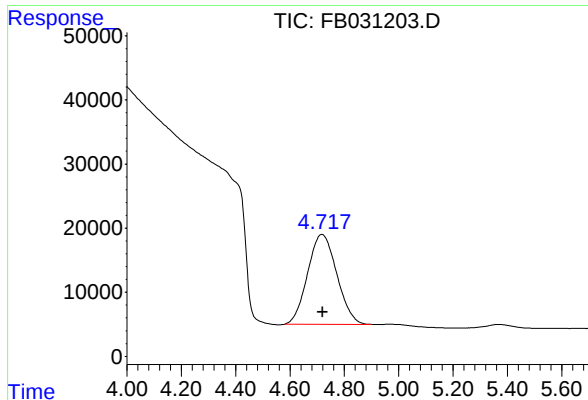

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 1044283
Conc: 26.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S1

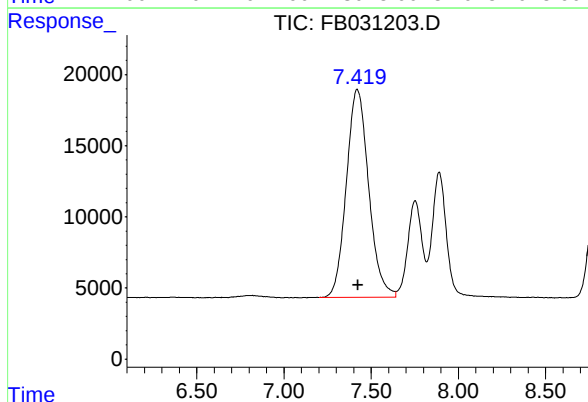


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.005 min
Response: 1301814
Conc: 27.79 ng/ml

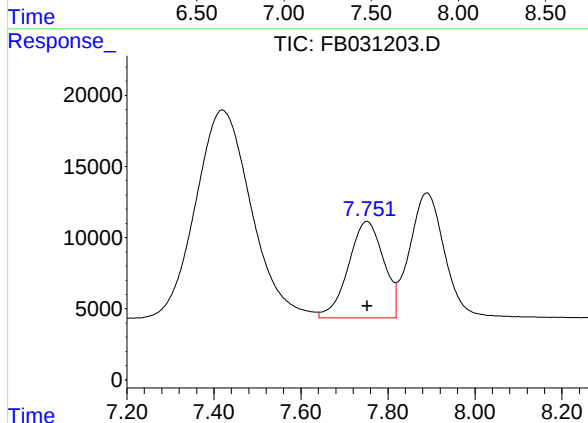


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.000 min
Response: 380972
Conc: 8.41 ng/ml

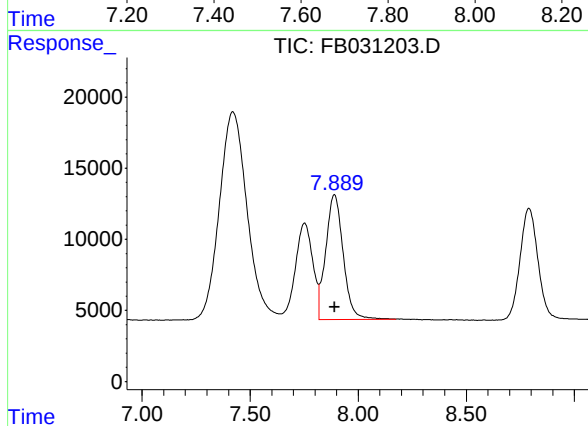

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 491740
Conc: 9.20 ng/ml

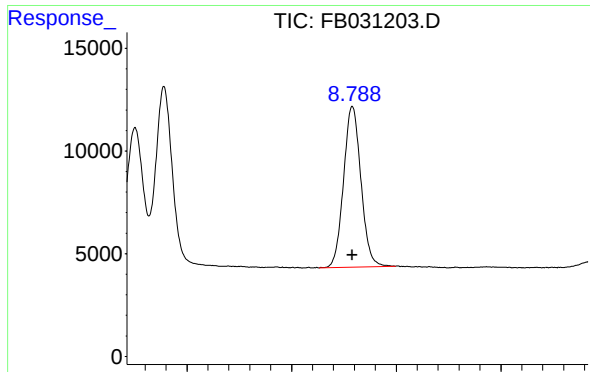

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 451447
Conc: 16.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S1

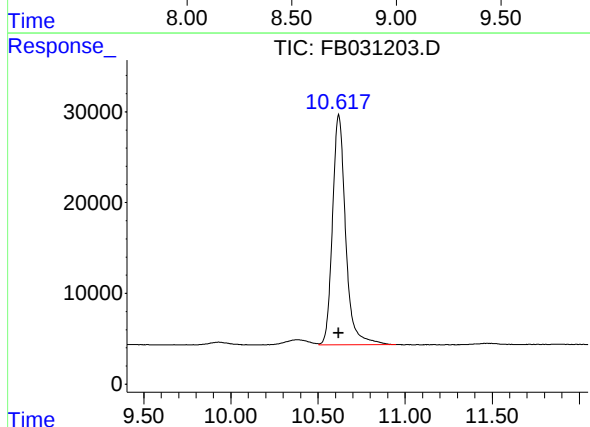


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 1329745
Conc: 26.63 ng/ml

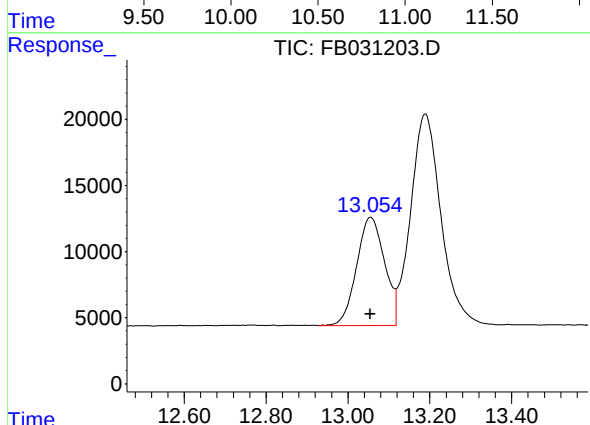


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 387833
Conc: 8.66 ng/ml

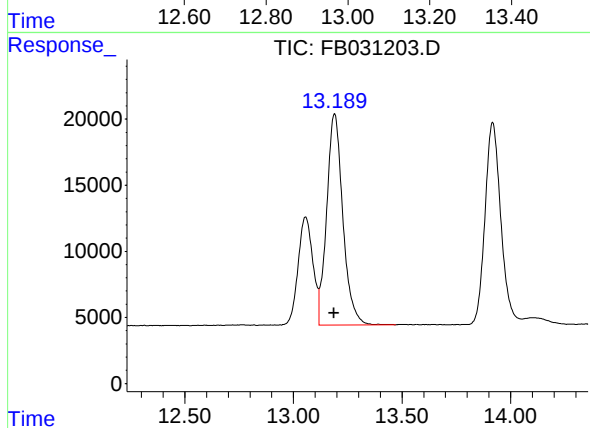

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 826401
Conc: 16.99 ng/ml

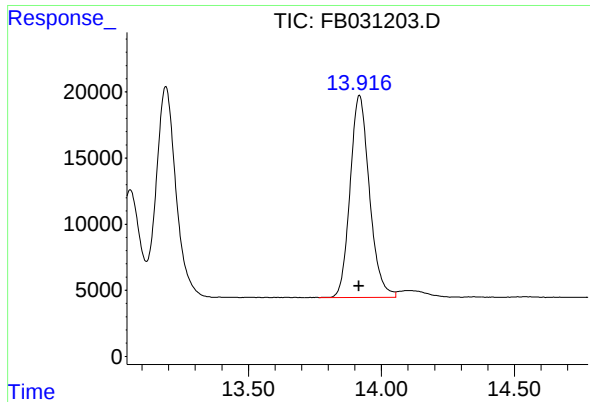

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 773638
Conc: 16.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S1

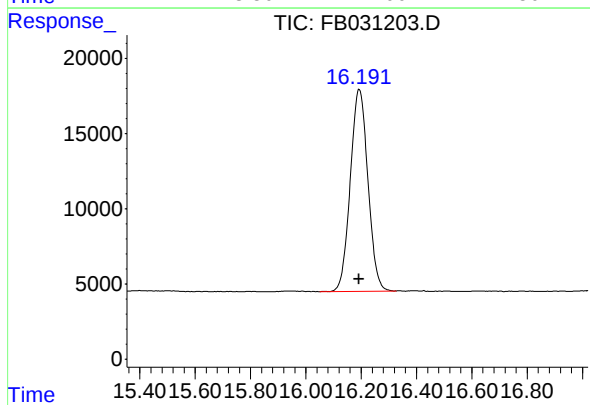

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 594560
Conc: 15.98 ng/ml