

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
 Data File : FB031221.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2024 18:15
 Operator : YP/AJ
 Sample : BSF1115S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1115S3

Integration File: Calibration.e
 Quant Time: Nov 18 02:31:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	467504	16.937 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.721	1073109	27.323 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	1311201	27.995 ng/ml
3) t n-Heptane	7.755	402000	8.870 ng/ml
4) t Benzene	7.894	502410	9.399 ng/ml
6) t Toluene	10.623	1395024	27.936 ng/ml
7) t Ethylbenzene	13.060	404084	9.027 ng/ml
8) t m-Xylene	13.194	863414	17.752 ng/ml
9) t O-Xylene	13.922	807247	17.709 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	632432	16.997 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
Data File : FB031221.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2024 18:15
Operator : YP/AJ
Sample : BSF1115S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1115S3

Integration File: Calibration.e
Quant Time: Nov 18 02:31:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

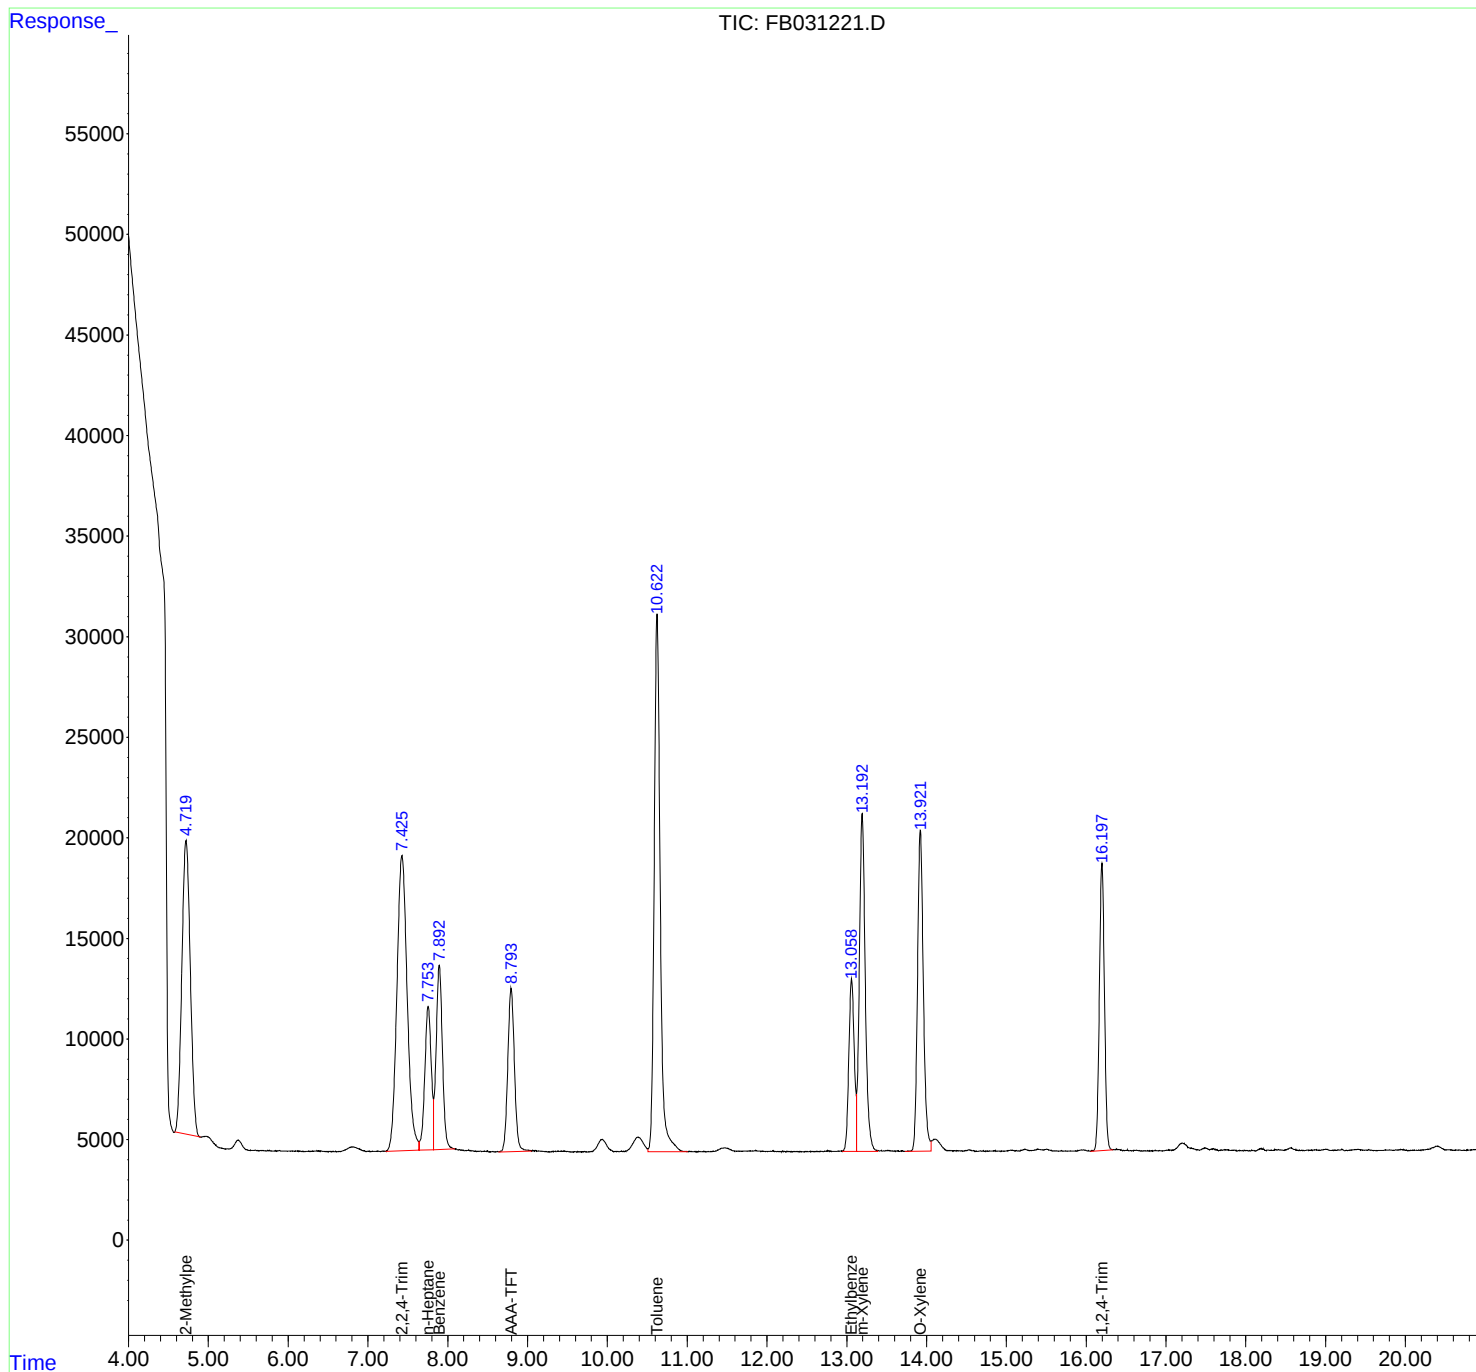


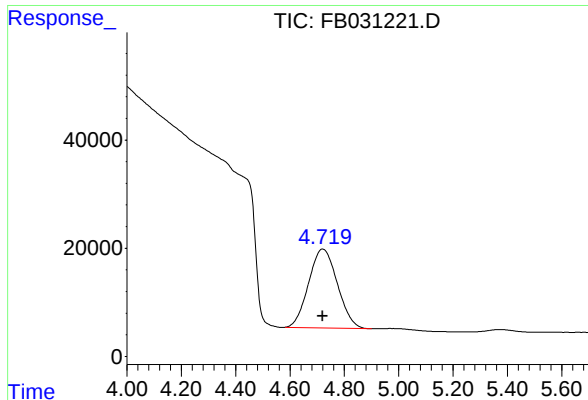

#1 2-Methylpentane


R.T.: 4.721 min
Delta R.T.: 0.000 min
Response: 1073109
Conc: 27.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S3

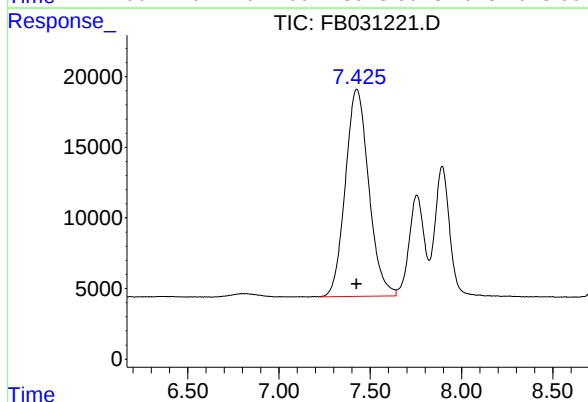


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.002 min
Response: 1311201
Conc: 28.00 ng/ml

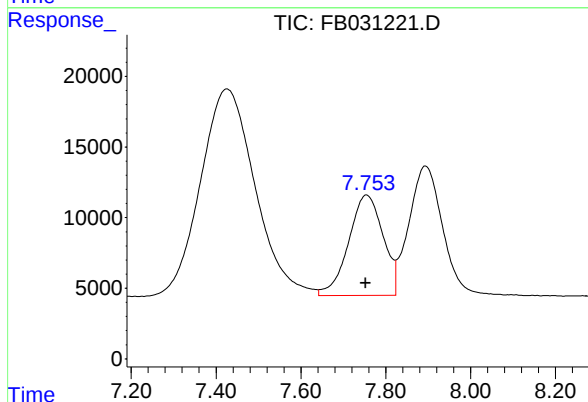


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.002 min
Response: 402000
Conc: 8.87 ng/ml

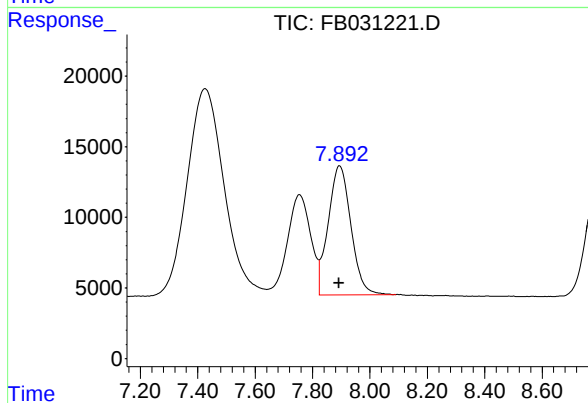

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 502410
Conc: 9.40 ng/ml

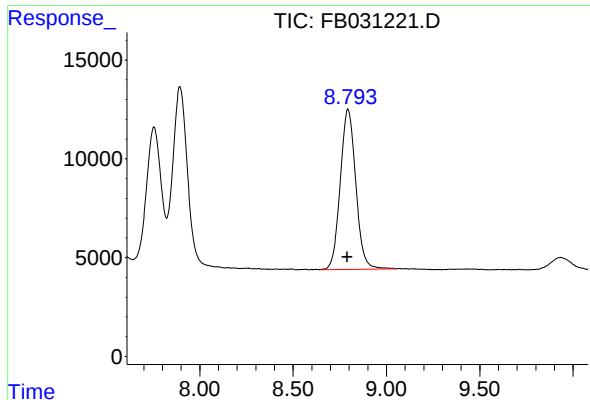

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 467504
Conc: 16.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S3

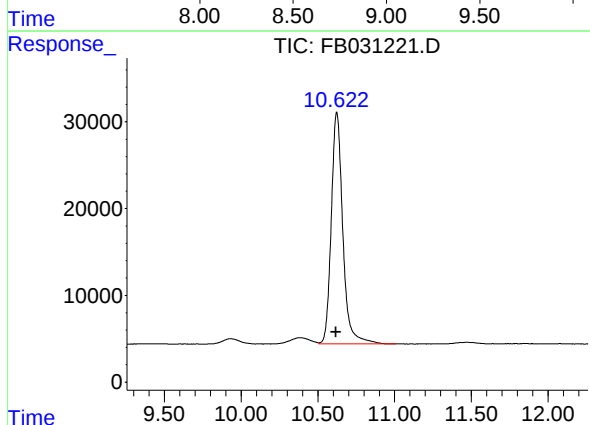


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 1395024
Conc: 27.94 ng/ml

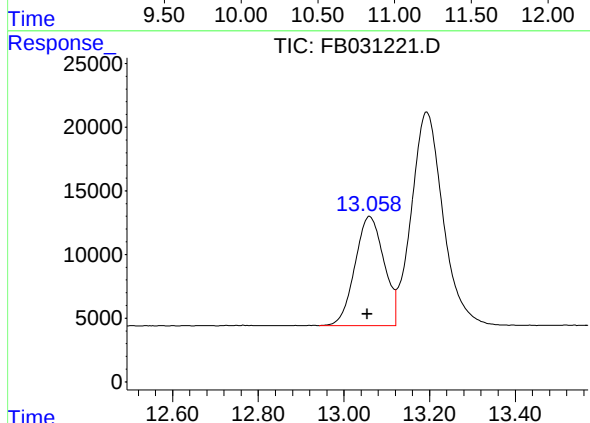


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 404084
Conc: 9.03 ng/ml

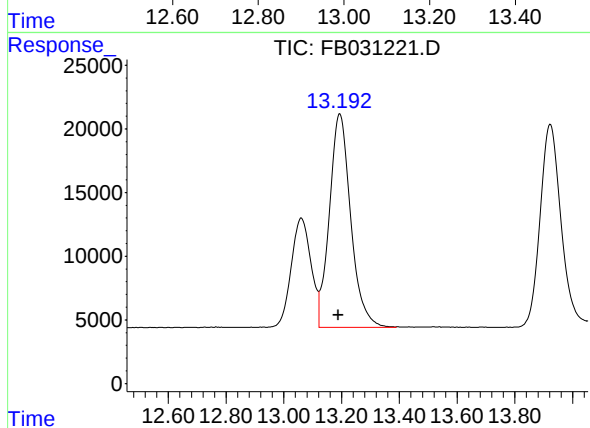

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.006 min
Response: 863414
Conc: 17.75 ng/ml

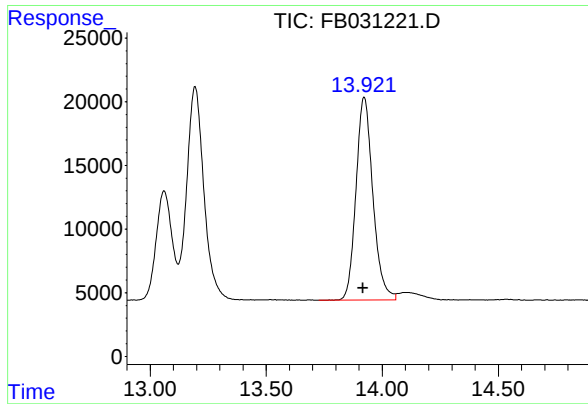

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.006 min
Response: 807247
Conc: 17.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S3

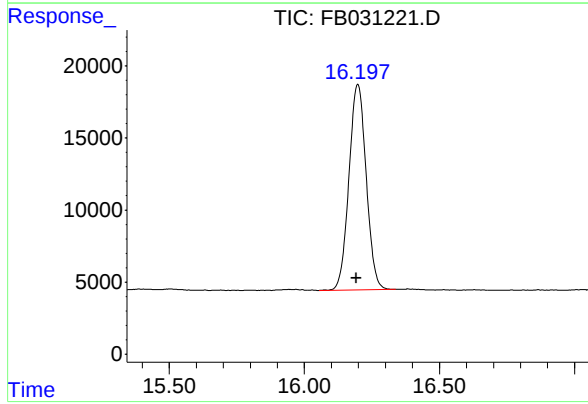

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.006 min
Response: 632432
Conc: 17.00 ng/ml