

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
 Data File : FB031233.D
 Signal(s) : FID2B.CH
 Acq On : 15 Nov 2024 00:57
 Operator : YP/AJ
 Sample : BSF1115S4
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1115S4

Integration File: Calibration.e
 Quant Time: Nov 18 02:32:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.794	446388	16.172 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.720	1114744	28.383 ng/ml
2) t	2,2,4-Trimethylpentane	7.427	1375769	29.374 ng/ml
3) t	n-Heptane	7.755	427626	9.436 ng/ml
4) t	Benzene	7.893	541453	10.129 ng/ml
6) t	Toluene	10.623	1504122	30.121 ng/ml
7) t	Ethylbenzene	13.060	435883	9.738 ng/ml
8) t	m-Xylene	13.194	922872	18.974 ng/ml
9) t	O-Xylene	13.922	862919	18.931 ng/ml
10) t	1,2,4-Trimethylbenzene	16.198	673983	18.114 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111524\
Data File : FB031233.D
Signal(s) : FID2B.CH
Acq On : 15 Nov 2024 00:57
Operator : YP/AJ
Sample : BSF1115S4
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1115S4

Integration File: Calibration.e
Quant Time: Nov 18 02:32:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

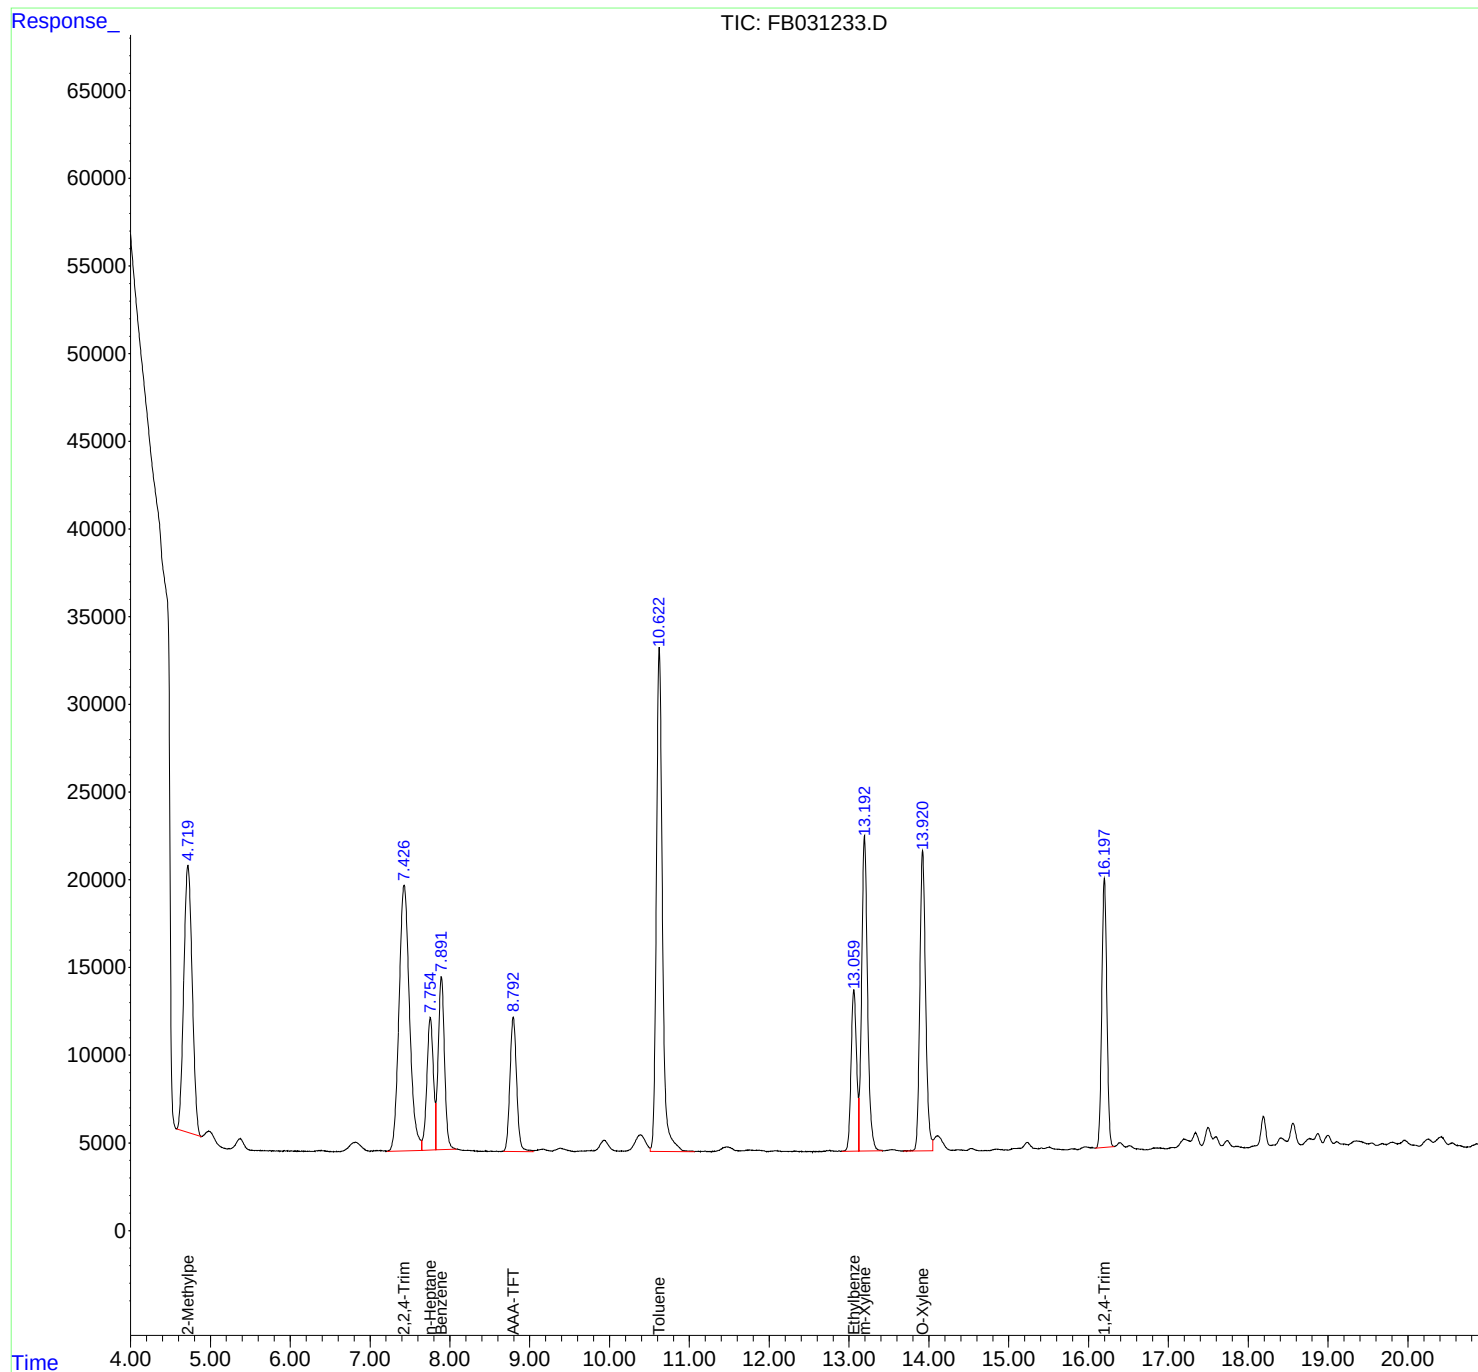


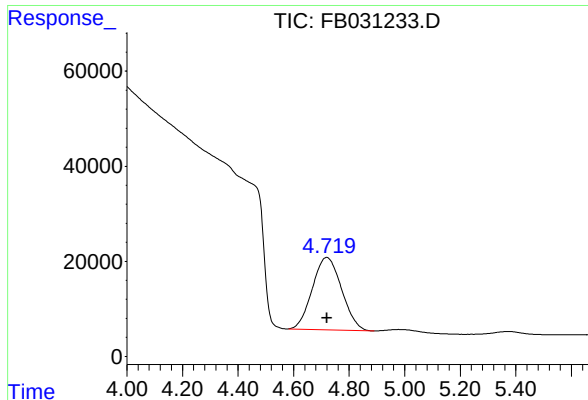

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 1114744
Conc: 28.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S4

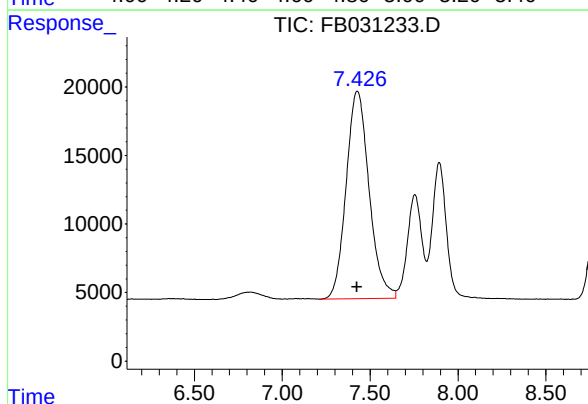


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.003 min
Response: 1375769
Conc: 29.37 ng/ml

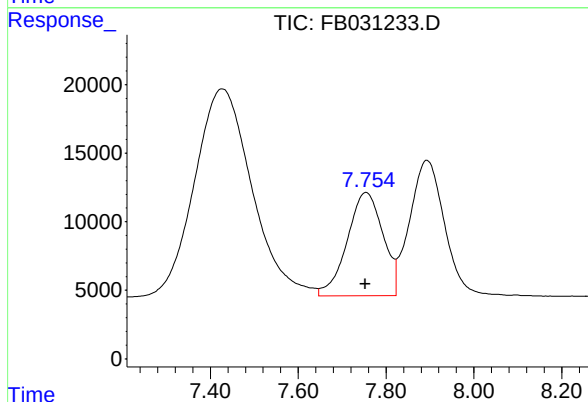


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 427626
Conc: 9.44 ng/ml

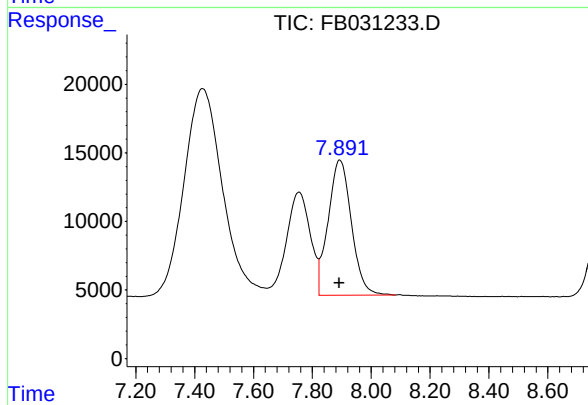

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.002 min
Response: 541453
Conc: 10.13 ng/ml

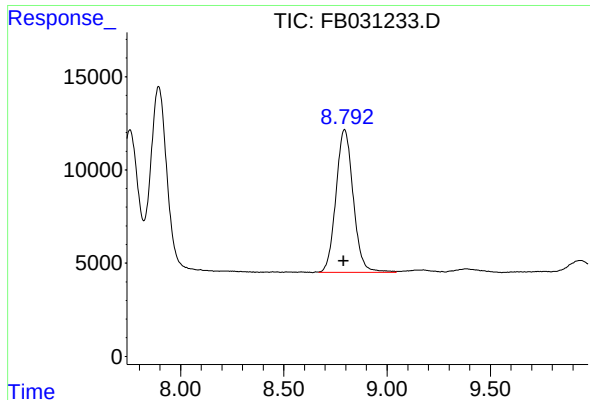

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 446388
Conc: 16.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S4

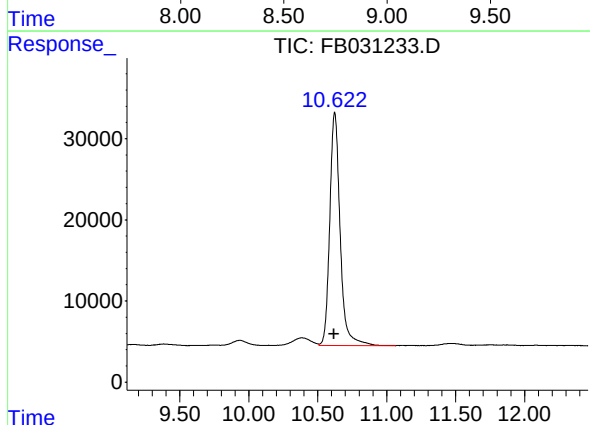


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 1504122
Conc: 30.12 ng/ml

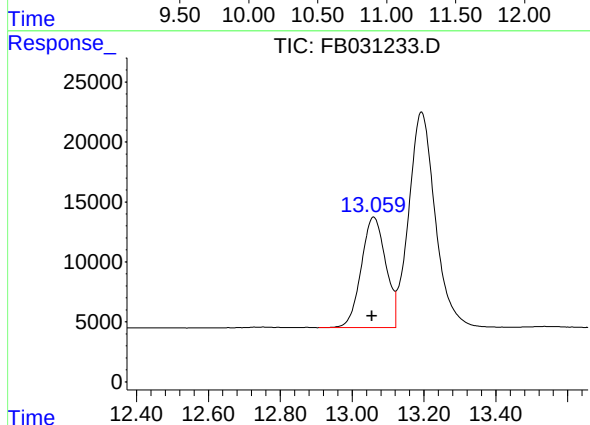


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 435883
Conc: 9.74 ng/ml

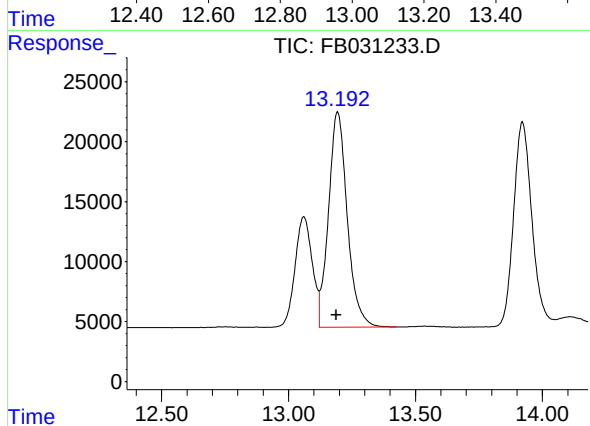

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.005 min
Response: 922872
Conc: 18.97 ng/ml

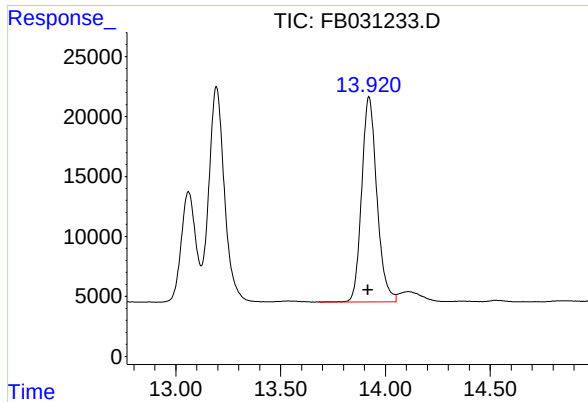

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.005 min
Response: 862919
Conc: 18.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1115S4

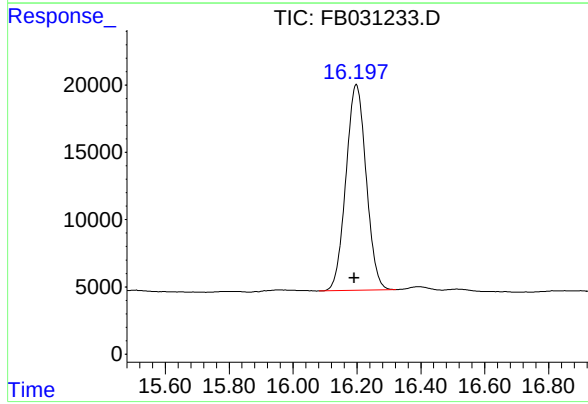

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.006 min
Response: 673983
Conc: 18.11 ng/ml