

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111621\
 Data File : FB026350.D
 Signal(s) : FID2B.CH
 Acq On : 16 Nov 2021 12:24
 Operator : AJ/MA
 Sample : BSF1116S1
 Misc : 4.99G\5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 17 00:12:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	260182	21.962 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	496354	29.809 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	583998	29.950 ng/ml
3) t n-Heptane	7.750	182218	9.876 ng/ml
4) t Benzene	7.887	216724	9.941 ng/ml
6) t Toluene	10.619	615475	29.674 ng/ml
7) t Ethylbenzene	13.056	193492	10.246 ng/ml
8) t m-Xylene	13.189	382573	20.114 ng/ml
9) t O-Xylene	13.916	373624	20.229 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	394956	20.833 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111621\
Data File : FB026350.D
Signal(s) : FID2B.CH
Acq On : 16 Nov 2021 12:24
Operator : AJ/MA
Sample : BSF1116S1
Misc : 4.99G\5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 17 00:12:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

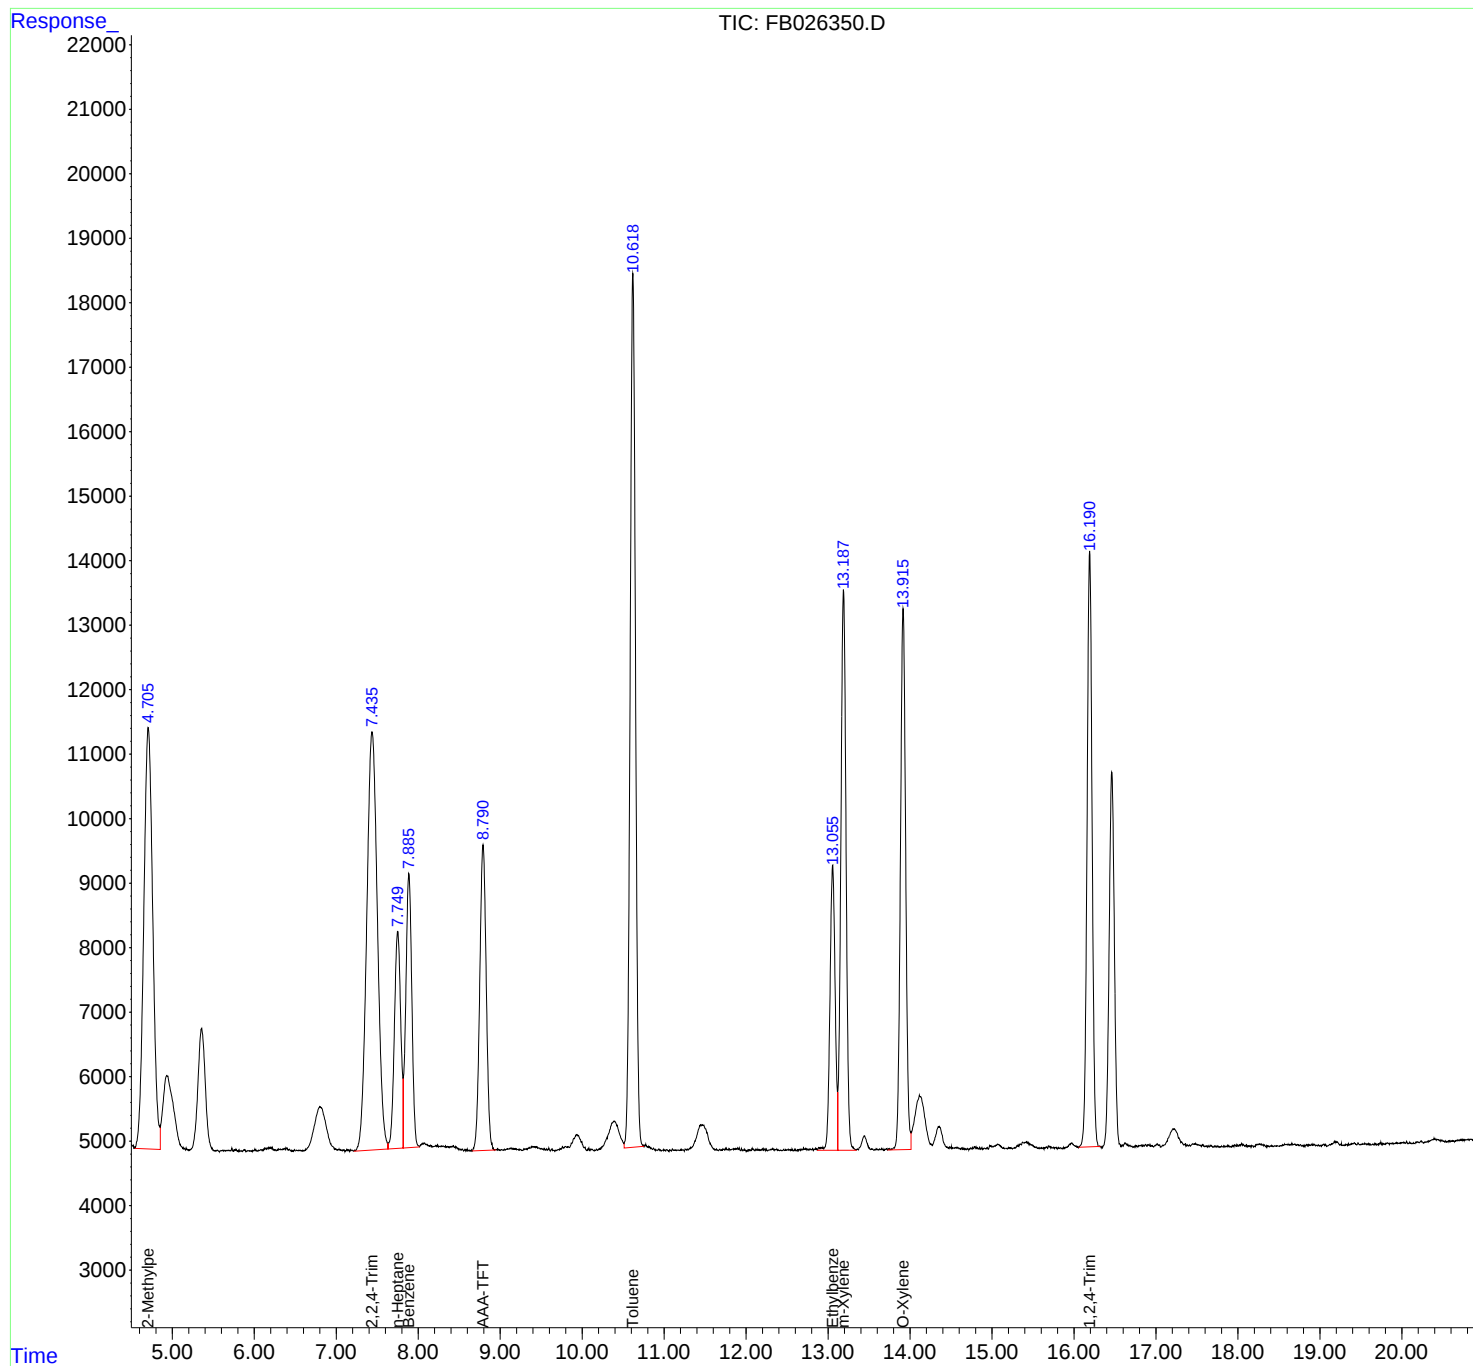

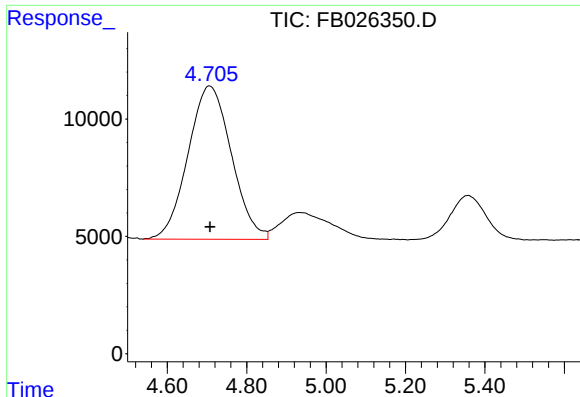


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.002 min
Response: 496354
Conc: 29.81 ng/ml

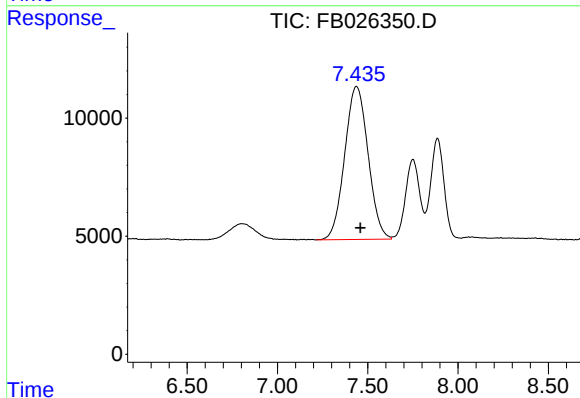


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: -0.023 min
Response: 583998
Conc: 29.95 ng/ml

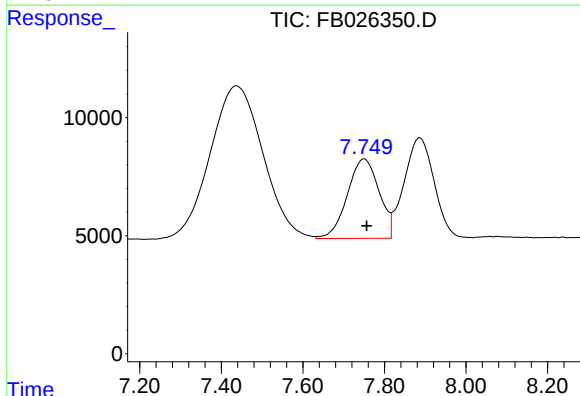


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.006 min
Response: 182218
Conc: 9.88 ng/ml

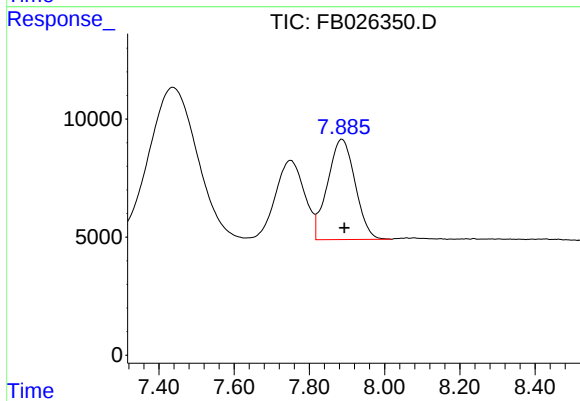


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.007 min
Response: 216724
Conc: 9.94 ng/ml

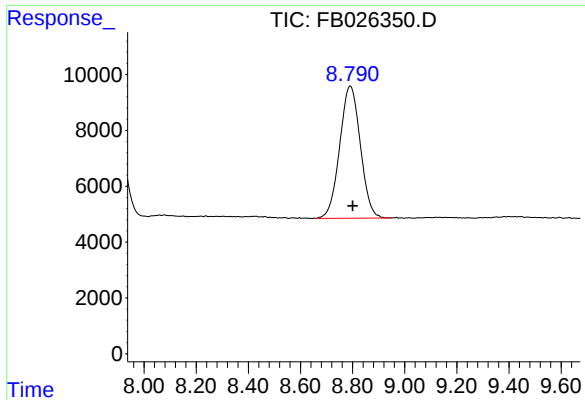


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.009 min
Response: 260182
Conc: 21.96 ng/ml

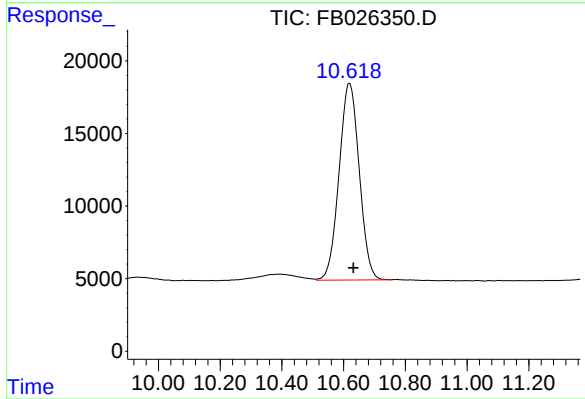


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.012 min
Response: 615475
Conc: 29.67 ng/ml

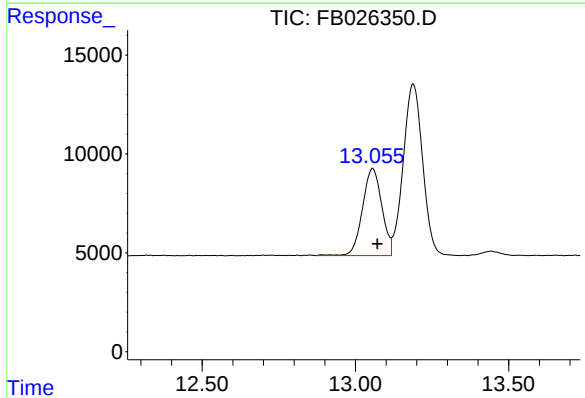


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.015 min
Response: 193492
Conc: 10.25 ng/ml

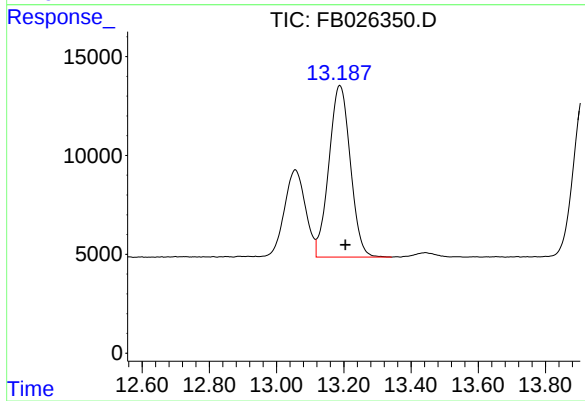


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.016 min
Response: 382573
Conc: 20.11 ng/ml

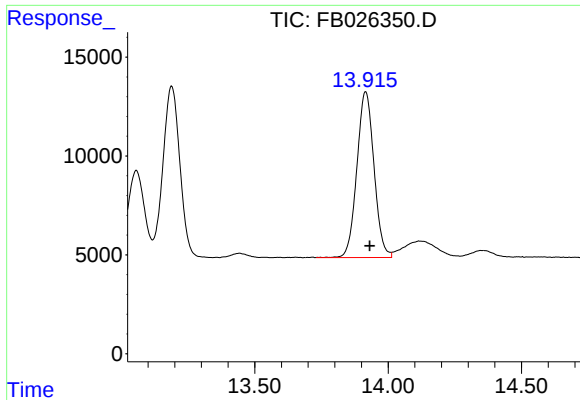

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.016 min
Response: 373624
Conc: 20.23 ng/ml

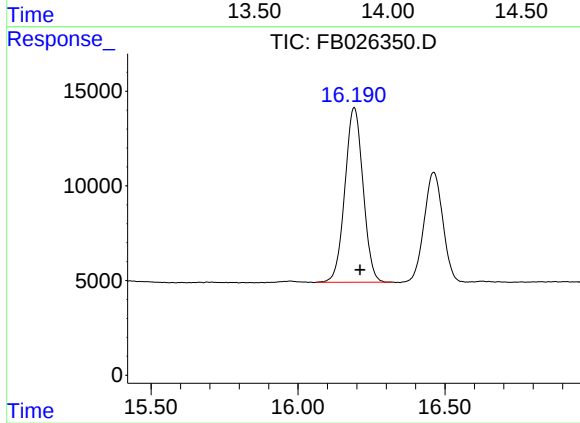

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.020 min
Response: 394956
Conc: 20.83 ng/ml