

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111621\
 Data File : FB026353.D
 Signal(s) : FID2B.CH
 Acq On : 16 Nov 2021 16:19
 Operator : AJ/MA
 Sample : M4684-01MSD
 Misc : 5.04G\5.00ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 17 00:13:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	231327	19.526 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	481301	28.905 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	576344	29.558 ng/ml
3) t n-Heptane	7.750	182973	9.917 ng/ml
4) t Benzene	7.886	215967	9.906 ng/ml
6) t Toluene	10.620	621295	29.955 ng/ml
7) t Ethylbenzene	13.057	194520	10.301 ng/ml
8) t m-Xylene	13.189	387290	20.362 ng/ml
9) t O-Xylene	13.917	376256	20.371 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	393943	20.780 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111621\
Data File : FB026353.D
Signal(s) : FID2B.CH
Acq On : 16 Nov 2021 16:19
Operator : AJ/MA
Sample : M4684-01MSD
Misc : 5.04G\5.00ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 17 00:13:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

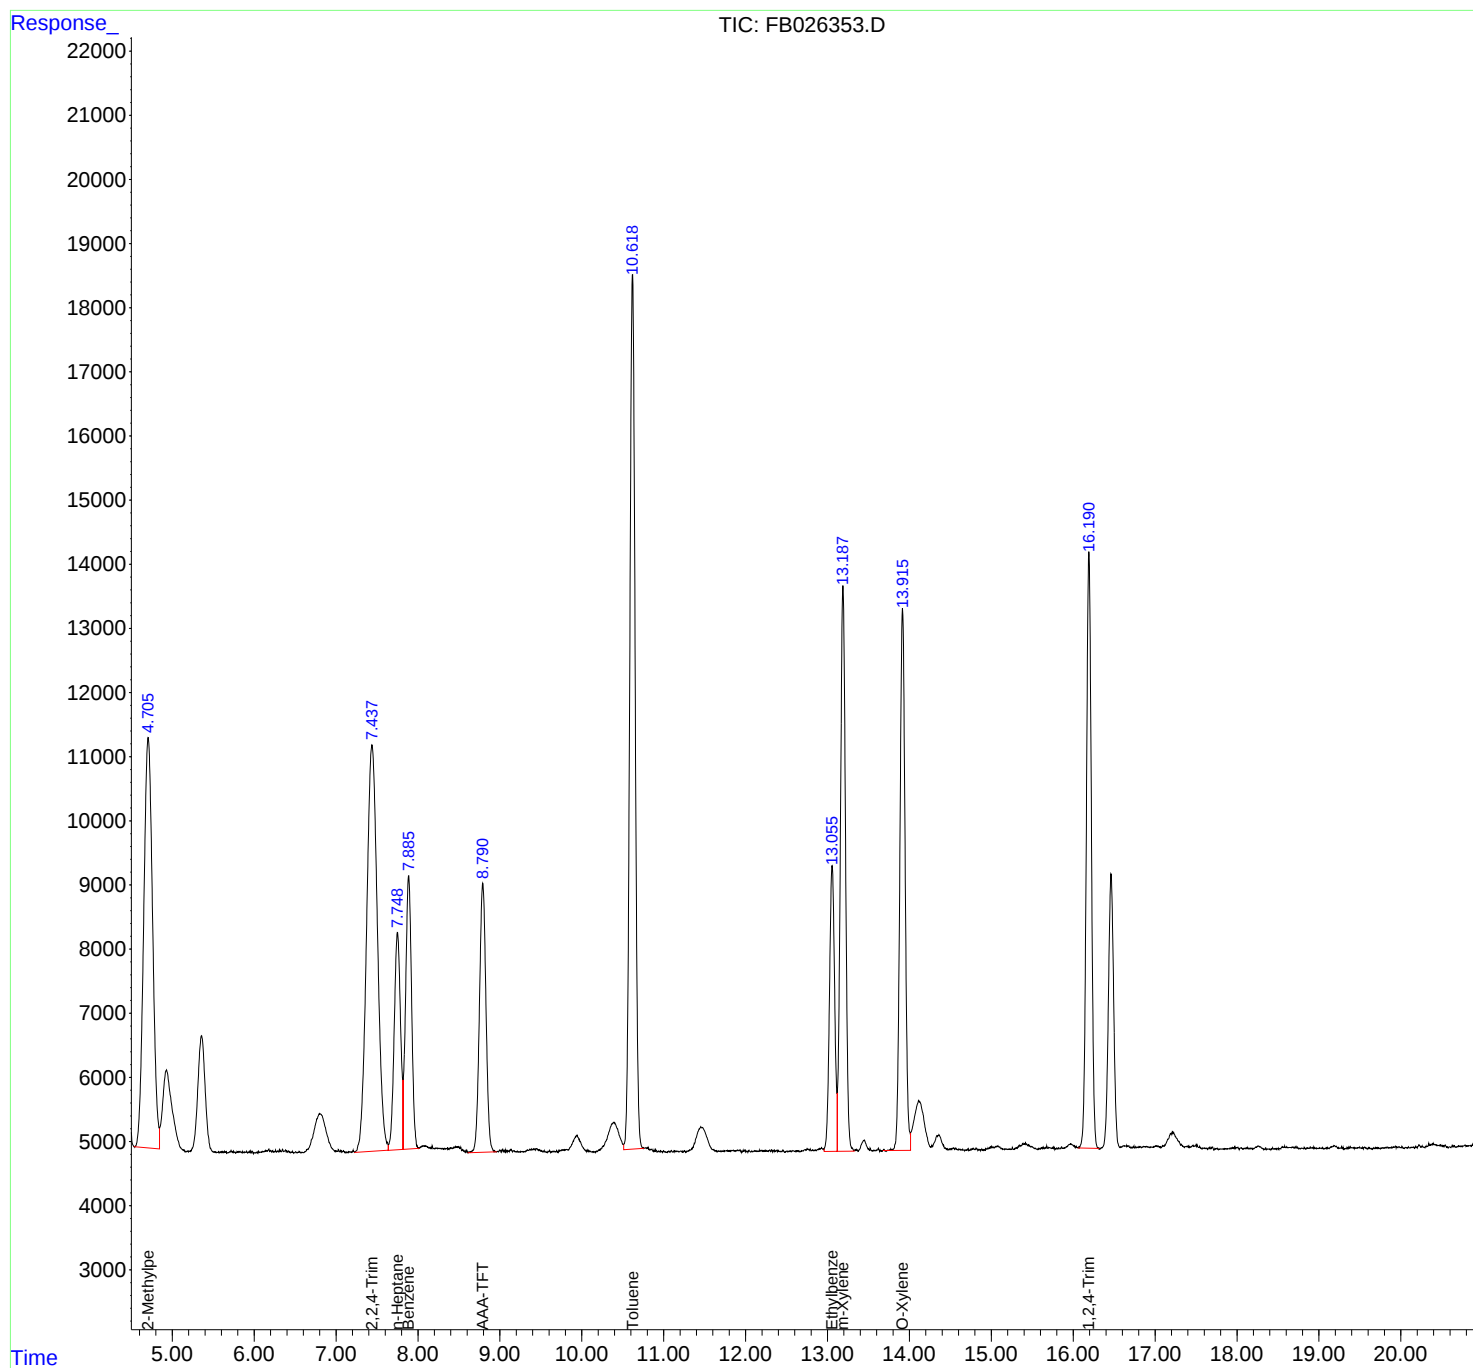

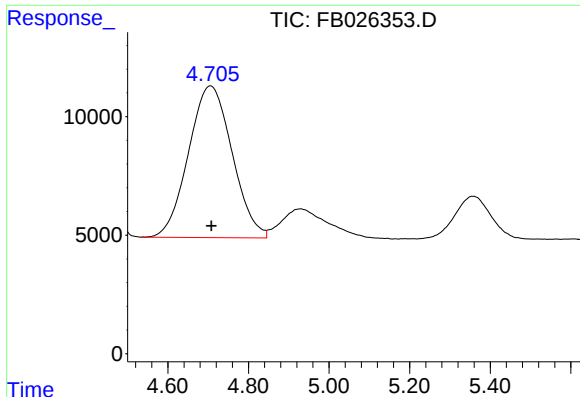


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.002 min
Response: 481301
Conc: 28.91 ng/ml

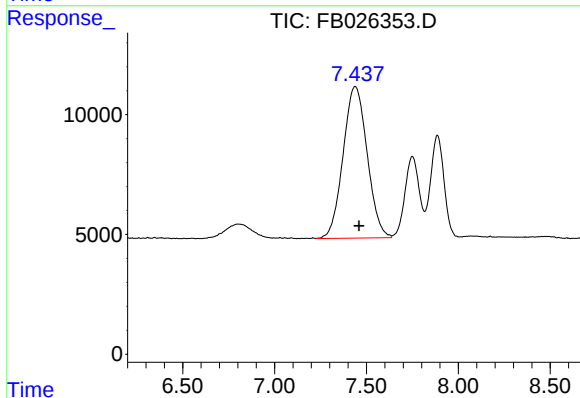


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: -0.021 min
Response: 576344
Conc: 29.56 ng/ml

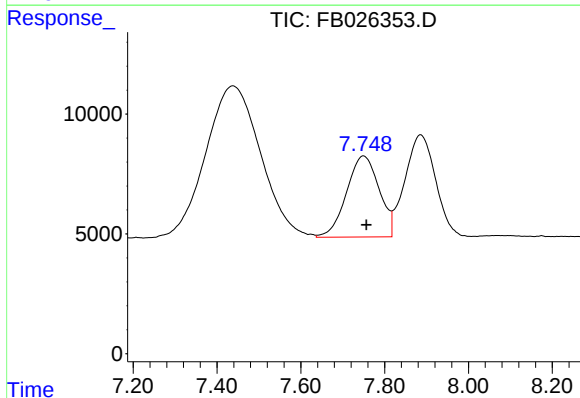


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.007 min
Response: 182973
Conc: 9.92 ng/ml

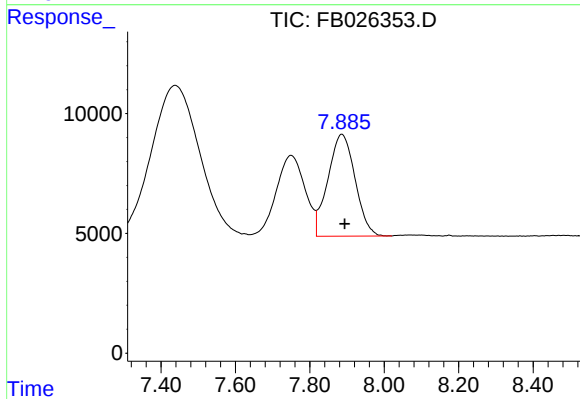


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.007 min
Response: 215967
Conc: 9.91 ng/ml

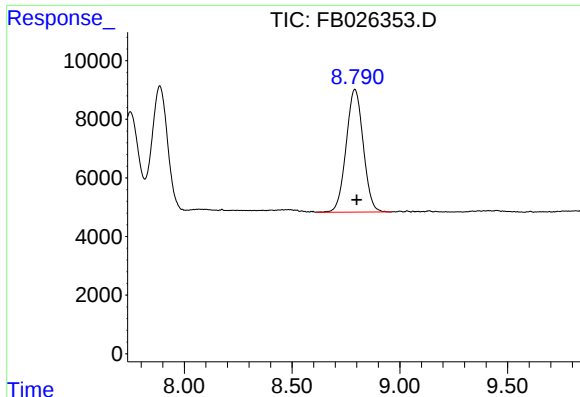


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.009 min
Response: 231327
Conc: 19.53 ng/ml

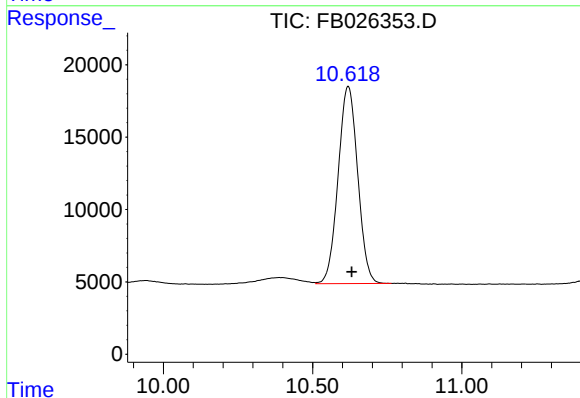


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.011 min
Response: 621295
Conc: 29.96 ng/ml

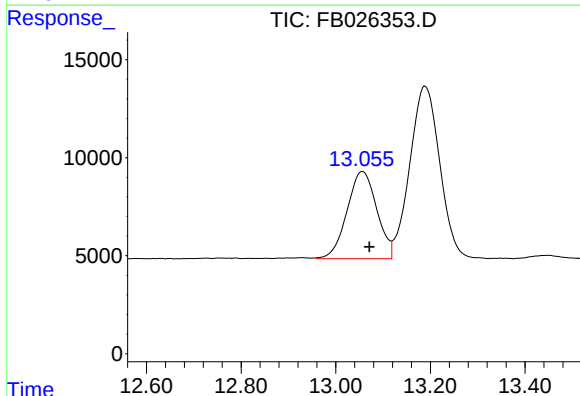


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.015 min
Response: 194520
Conc: 10.30 ng/ml

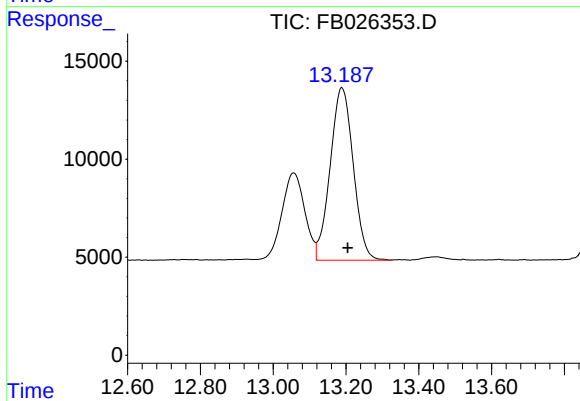


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.015 min
Response: 387290
Conc: 20.36 ng/ml

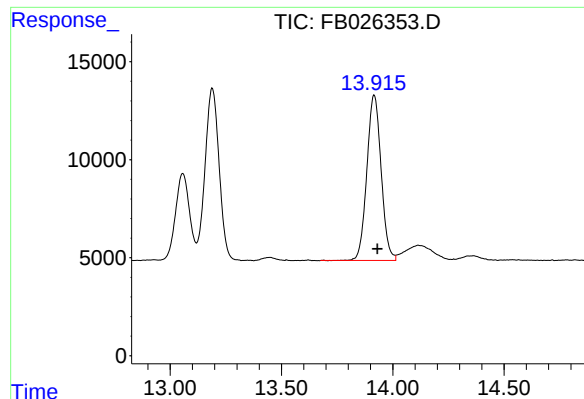

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.015 min
Response: 376256
Conc: 20.37 ng/ml

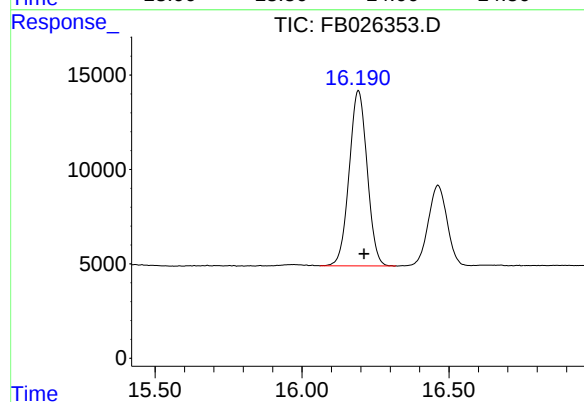

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.019 min
Response: 393943
Conc: 20.78 ng/ml