

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111623\
 Data File : FB030465.D
 Signal(s) : FID2B.CH
 Acq On : 16 Nov 2023 13:50
 Operator : YP/AJ
 Sample : 05449-02
 Misc : 3.16G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 16 23:19:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
 Quant Title :
 QLast Update : Wed Nov 08 11:36:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.782	181781	13.375 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.389	16529	0.834 ng/ml
3) t n-Heptane	7.705	14037	0.621 ng/ml
4) t Benzene	7.881	9201	0.355 ng/ml
6) t Toluene	10.611	27757	1.107 ng/ml
7) t Ethylbenzene	13.036	15644	0.671 ng/ml
8) t m-Xylene	13.176	19436	0.837 ng/ml
9) t O-Xylene	13.906	21163	0.941 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	12670	0.563 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111623\
Data File : FB030465.D
Signal(s) : FID2B.CH
Acq On : 16 Nov 2023 13:50
Operator : YP/AJ
Sample : 05449-02
Misc : 3.16G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 16 23:19:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
Quant Title :
QLast Update : Wed Nov 08 11:36:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

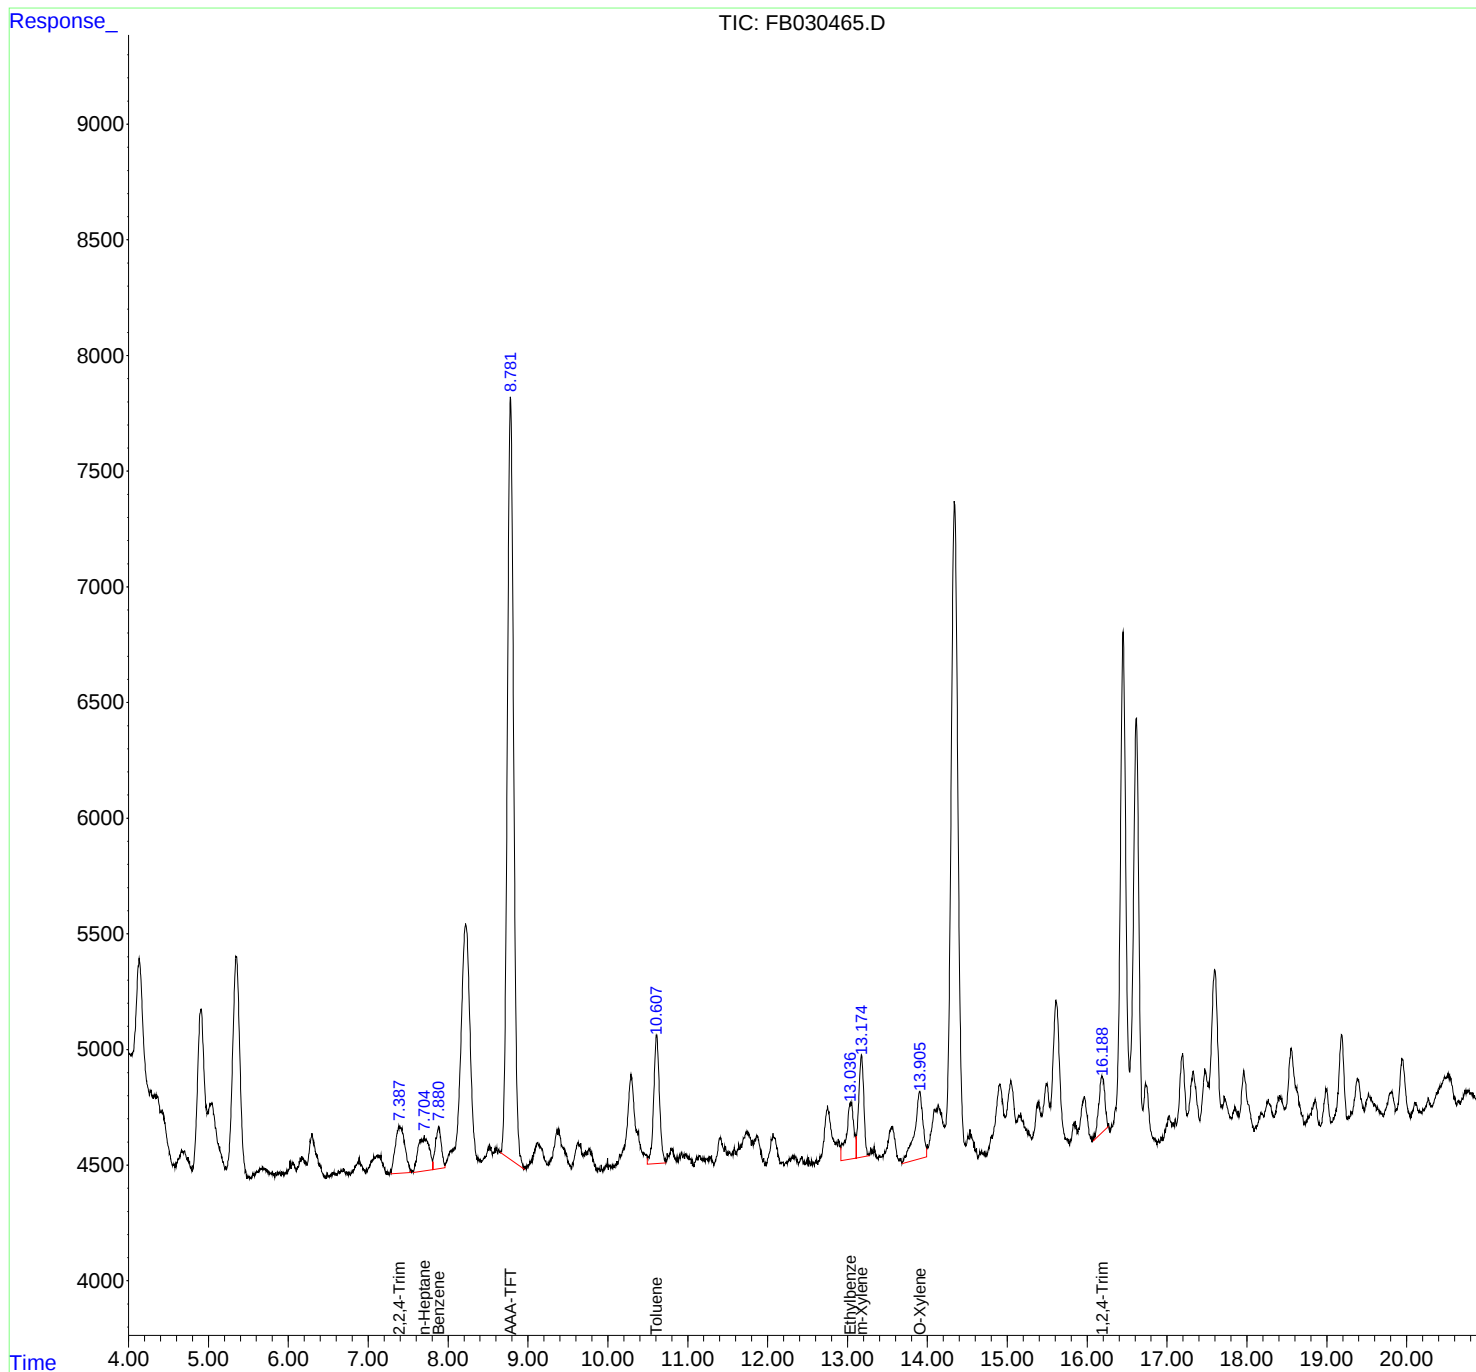

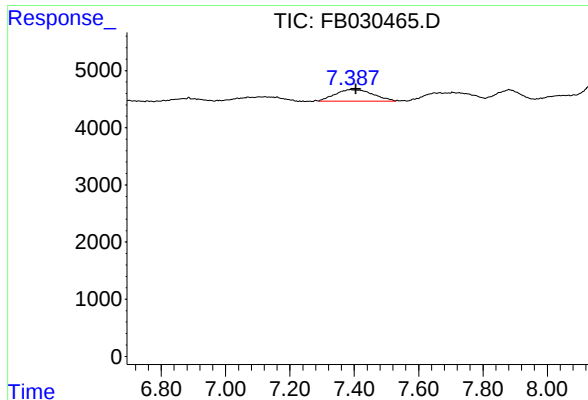


#2 2,2,4-Trimethylpentane

R.T.: 7.389 min
Delta R.T.: -0.016 min
Response: 16529
Conc: 0.83 ng/ml

Instrument :


FID_B

ClientSampleId :

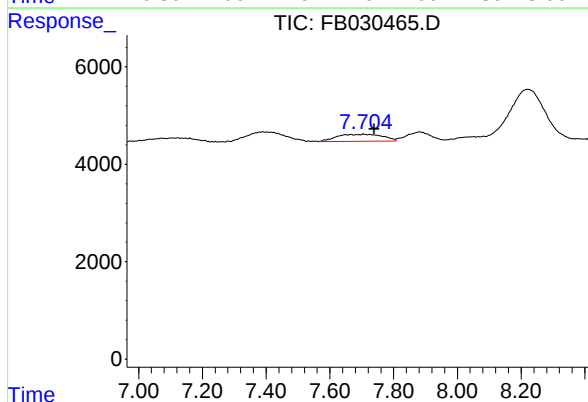


#3 n-Heptane

R.T.: 7.705 min
Delta R.T.: -0.035 min
Response: 14037
Conc: 0.62 ng/ml

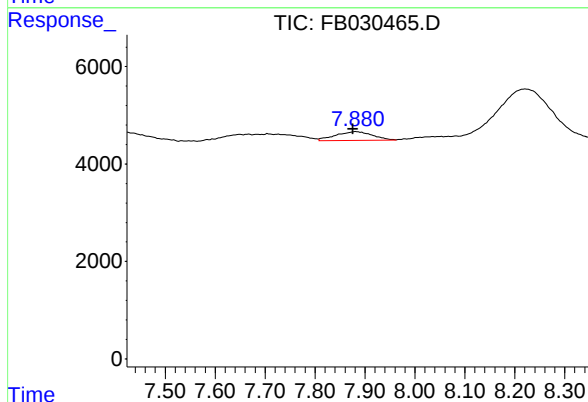


#4 Benzene

R.T.: 7.881 min
Delta R.T.: 0.005 min
Response: 9201
Conc: 0.35 ng/ml

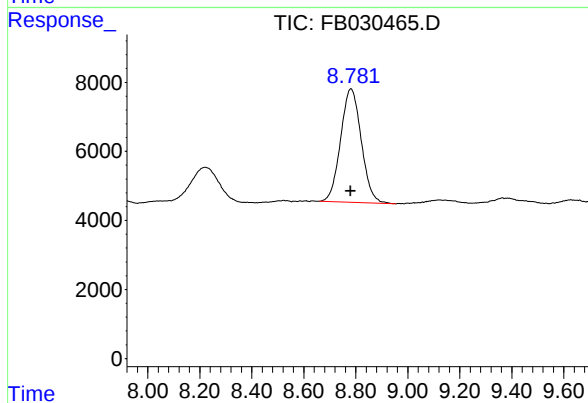

#5 AAA-TFT


R.T.: 8.782 min
Delta R.T.: 0.002 min
Response: 181781
Conc: 13.38 ng/ml

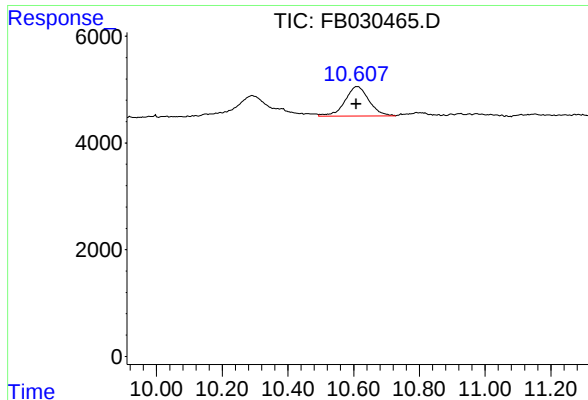

#6 Toluene


R.T.: 10.611 min
Delta R.T.: 0.003 min
Response: 27757
Conc: 1.11 ng/ml

Instrument : FID_B
ClientSampleId :

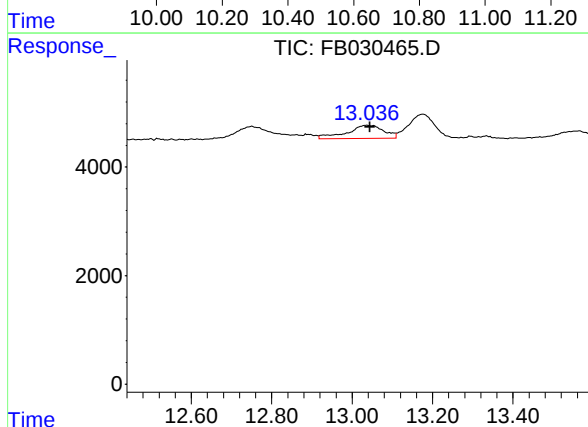


#7 Ethylbenzene

R.T.: 13.036 min
Delta R.T.: -0.008 min
Response: 15644
Conc: 0.67 ng/ml

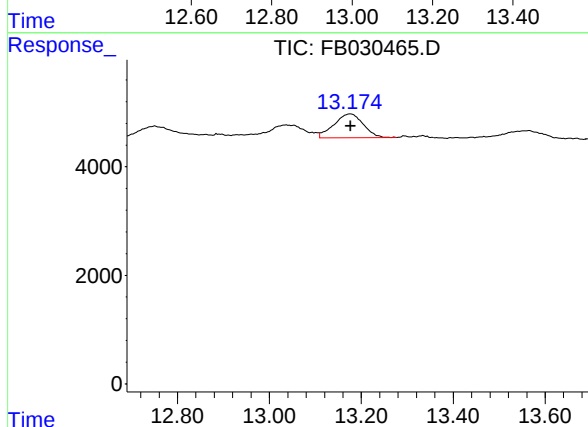


#8 m-Xylene

R.T.: 13.176 min
Delta R.T.: 0.000 min
Response: 19436
Conc: 0.84 ng/ml

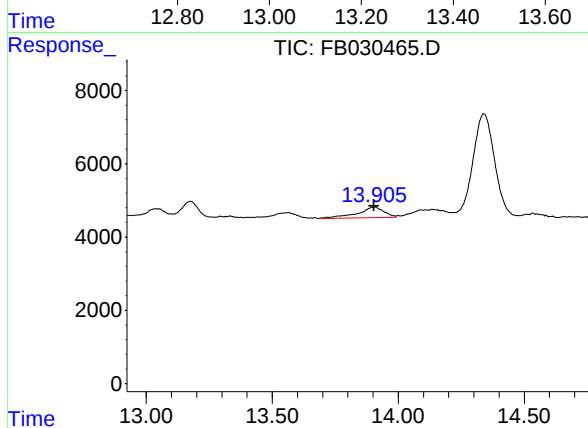

#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: 0.002 min
Response: 21163
Conc: 0.94 ng/ml

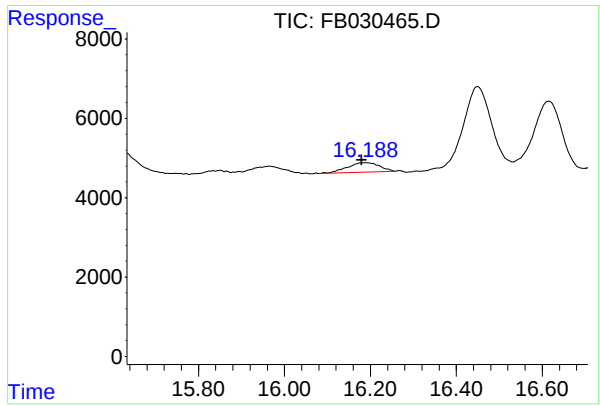

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.011 min
Response: 12670
Conc: 0.56 ng/ml

Instrument :

FID_B

ClientSampleId :