

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111623\
 Data File : FB030475.D
 Signal(s) : FID2B.CH
 Acq On : 16 Nov 2023 20:49
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 17 00:21:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
 Quant Title :
 QLast Update : Wed Nov 08 11:36:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.783	227229	16.719 ng/ml
Target Compounds				
6) t	Toluene	10.610	20379	0.813 ng/ml
7) t	Ethylbenzene	13.051	5491	0.235 ng/ml
8) t	m-Xylene	13.177	23194	0.999 ng/ml
9) t	O-Xylene	13.905	8334	0.370 ng/ml
10) t	1,2,4-Trimethylbenzene	16.182	21590	0.960 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111623\
Data File : FB030475.D
Signal(s) : FID2B.CH
Acq On : 16 Nov 2023 20:49
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 17 00:21:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
Quant Title :
QLast Update : Wed Nov 08 11:36:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

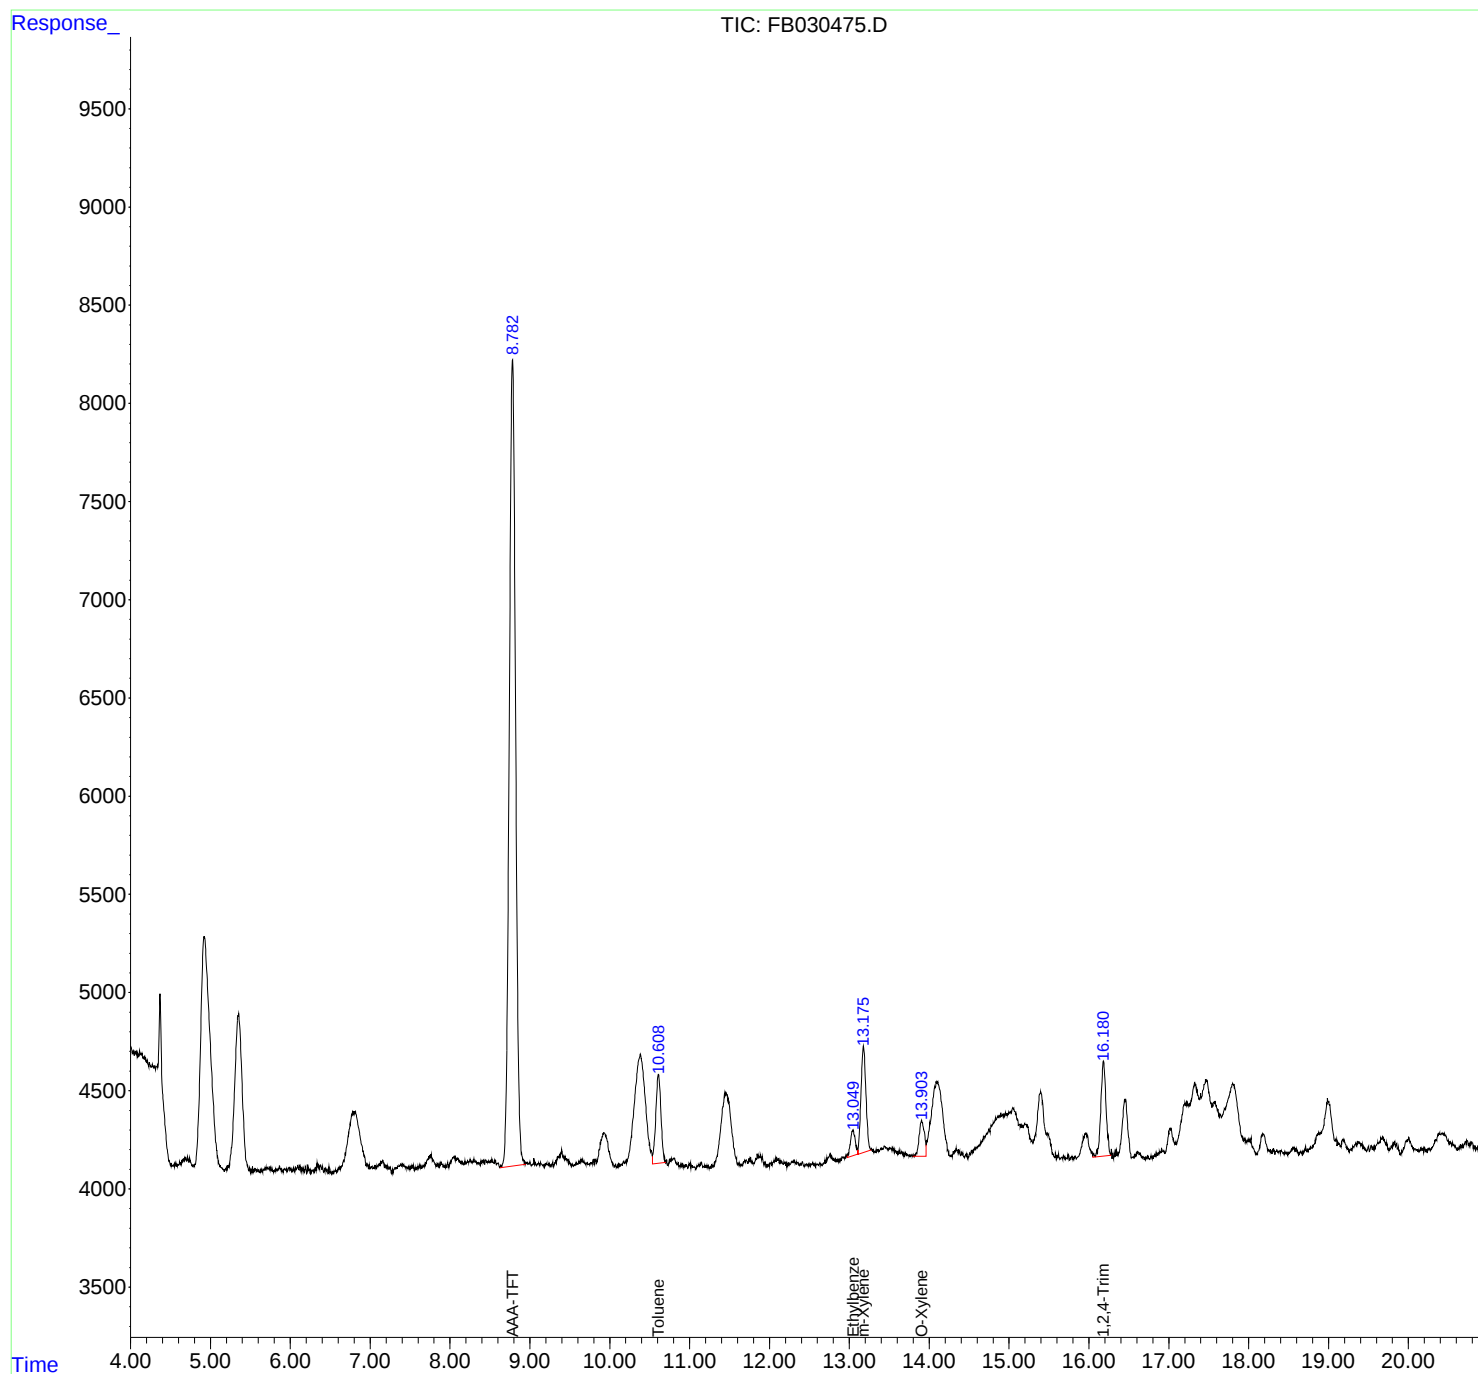


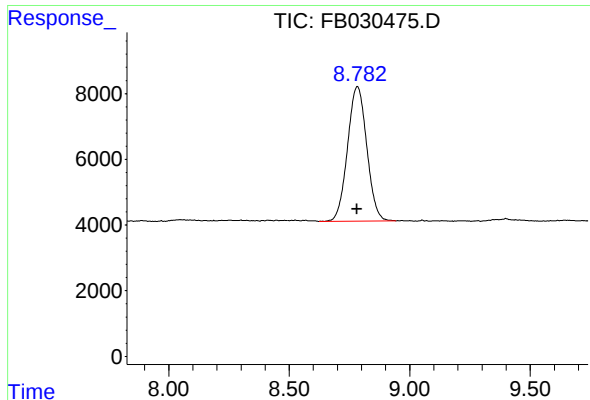

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: 0.003 min
Response: 227229
Conc: 16.72 ng/ml

Instrument :
FID_B
ClientSampleId :

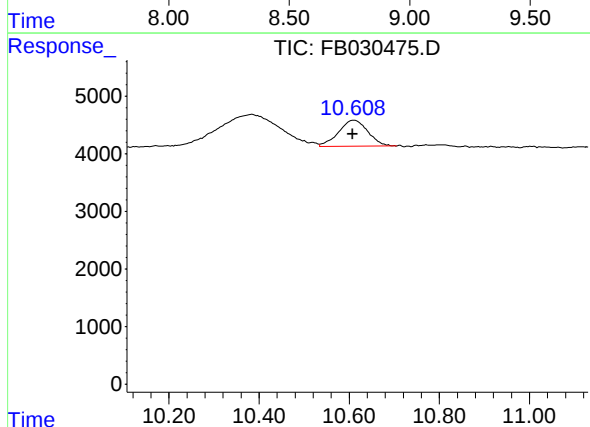


#6 Toluene

R.T.: 10.610 min
Delta R.T.: 0.002 min
Response: 20379
Conc: 0.81 ng/ml

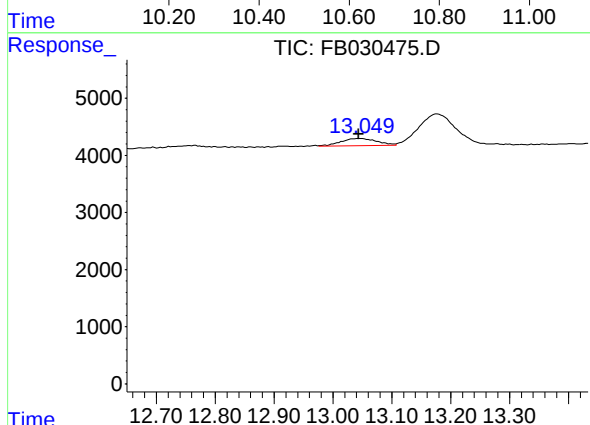


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: 0.007 min
Response: 5491
Conc: 0.24 ng/ml

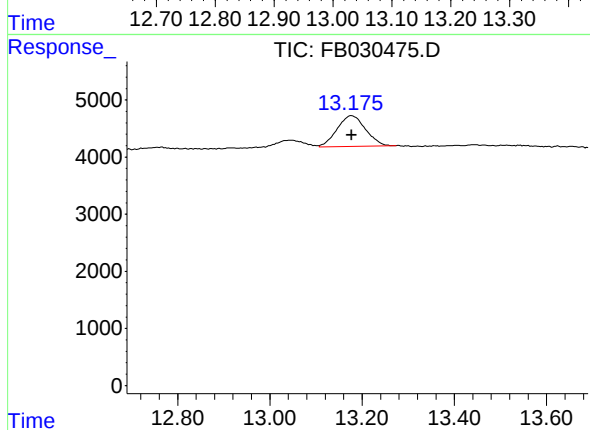

#8 m-Xylene


R.T.: 13.177 min
Delta R.T.: 0.000 min
Response: 23194
Conc: 1.00 ng/ml

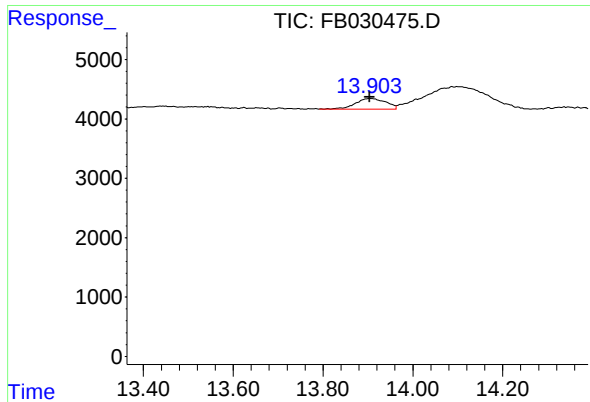

#9 O-Xylene

R.T.: 13.905 min
Delta R.T.: 0.000 min
Response: 8334
Conc: 0.37 ng/ml

Instrument :
FID_B
ClientSampleId :

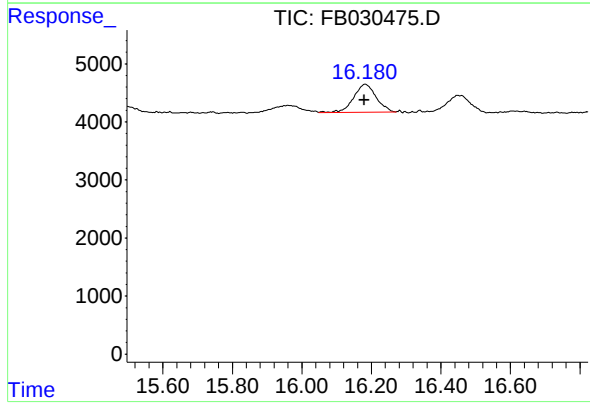

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: 0.003 min
Response: 21590
Conc: 0.96 ng/ml