

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111623\
 Data File : FB030469.D
 Signal(s) : FID2B.CH
 Acq On : 16 Nov 2023 16:22
 Operator : YP/AJ
 Sample : BSF1116S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1116S2

Integration File: Calibration.e
 Quant Time: Nov 16 23:20:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
 Quant Title :
 QLast Update : Wed Nov 08 11:36:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.782	295765	21.762 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.702	657994	33.001 ng/ml
2) t	2,2,4-Trimethylpentane	7.406	670935	33.862 ng/ml
3) t	n-Heptane	7.741	252884	11.191 ng/ml
4) t	Benzene	7.877	293691	11.316 ng/ml
6) t	Toluene	10.609	858868	34.266 ng/ml
7) t	Ethylbenzene	13.046	262459	11.254 ng/ml
8) t	m-Xylene	13.179	523527	22.556 ng/ml
9) t	O-Xylene	13.905	505543	22.467 ng/ml
10) t	1,2,4-Trimethylbenzene	16.180	513859	22.840 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111623\
Data File : FB030469.D
Signal(s) : FID2B.CH
Acq On : 16 Nov 2023 16:22
Operator : YP/AJ
Sample : BSF1116S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1116S2

Integration File: Calibration.e
Quant Time: Nov 16 23:20:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110823.M
Quant Title :
QLast Update : Wed Nov 08 11:36:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

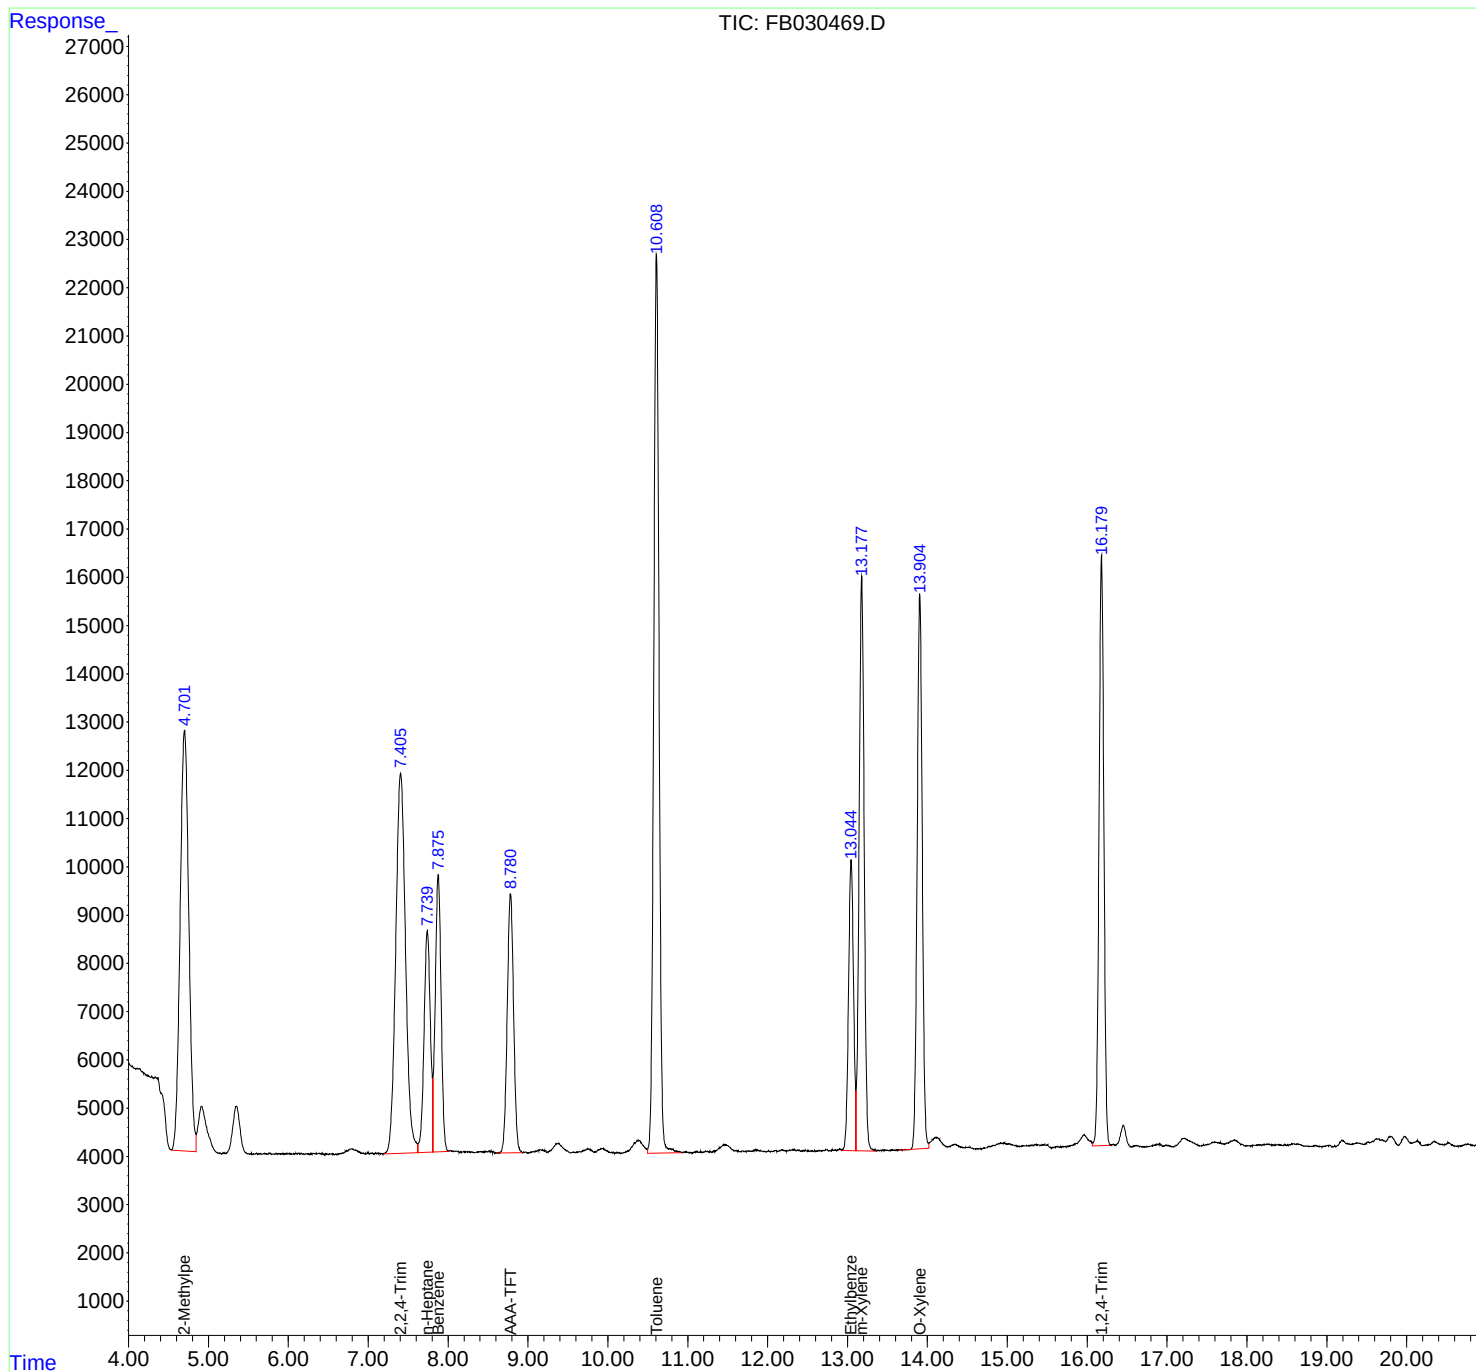


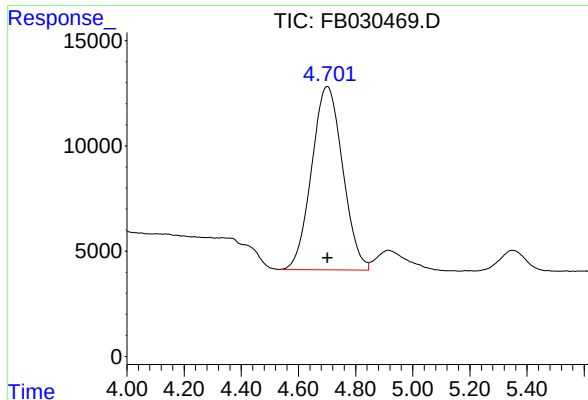

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 657994
Conc: 33.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1116S2

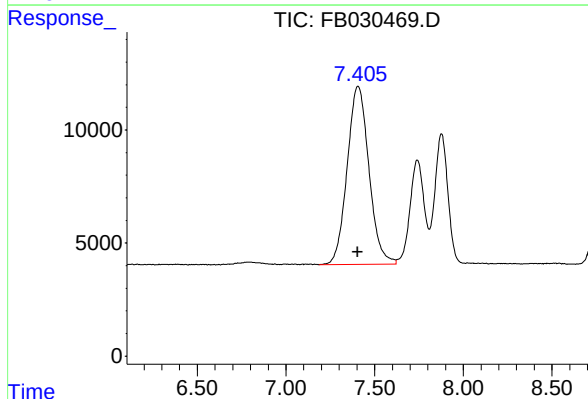


#2 2,2,4-Trimethylpentane

R.T.: 7.406 min
Delta R.T.: 0.002 min
Response: 670935
Conc: 33.86 ng/ml

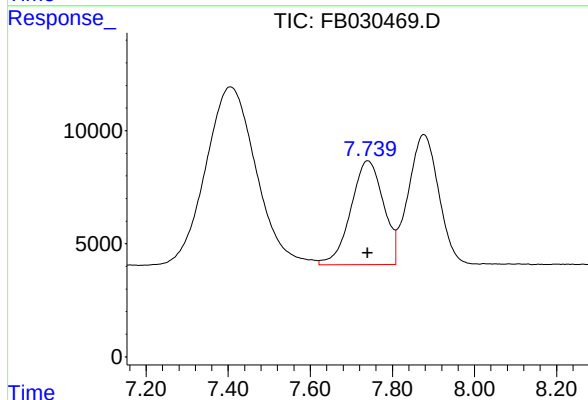


#3 n-Heptane

R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 252884
Conc: 11.19 ng/ml

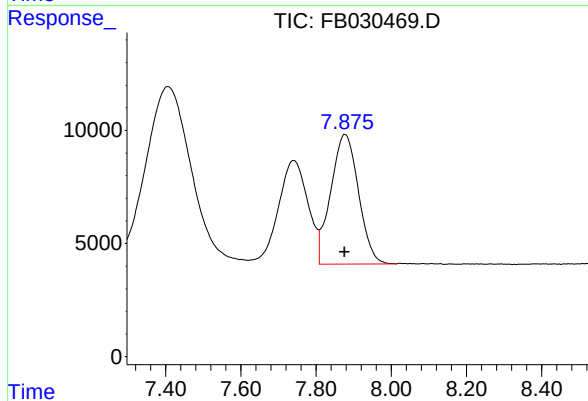

#4 Benzene


R.T.: 7.877 min
Delta R.T.: 0.000 min
Response: 293691
Conc: 11.32 ng/ml

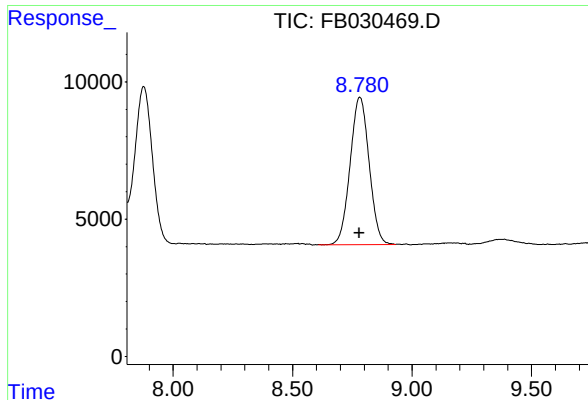

#5 AAA-TFT


R.T.: 8.782 min
Delta R.T.: 0.001 min
Response: 295765
Conc: 21.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1116S2

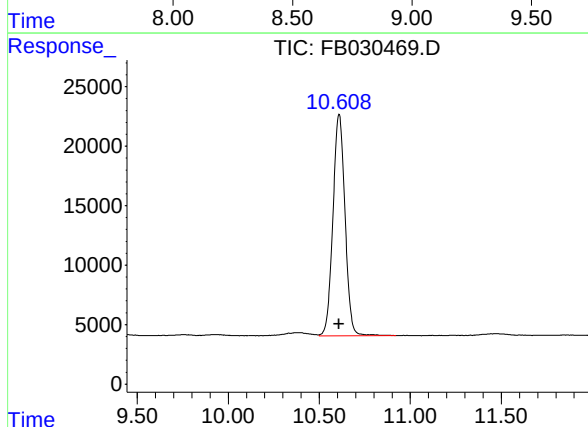


#6 Toluene

R.T.: 10.609 min
Delta R.T.: 0.001 min
Response: 858868
Conc: 34.27 ng/ml

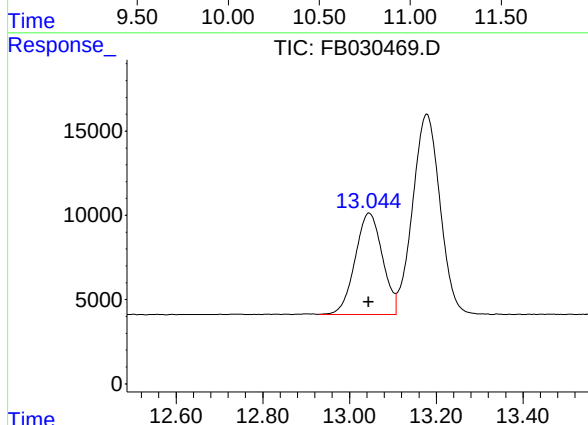


#7 Ethylbenzene

R.T.: 13.046 min
Delta R.T.: 0.002 min
Response: 262459
Conc: 11.25 ng/ml

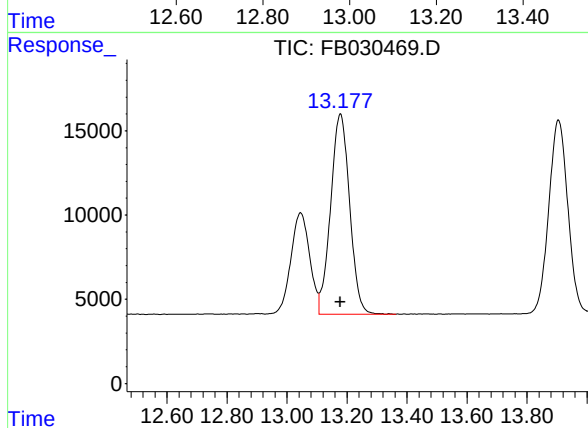

#8 m-Xylene


R.T.: 13.179 min
Delta R.T.: 0.001 min
Response: 523527
Conc: 22.56 ng/ml

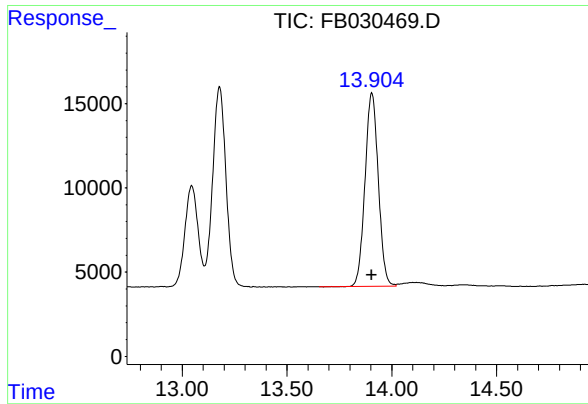

#9 O-Xylene

R.T.: 13.905 min
Delta R.T.: 0.001 min
Response: 505543
Conc: 22.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1116S2

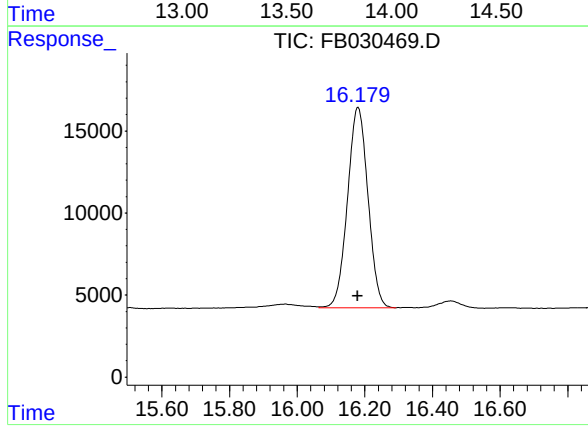

#10 1,2,4-Trimethylbenzene

R.T.: 16.180 min
Delta R.T.: 0.001 min
Response: 513859
Conc: 22.84 ng/ml