

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111721\
 Data File : FB026363.D
 Signal(s) : FID2B.CH
 Acq On : 17 Nov 2021 17:03
 Operator : AJ/MA
 Sample : VBF1117S2
 Misc : 5.00G\5.00ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 18 08:48:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	217464	18.356 ng/ml
Target Compounds			
6) t Toluene	10.620	5810	0.280 ng/ml
8) t m-Xylene	13.188	6372	0.335 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	7122	0.376 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111721\
Data File : FB026363.D
Signal(s) : FID2B.CH
Acq On : 17 Nov 2021 17:03
Operator : AJ/MA
Sample : VBF1117S2
Misc : 5.00G\5.00ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 18 08:48:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

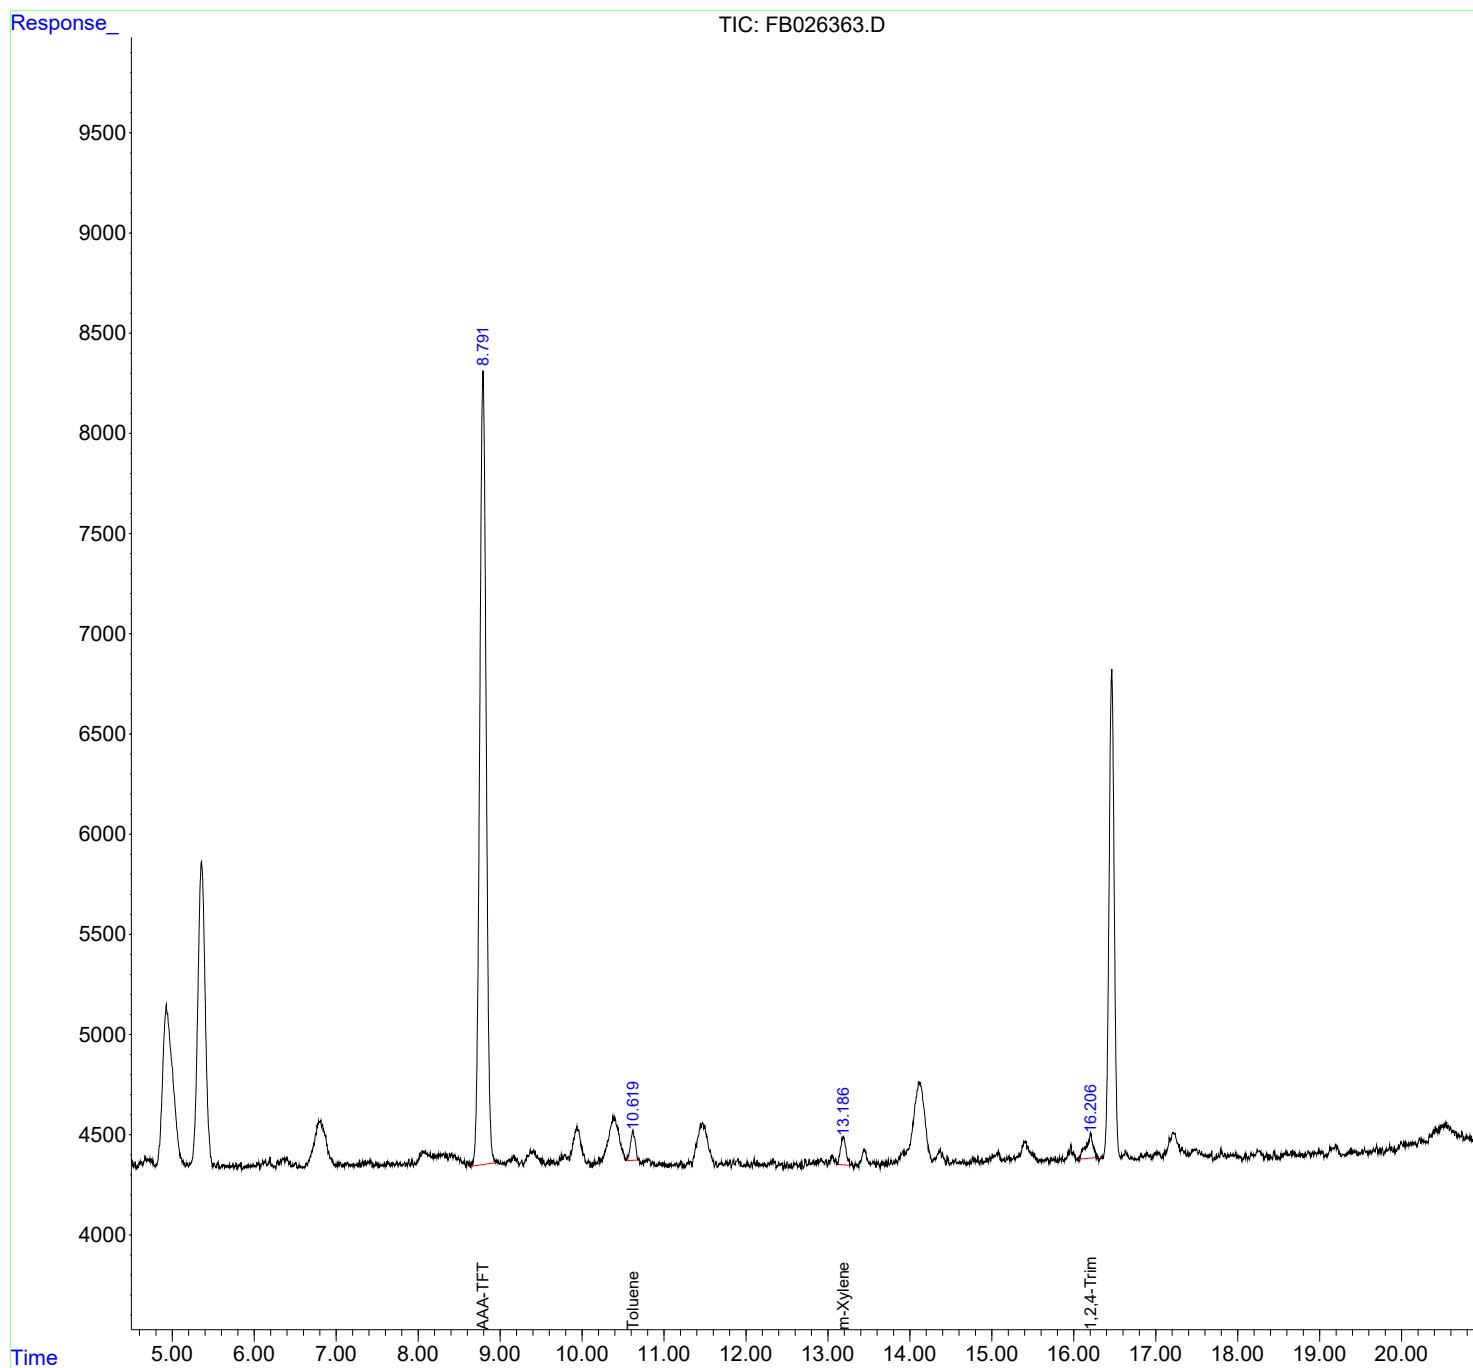


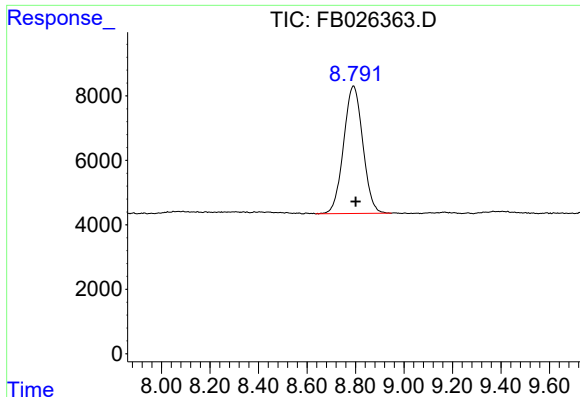

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.008 min
Response: 217464
Conc: 18.36 ng/ml

Instrument :
FID_B
ClientSampleId :

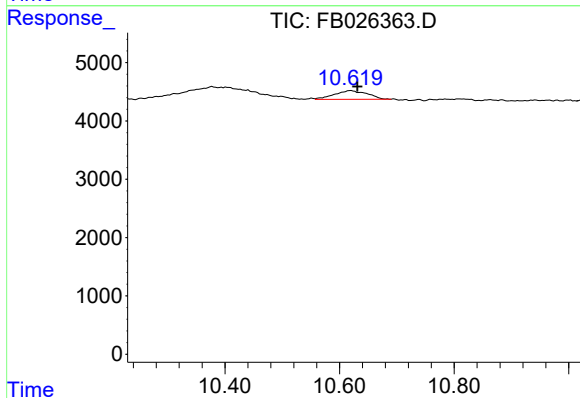


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.011 min
Response: 5810
Conc: 0.28 ng/ml

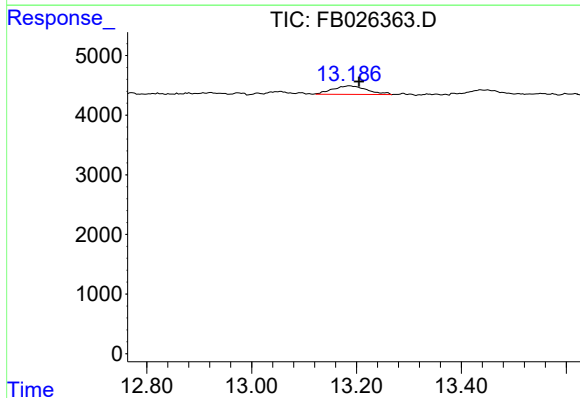

#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: -0.017 min
Response: 6372
Conc: 0.34 ng/ml

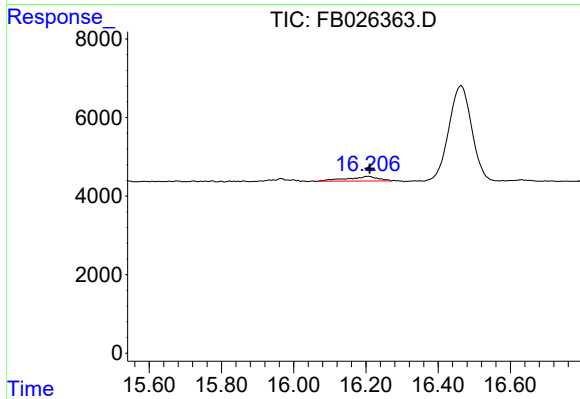

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 7122
Conc: 0.38 ng/ml