

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111721\
 Data File : FB026368.D
 Signal(s) : FID2B.CH
 Acq On : 17 Nov 2021 20:04
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 18 08:49:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	238316	20.116 ng/ml
Target Compounds			
6) t Toluene	10.620	10402	0.502 ng/ml
8) t m-Xylene	13.189	13383	0.704 ng/ml
9) t O-Xylene	13.913	5375	0.291 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	10965	0.578 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111721\
Data File : FB026368.D
Signal(s) : FID2B.CH
Acq On : 17 Nov 2021 20:04
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 18 08:49:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

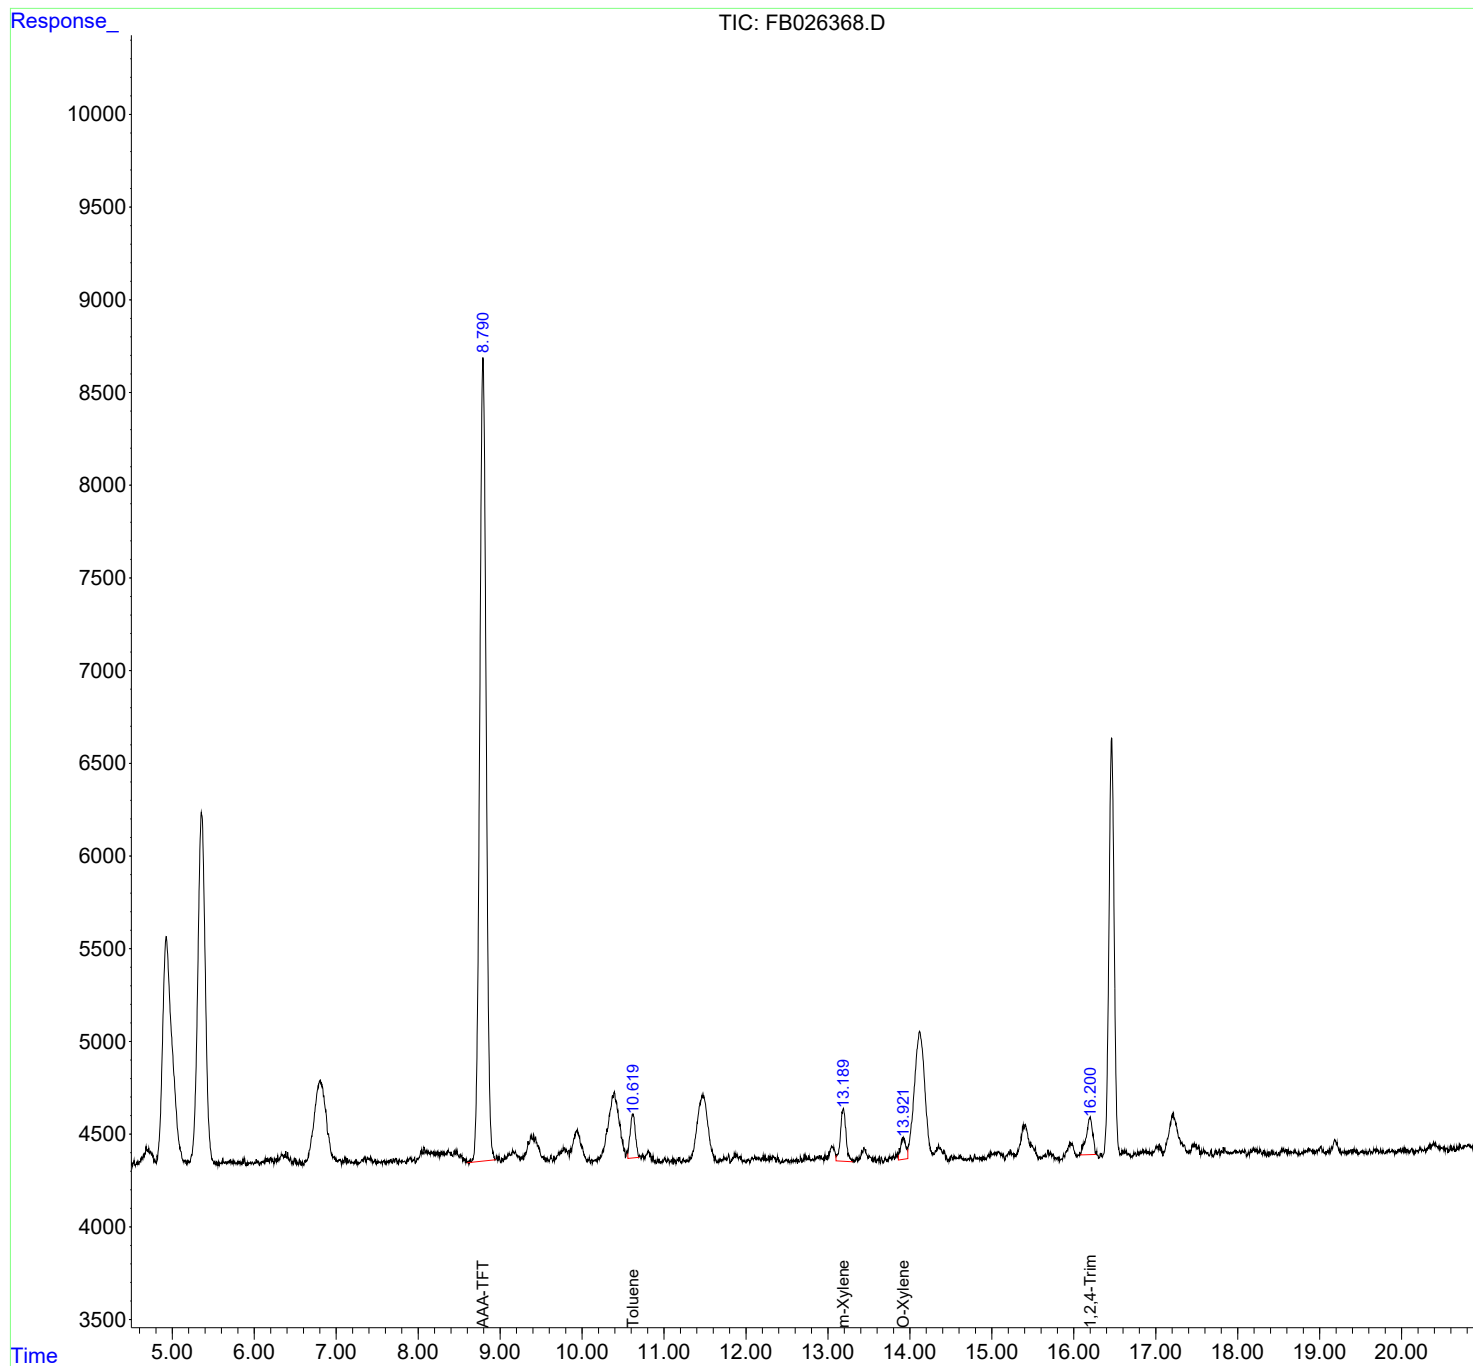


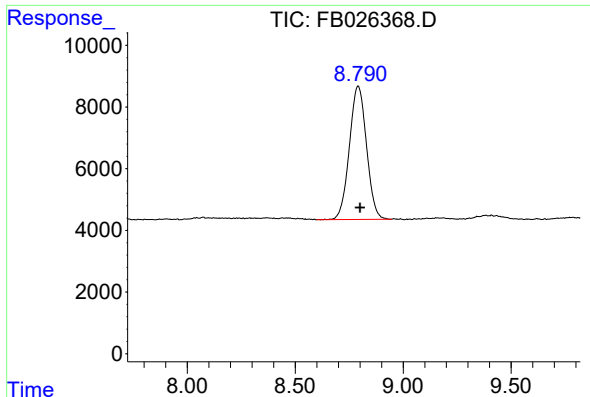

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.008 min
Response: 238316
Conc: 20.12 ng/ml

Instrument :
FID_B
ClientSampleId :

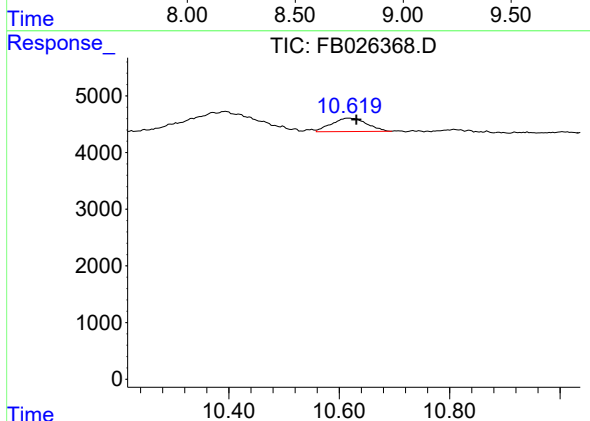


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.011 min
Response: 10402
Conc: 0.50 ng/ml

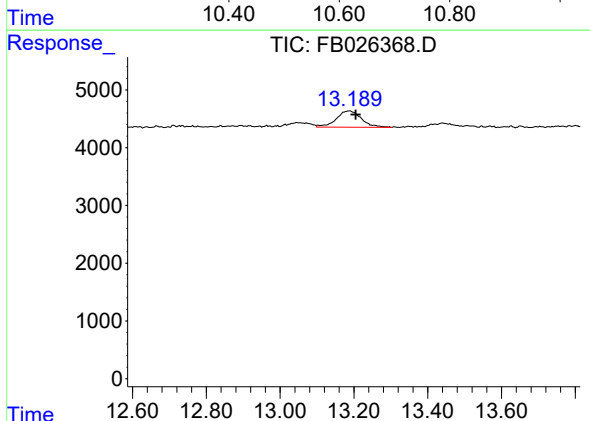


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.016 min
Response: 13383
Conc: 0.70 ng/ml

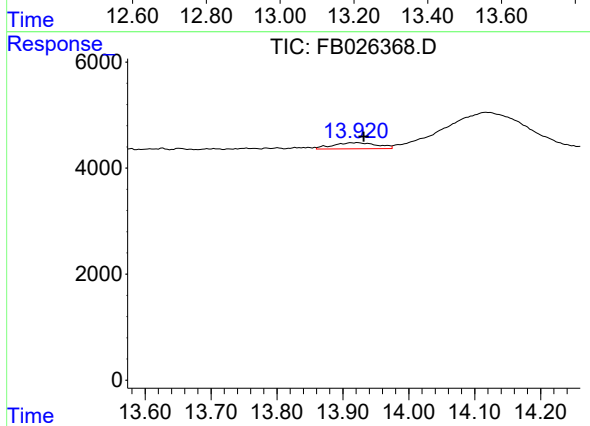

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.018 min
Response: 5375
Conc: 0.29 ng/ml

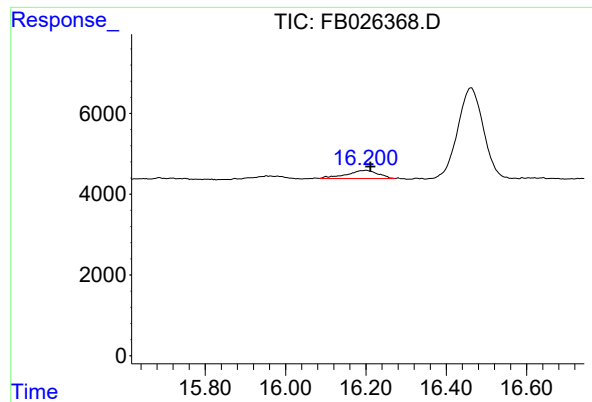

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: -0.010 min
Response: 10965
Conc: 0.58 ng/ml

Instrument :

FID_B

ClientSampleId :