

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111721\
 Data File : FB026357.D
 Signal(s) : FID2B.CH
 Acq On : 17 Nov 2021 12:41
 Operator : AJ/MA
 Sample : BSF1117S1
 Misc : 5.01G\5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1117S1

Integration File: Calibration.e
 Quant Time: Nov 18 08:48:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	241693	20.401 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	471584	28.322 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	564967	28.974 ng/ml
3) t n-Heptane	7.747	174787	9.473 ng/ml
4) t Benzene	7.885	207686	9.526 ng/ml
6) t Toluene	10.618	601581	29.005 ng/ml
7) t Ethylbenzene	13.055	188414	9.977 ng/ml
8) t m-Xylene	13.188	376751	19.808 ng/ml
9) t O-Xylene	13.915	369277	19.994 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	380426	20.067 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111721\
Data File : FB026357.D
Signal(s) : FID2B.CH
Acq On : 17 Nov 2021 12:41
Operator : AJ/MA
Sample : BSF1117S1
Misc : 5.01G\5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1117S1

Integration File: Calibration.e
Quant Time: Nov 18 08:48:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

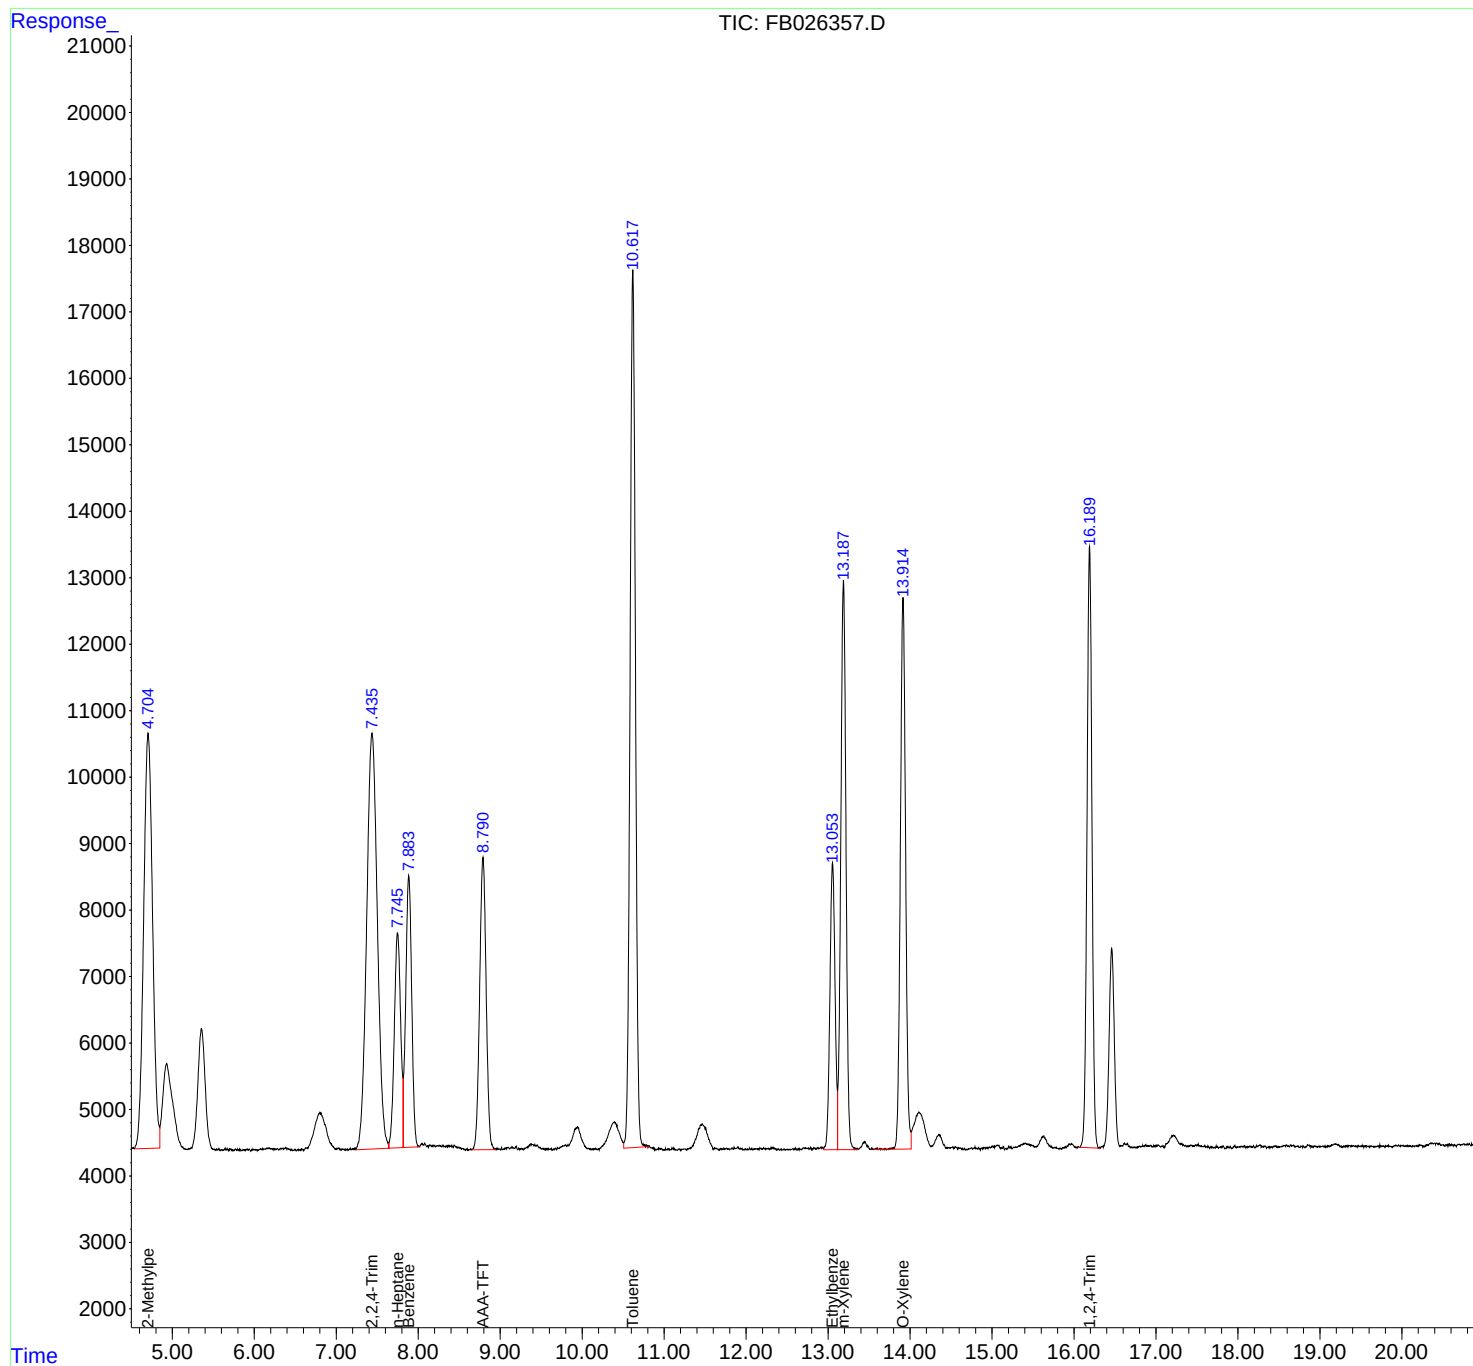


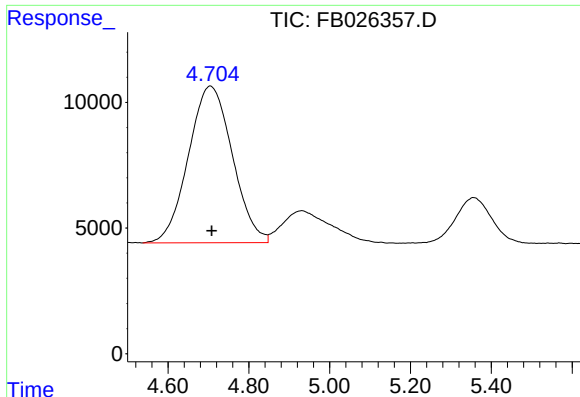

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.003 min
Response: 471584
Conc: 28.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1117S1

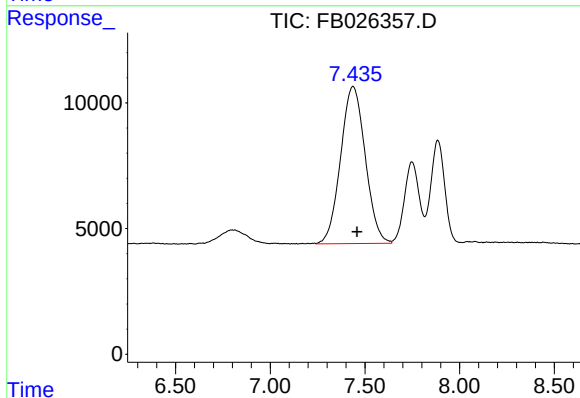


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: -0.023 min
Response: 564967
Conc: 28.97 ng/ml

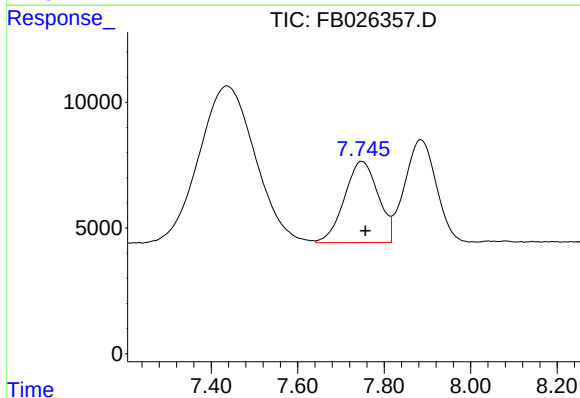


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.010 min
Response: 174787
Conc: 9.47 ng/ml

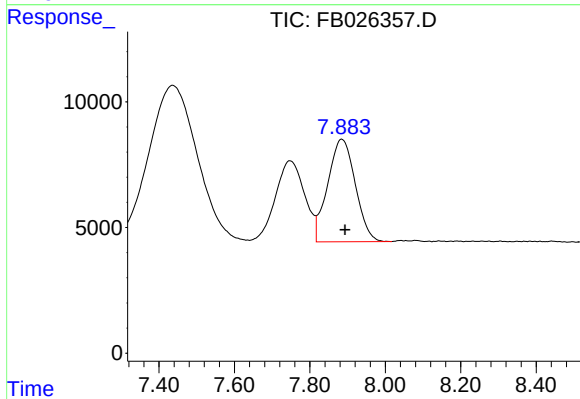

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.008 min
Response: 207686
Conc: 9.53 ng/ml

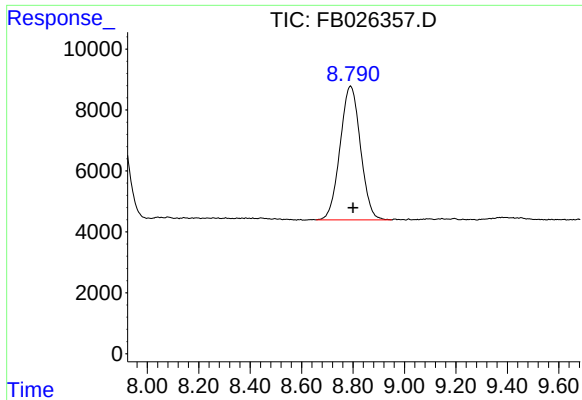

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.009 min
Response: 241693
Conc: 20.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1117S1

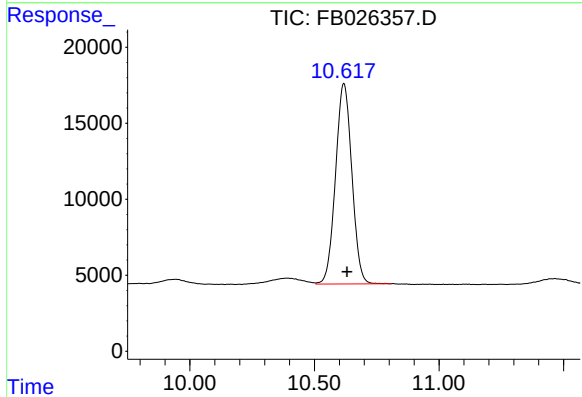


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.013 min
Response: 601581
Conc: 29.00 ng/ml

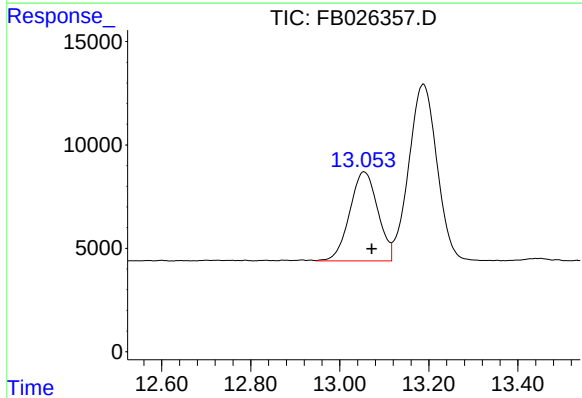


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.017 min
Response: 188414
Conc: 9.98 ng/ml

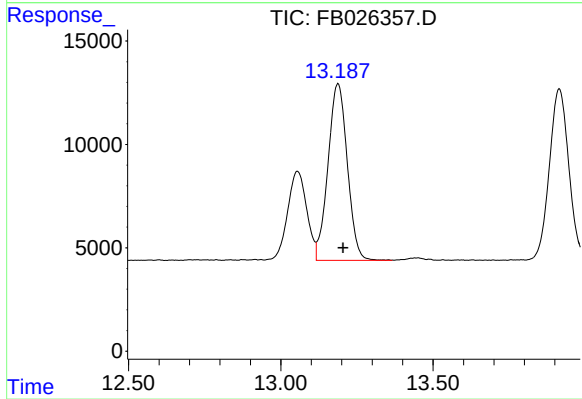

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.017 min
Response: 376751
Conc: 19.81 ng/ml

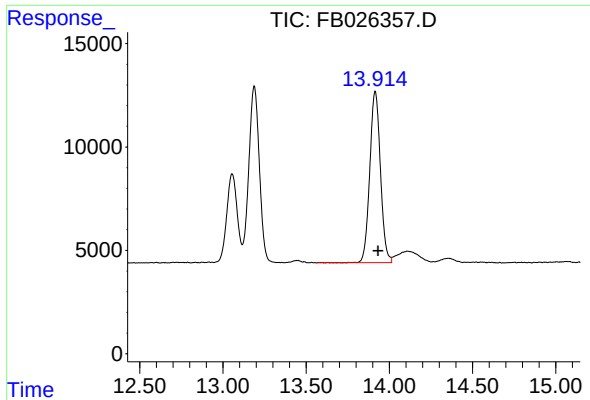

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.017 min
Response: 369277
Conc: 19.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1117S1

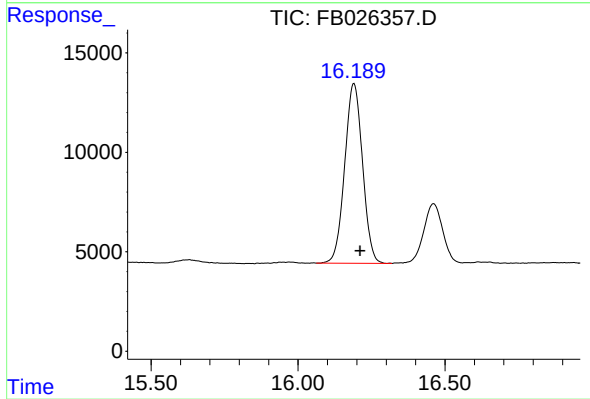

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.021 min
Response: 380426
Conc: 20.07 ng/ml