

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111722\
 Data File : FB029051.D
 Signal(s) : FID2B.CH
 Acq On : 17 Nov 2022 12:32
 Operator : AJ/MA
 Sample : N5598-12MS
 Misc : 1.44G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 18 04:46:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	278410	21.909 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	429652	26.359 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	503940	28.680 ng/ml
3) t n-Heptane	7.745	164147	9.336 ng/ml
4) t Benzene	7.880	232390	11.333 ng/ml
6) t Toluene	10.615	665791	33.102 ng/ml
7) t Ethylbenzene	13.052	209223	11.032 ng/ml
8) t m-Xylene	13.185	407834	21.678 ng/ml
9) t O-Xylene	13.913	394384	21.498 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	370510	20.112 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111722\
Data File : FB029051.D
Signal(s) : FID2B.CH
Acq On : 17 Nov 2022 12:32
Operator : AJ/MA
Sample : N5598-12MS
Misc : 1.44G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 18 04:46:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

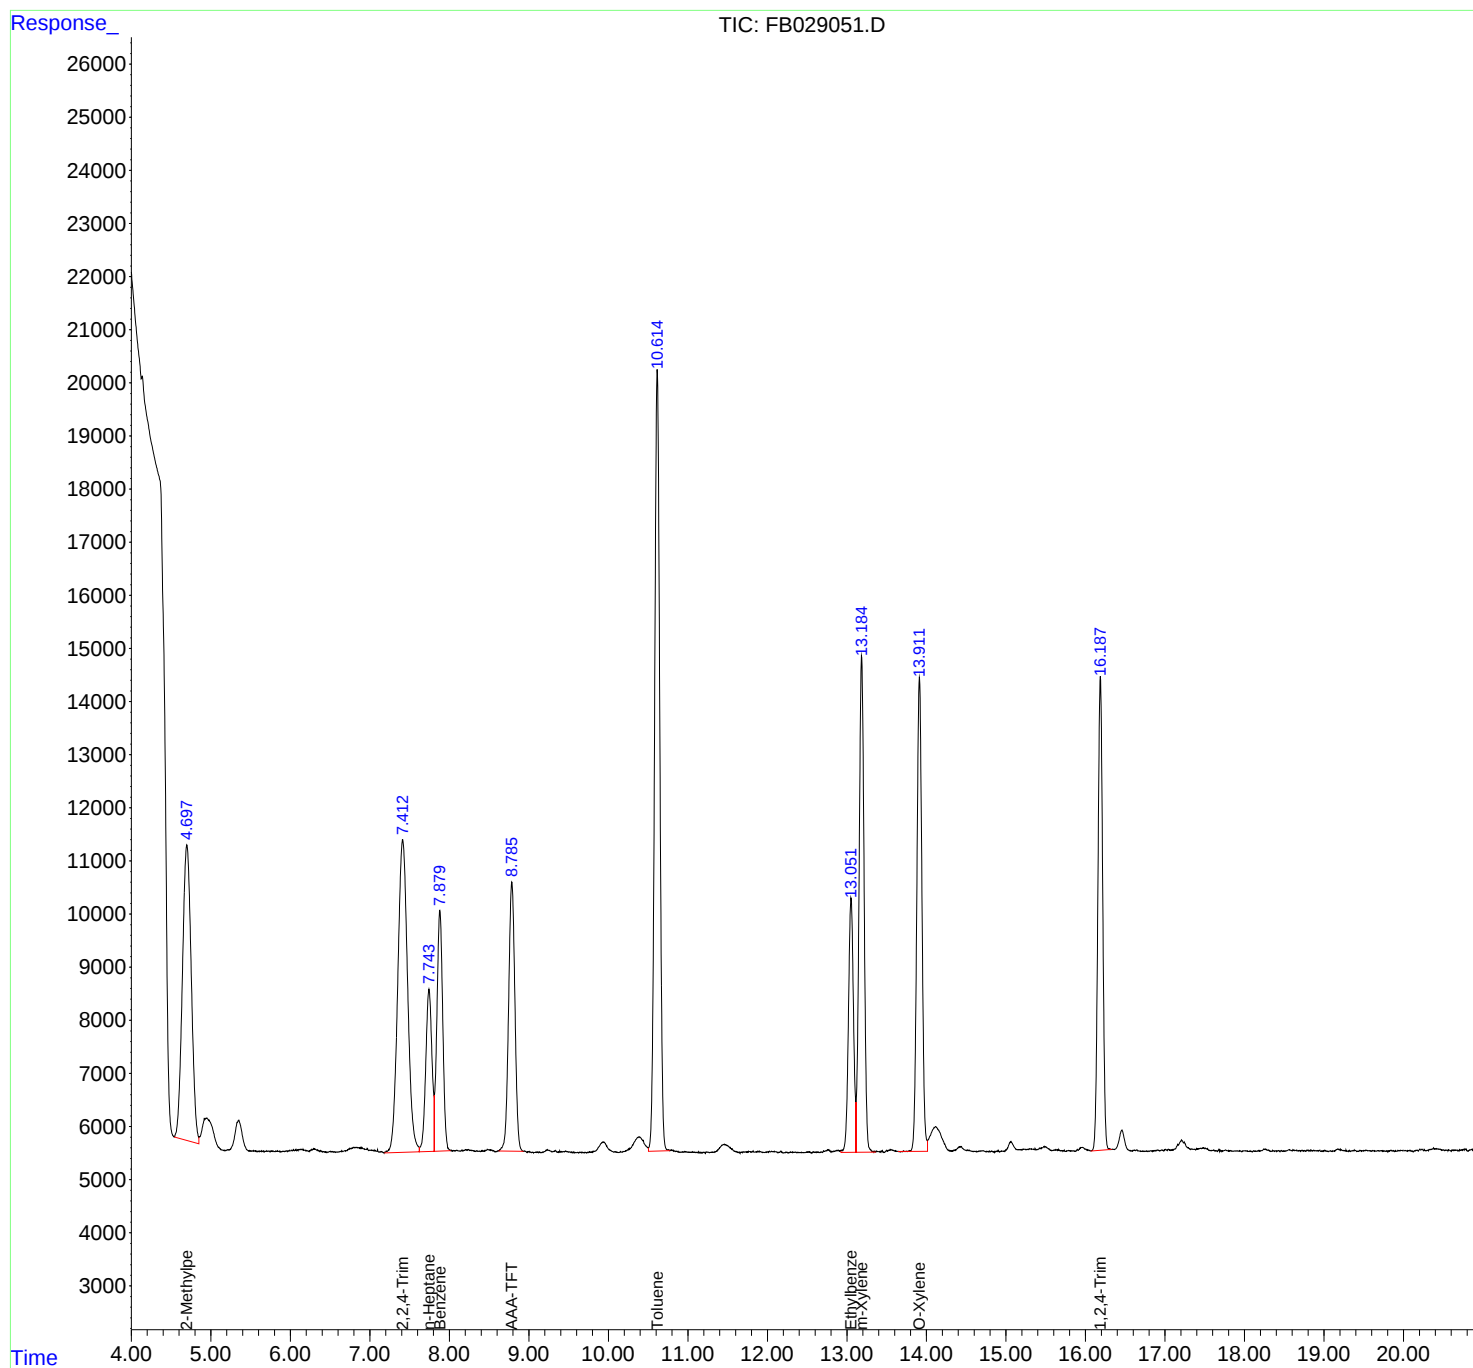


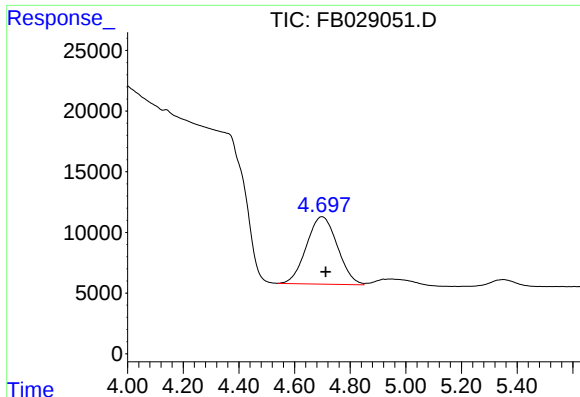

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.013 min
Response: 429652
Conc: 26.36 ng/ml

Instrument :
FID_B
ClientSampleId :

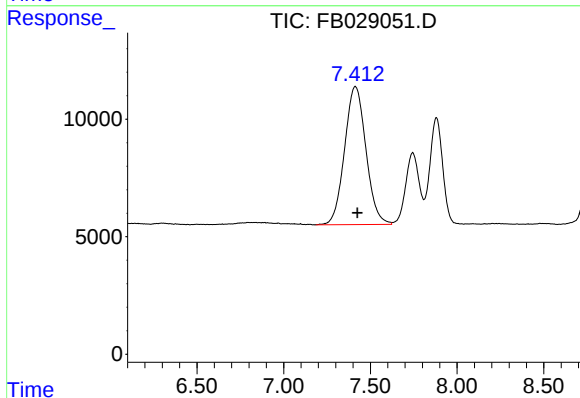


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.011 min
Response: 503940
Conc: 28.68 ng/ml

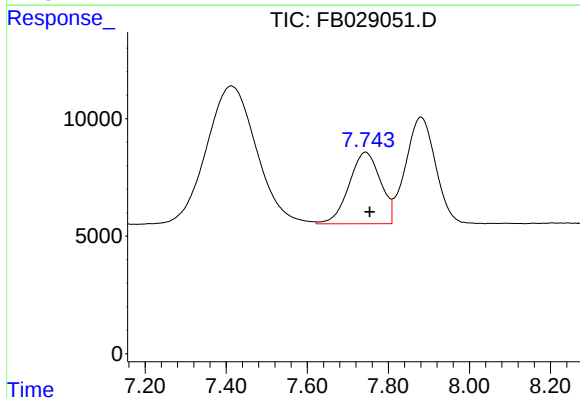


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.010 min
Response: 164147
Conc: 9.34 ng/ml

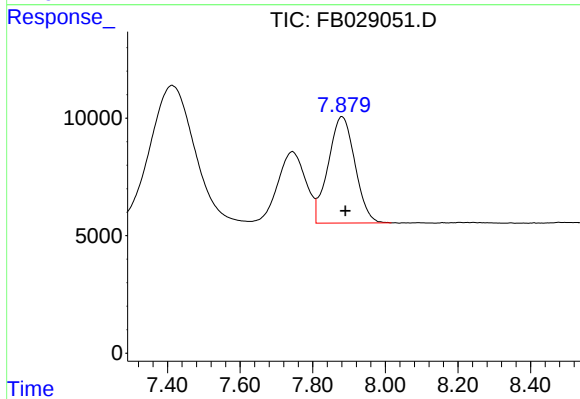

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.010 min
Response: 232390
Conc: 11.33 ng/ml

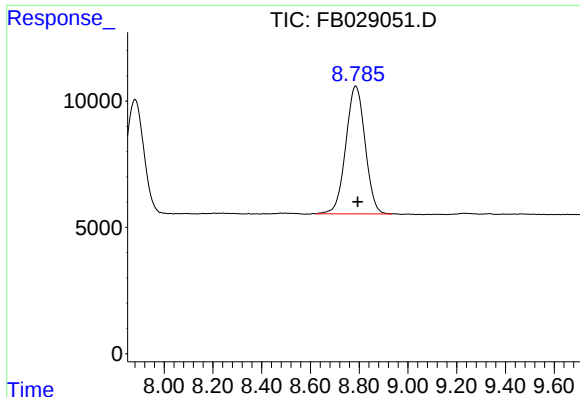

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.009 min
Response: 278410
Conc: 21.91 ng/ml

Instrument :
FID_B
ClientSampleId :

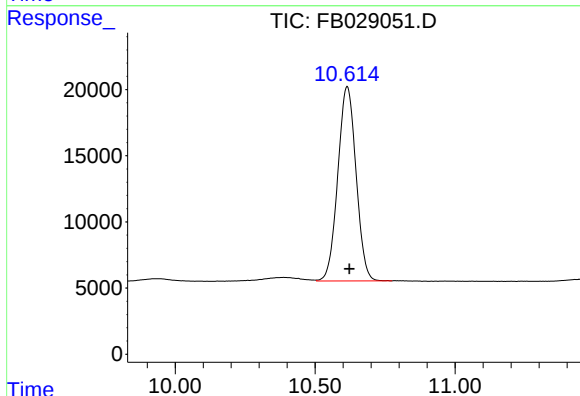


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.008 min
Response: 665791
Conc: 33.10 ng/ml

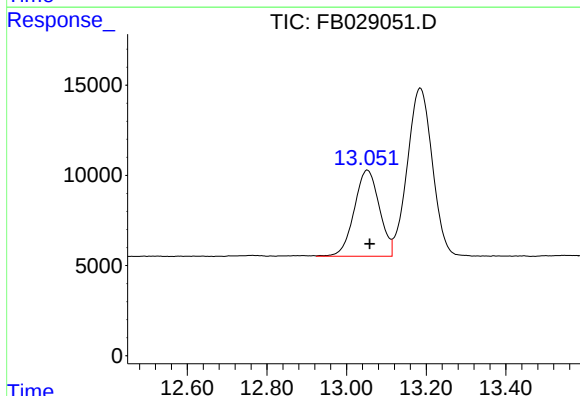


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.006 min
Response: 209223
Conc: 11.03 ng/ml

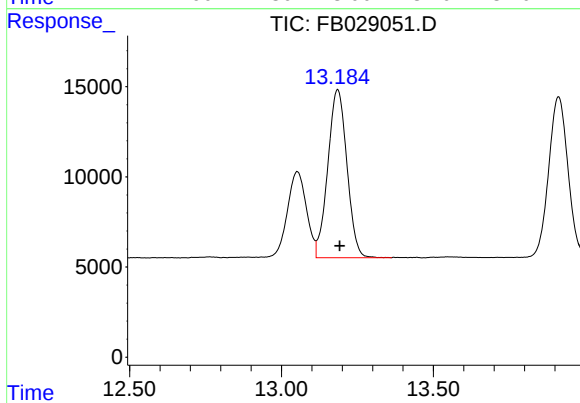

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.006 min
Response: 407834
Conc: 21.68 ng/ml

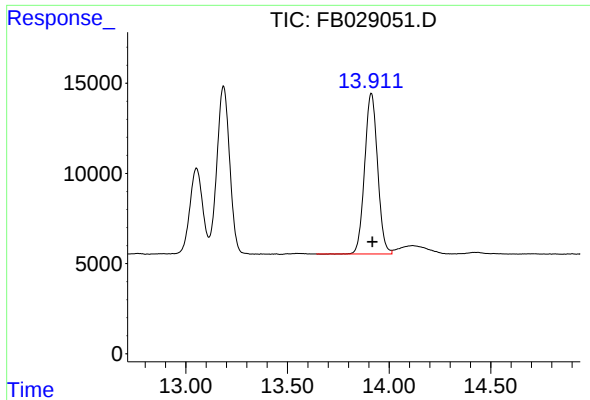

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.006 min
Response: 394384
Conc: 21.50 ng/ml

Instrument :
FID_B
ClientSampleId :

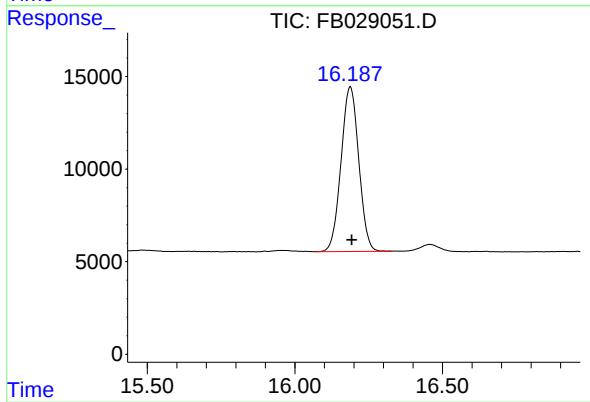

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.005 min
Response: 370510
Conc: 20.11 ng/ml