

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111722\
 Data File : FB029048.D
 Signal(s) : FID2B.CH
 Acq On : 17 Nov 2022 10:38
 Operator : AJ/MA
 Sample : BSF1117S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1117S1

Integration File: Calibration.e
 Quant Time: Nov 18 04:46:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	276583	21.766 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	405391	24.871 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	478880	27.254 ng/ml
3) t n-Heptane	7.747	142067	8.080 ng/ml
4) t Benzene	7.884	187493	9.143 ng/ml
6) t Toluene	10.617	539438	26.820 ng/ml
7) t Ethylbenzene	13.054	173852	9.167 ng/ml
8) t m-Xylene	13.187	347629	18.478 ng/ml
9) t O-Xylene	13.913	346916	18.910 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	355413	19.293 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111722\
Data File : FB029048.D
Signal(s) : FID2B.CH
Acq On : 17 Nov 2022 10:38
Operator : AJ/MA
Sample : BSF1117S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1117S1

Integration File: Calibration.e
Quant Time: Nov 18 04:46:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

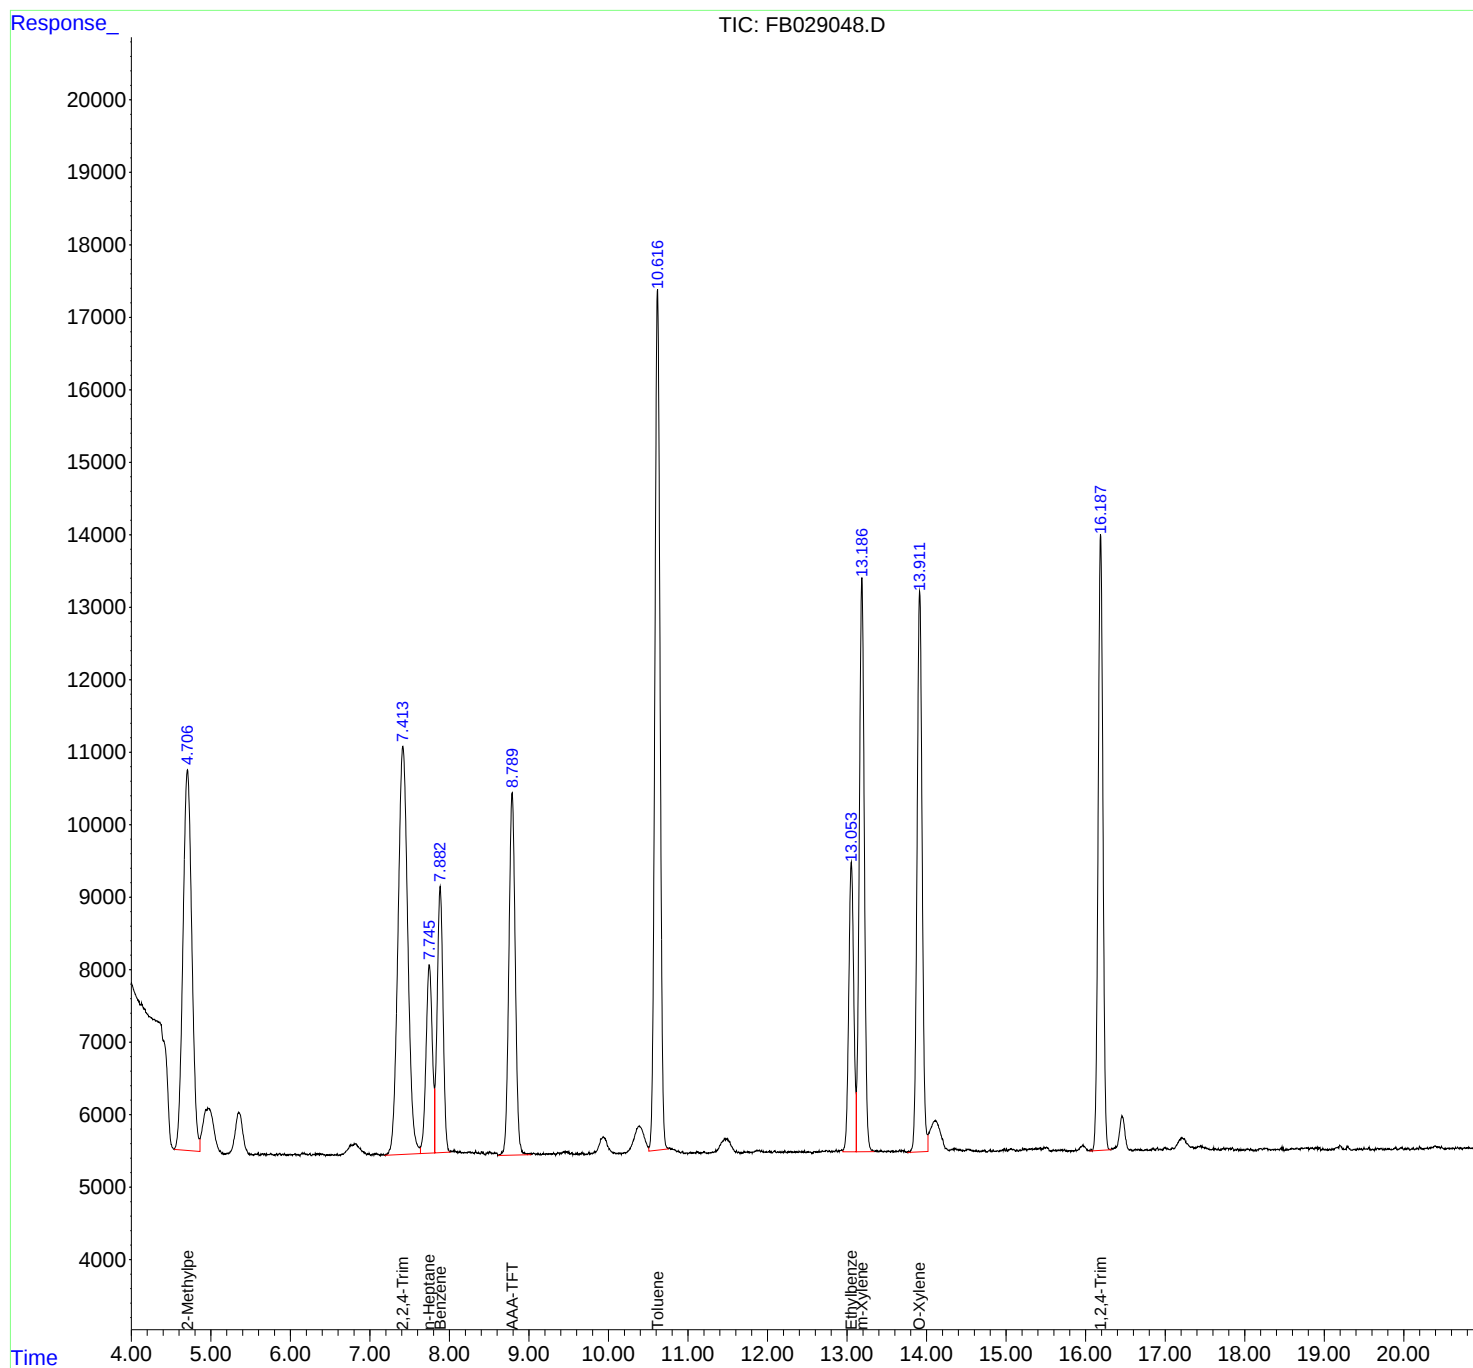


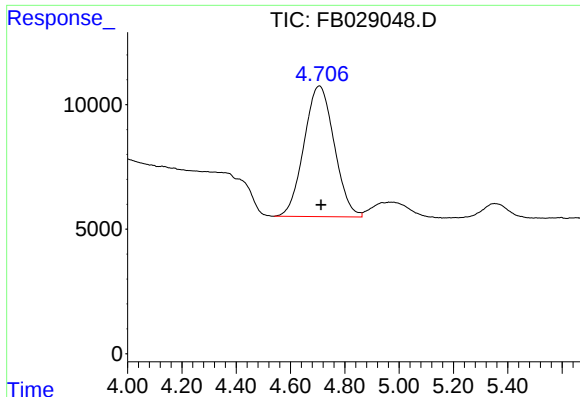

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.005 min
Response: 405391
Conc: 24.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1117S1

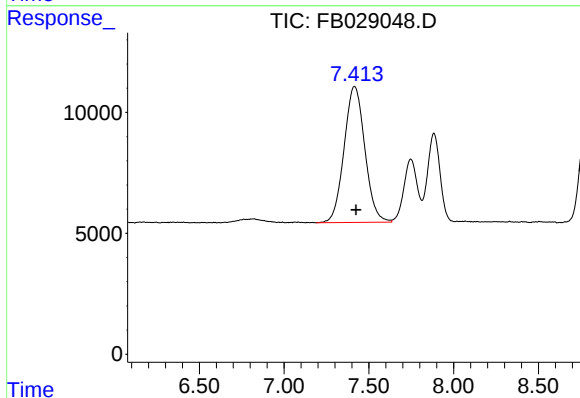


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.010 min
Response: 478880
Conc: 27.25 ng/ml

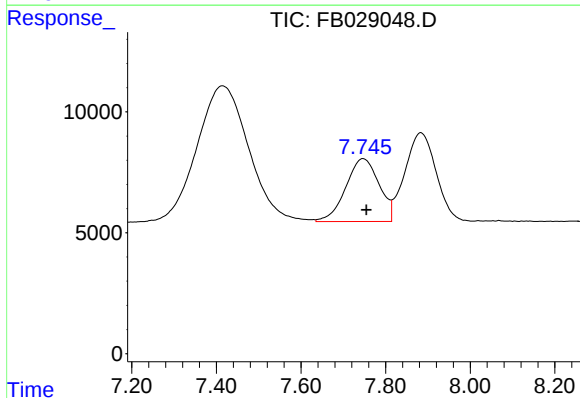


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.008 min
Response: 142067
Conc: 8.08 ng/ml

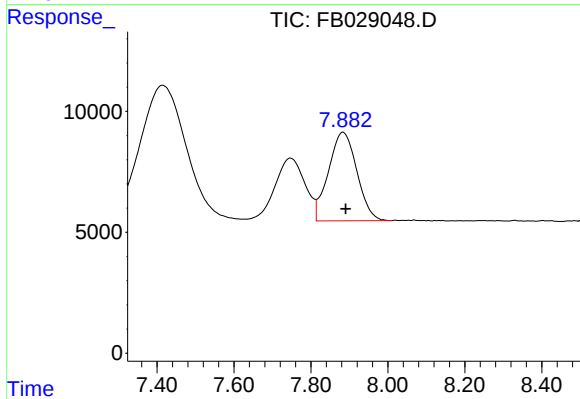

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.007 min
Response: 187493
Conc: 9.14 ng/ml

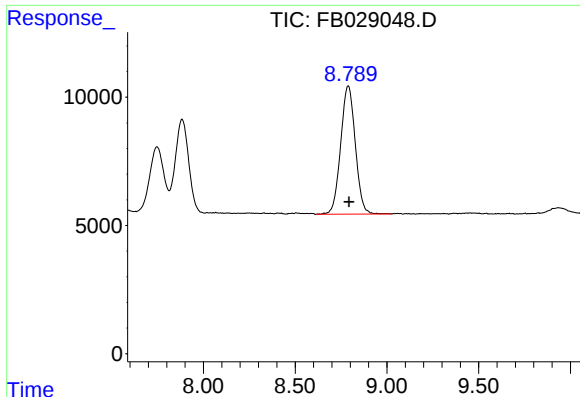

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.005 min
Response: 276583
Conc: 21.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1117S1

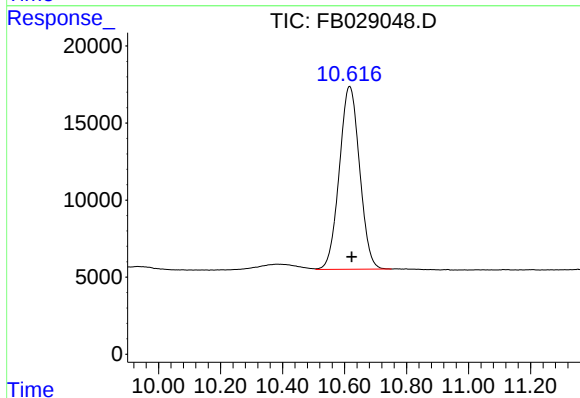


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.006 min
Response: 539438
Conc: 26.82 ng/ml

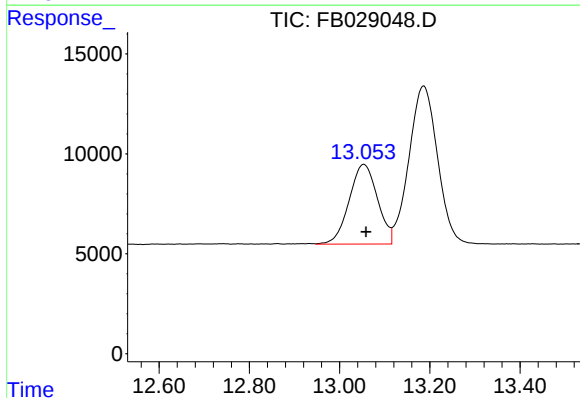


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 173852
Conc: 9.17 ng/ml

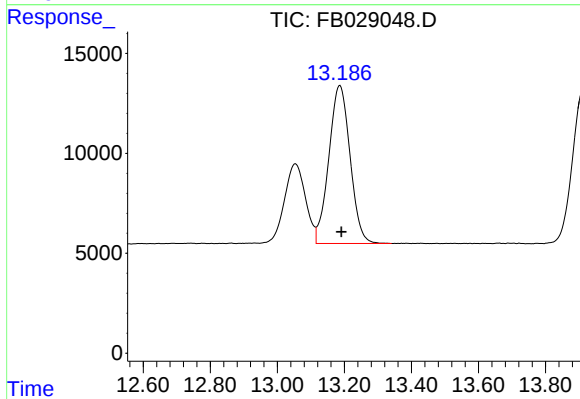

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 347629
Conc: 18.48 ng/ml

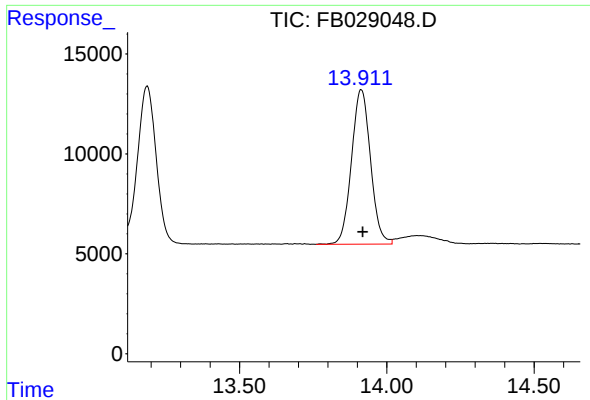

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 346916
Conc: 18.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1117S1

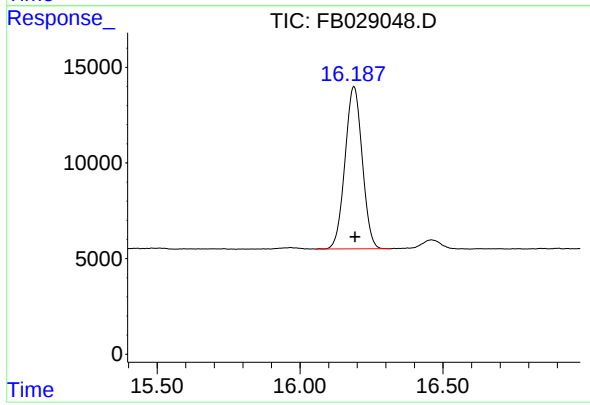

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.004 min
Response: 355413
Conc: 19.29 ng/ml