

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111722\
 Data File : FB029052.D
 Signal(s) : FID2B.CH
 Acq On : 17 Nov 2022 13:09
 Operator : AJ/MA
 Sample : N5598-12MSD
 Misc : 1.16G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FRAC-TANK-SLURRY-0760533MSD

Integration File: Calibration.e
 Quant Time: Nov 18 04:46:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
 Quant Title :
 QLast Update : Tue Nov 01 12:44:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	312771	24.613 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.697	413410	25.363 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	475062	27.036 ng/ml
3) t n-Heptane	7.745	155192	8.827 ng/ml
4) t Benzene	7.882	218958	10.678 ng/ml
6) t Toluene	10.616	635579	31.600 ng/ml
7) t Ethylbenzene	13.053	198289	10.455 ng/ml
8) t m-Xylene	13.185	386910	20.566 ng/ml
9) t O-Xylene	13.913	376666	20.532 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	360488	19.568 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111722\
Data File : FB029052.D
Signal(s) : FID2B.CH
Acq On : 17 Nov 2022 13:09
Operator : AJ/MA
Sample : N5598-12MSD
Misc : 1.16G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FRAC-TANK-SLURRY-0760533MSD

Integration File: Calibration.e
Quant Time: Nov 18 04:46:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110122.M
Quant Title :
QLast Update : Tue Nov 01 12:44:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

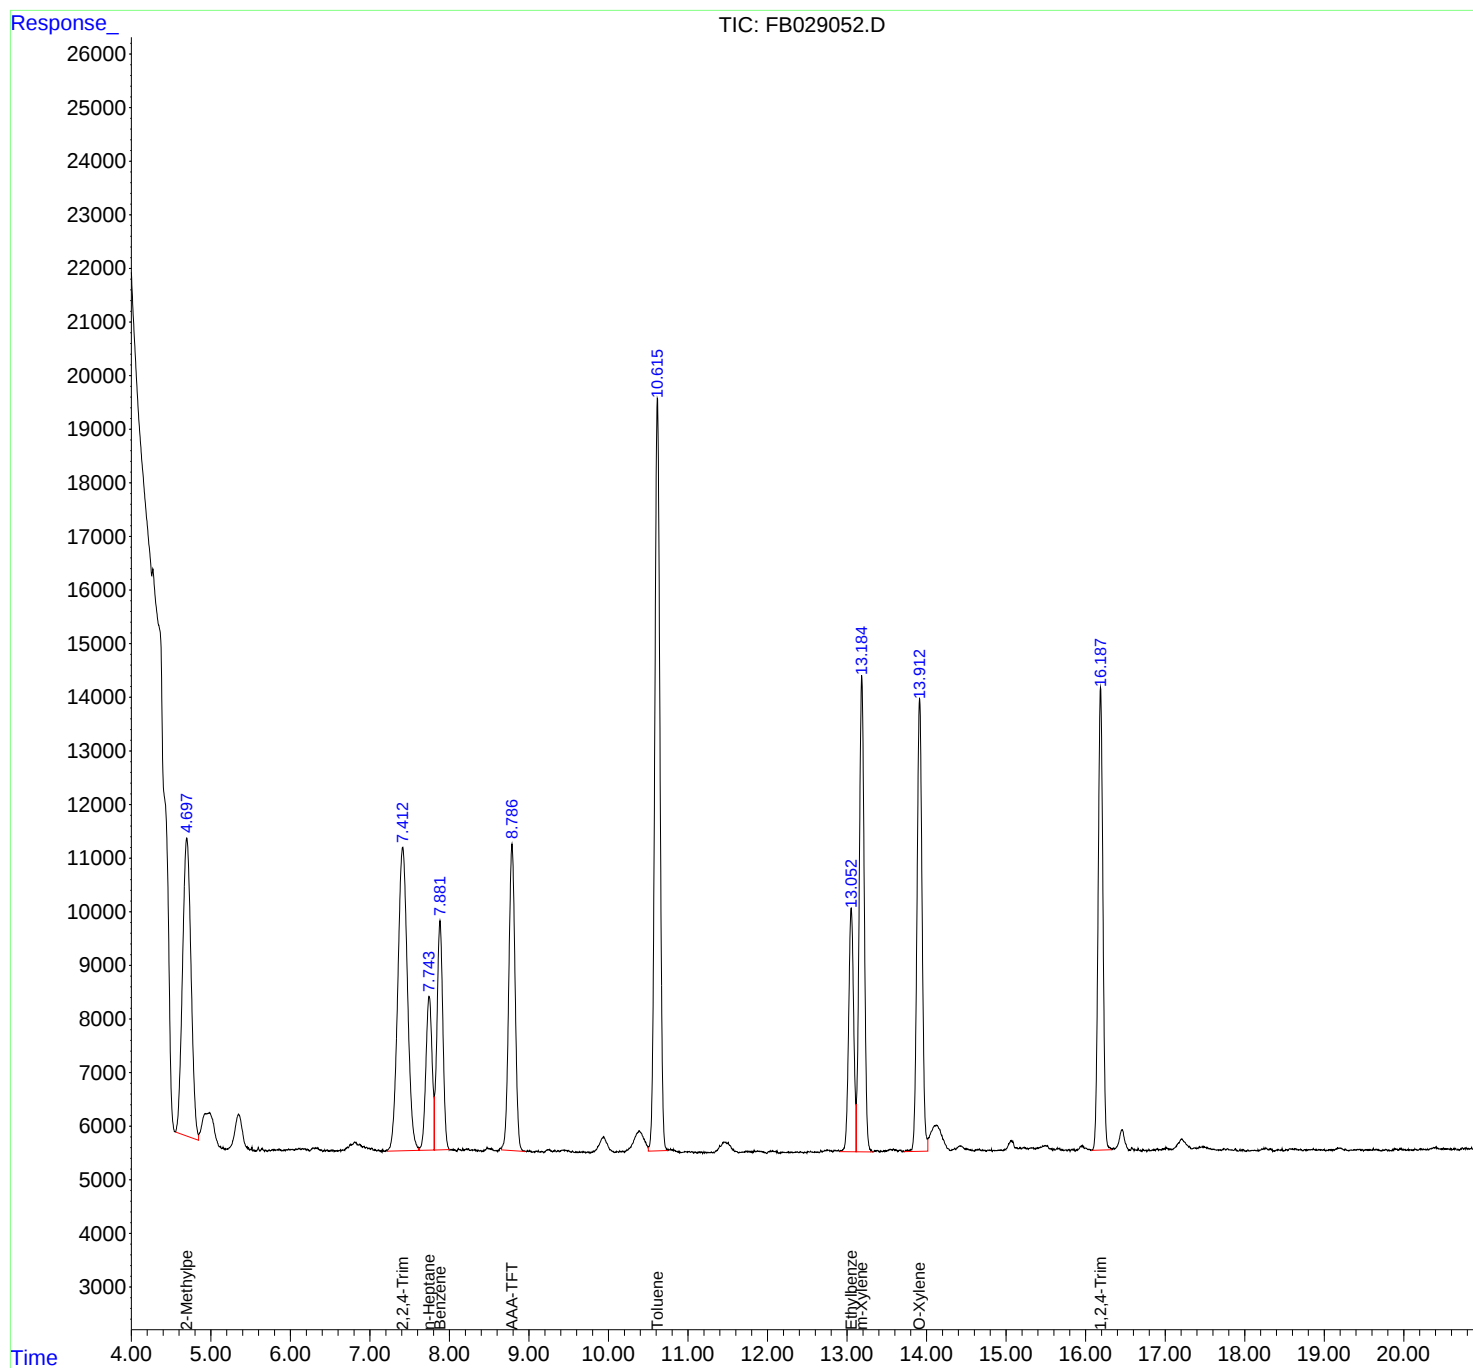


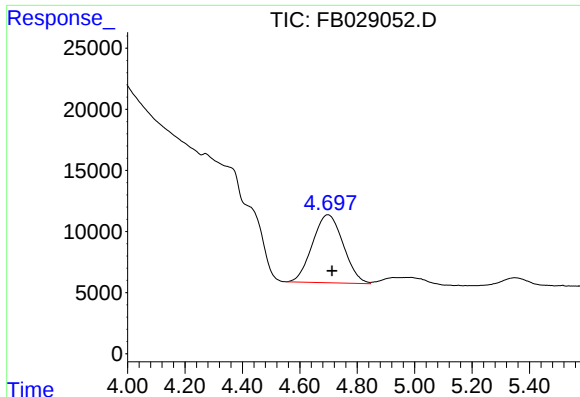

#1 2-Methylpentane


R.T.: 4.697 min
Delta R.T.: -0.015 min
Response: 413410
Conc: 25.36 ng/ml

Instrument :
FID_B
ClientSampleId :
FRAC-TANK-SLURRY-0760533MSD

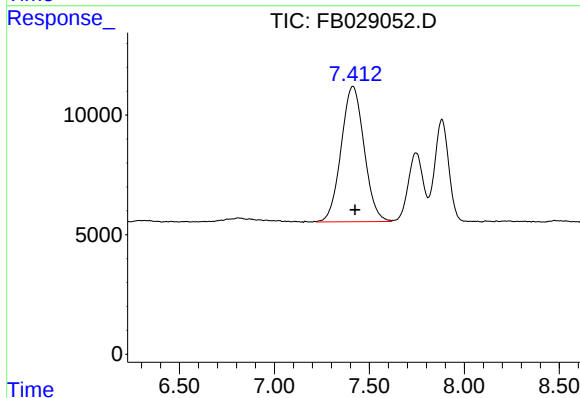


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.011 min
Response: 475062
Conc: 27.04 ng/ml

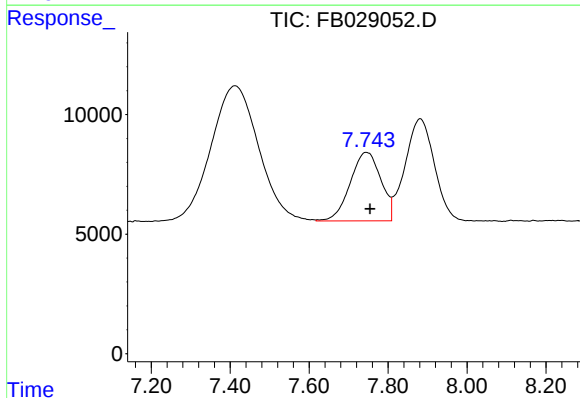


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.010 min
Response: 155192
Conc: 8.83 ng/ml

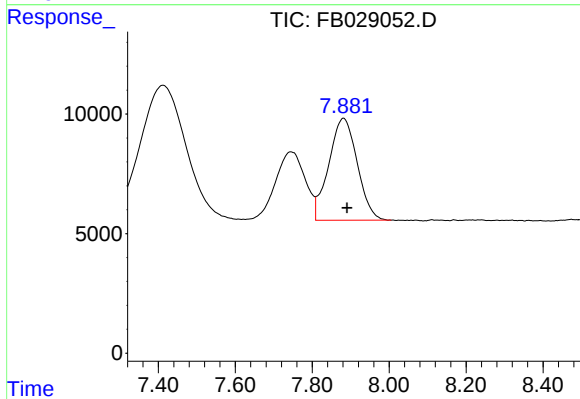

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.008 min
Response: 218958
Conc: 10.68 ng/ml

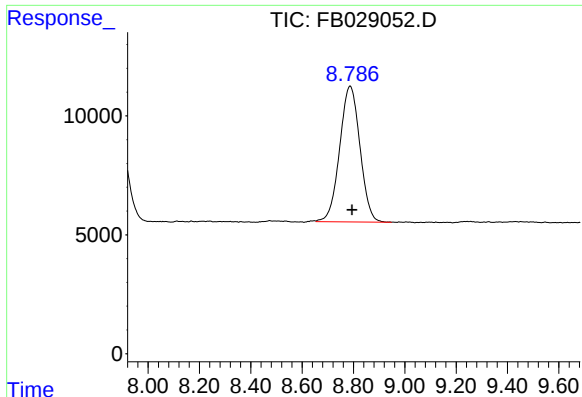

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.007 min
Response: 312771
Conc: 24.61 ng/ml

Instrument :
FID_B
ClientSampleId :
FRAC-TANK-SLURRY-0760533MSD

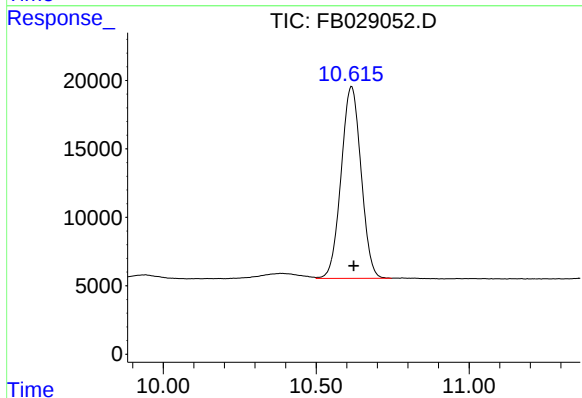


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.007 min
Response: 635579
Conc: 31.60 ng/ml

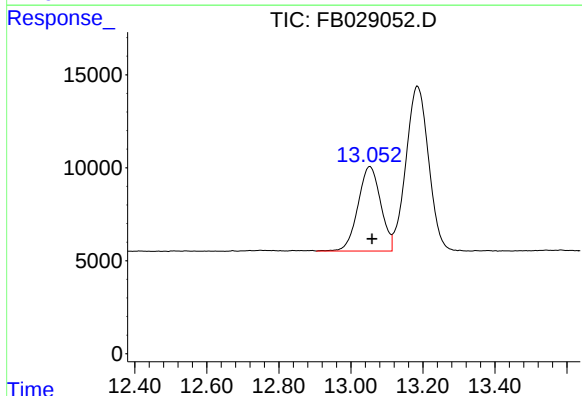


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 198289
Conc: 10.46 ng/ml

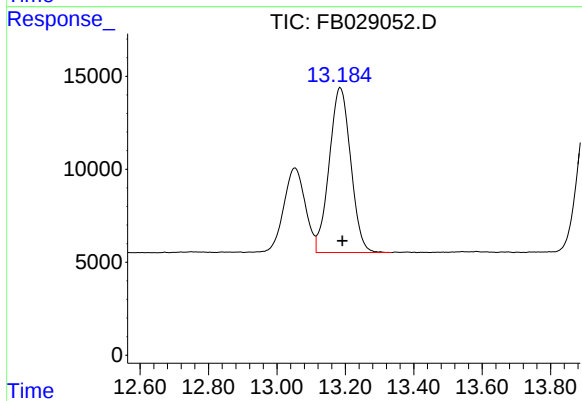

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.006 min
Response: 386910
Conc: 20.57 ng/ml

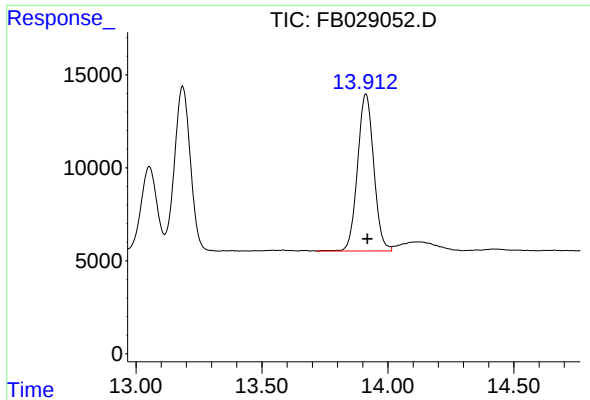

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 376666
Conc: 20.53 ng/ml

Instrument :
FID_B
ClientSampleId :
FRAC-TANK-SLURRY-0760533MSD

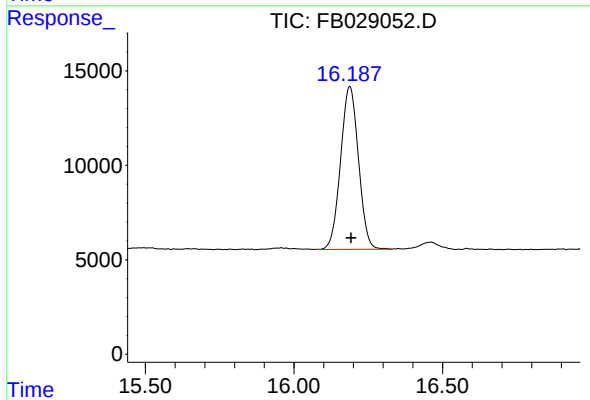

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.004 min
Response: 360488
Conc: 19.57 ng/ml