

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111819\
 Data File : FB023028.D
 Signal(s) : FID2B.CH
 Acq On : 18 Nov 2019 17:19
 Operator : DD/AJ
 Sample : K5665-02 50X
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 19 00:40:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	475539	21.124 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	932059	28.975 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1107333	31.369 ng/ml
3) t n-Heptane	7.759	352659	10.138 ng/ml
4) t Benzene	7.894	445752	10.291 ng/ml
6) t Toluene	10.632	1305283	30.278 ng/ml
7) t Ethylbenzene	13.073	409648	10.261 ng/ml
8) t m-Xylene	13.206	775341	20.529 ng/ml
9) t O-Xylene	13.934	731931	20.536 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	613557	21.636 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111819\
Data File : FB023028.D
Signal(s) : FID2B.CH
Acq On : 18 Nov 2019 17:19
Operator : DD/AJ
Sample : K5665-02 50X
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 19 00:40:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

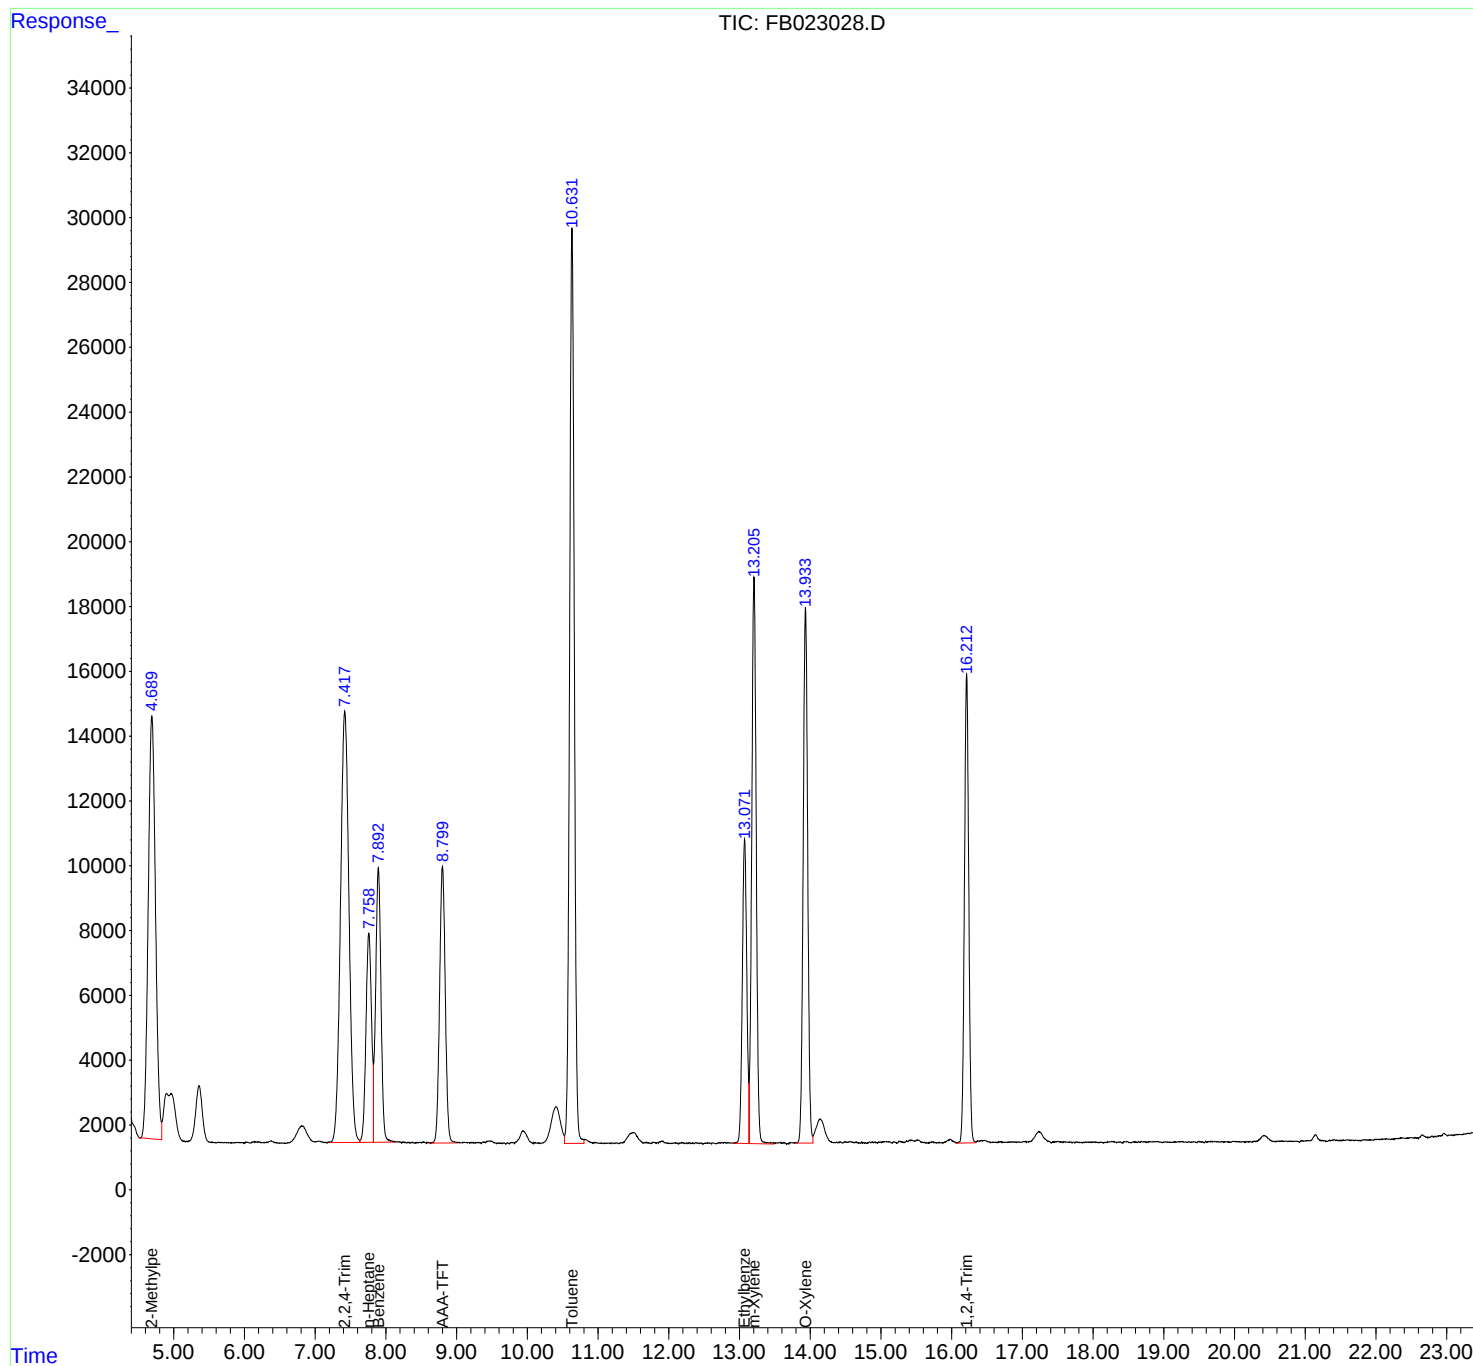

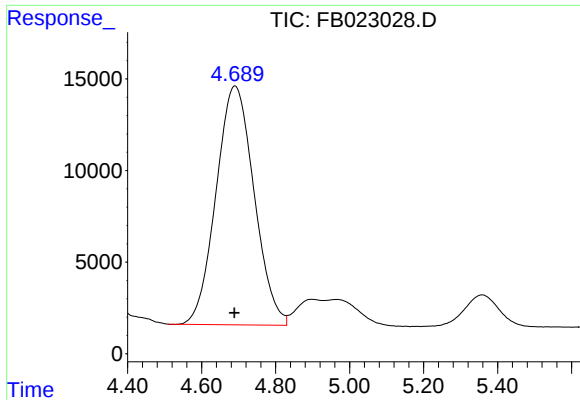


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 932059
Conc: 28.98 ng/ml

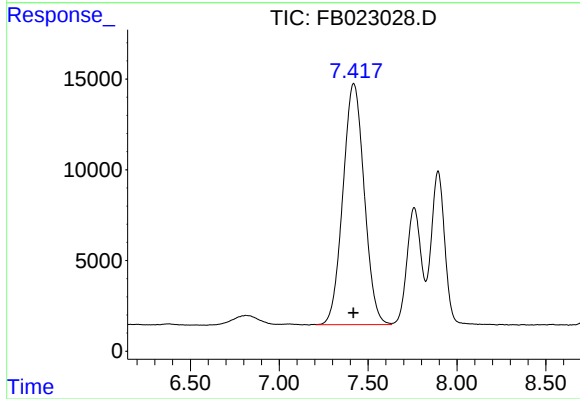


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1107333
Conc: 31.37 ng/ml

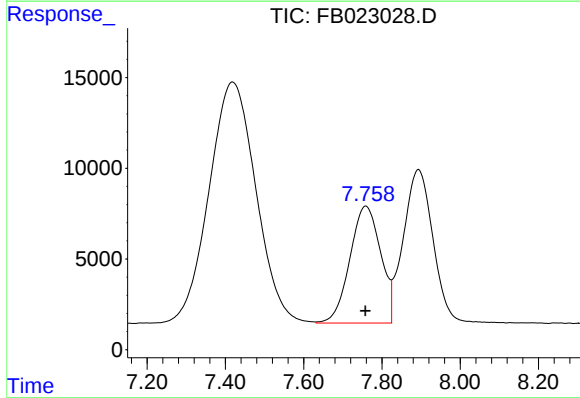


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 352659
Conc: 10.14 ng/ml

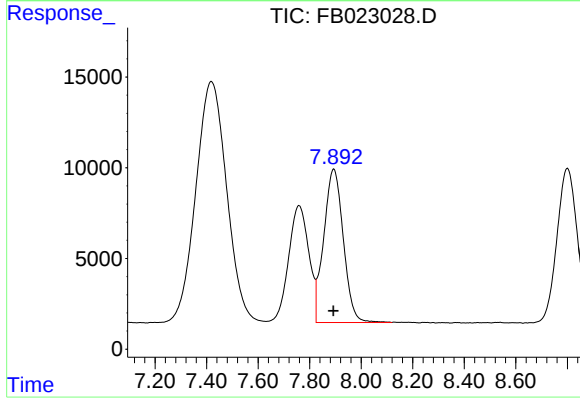


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 445752
Conc: 10.29 ng/ml

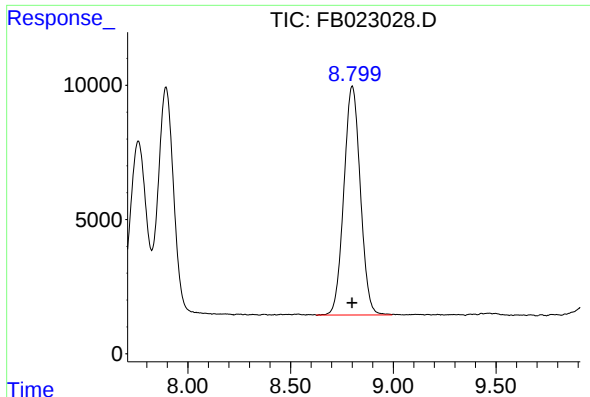


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 475539
Conc: 21.12 ng/ml

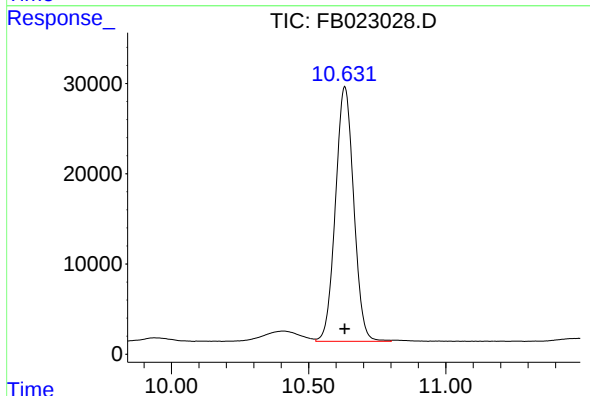


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1305283
Conc: 30.28 ng/ml

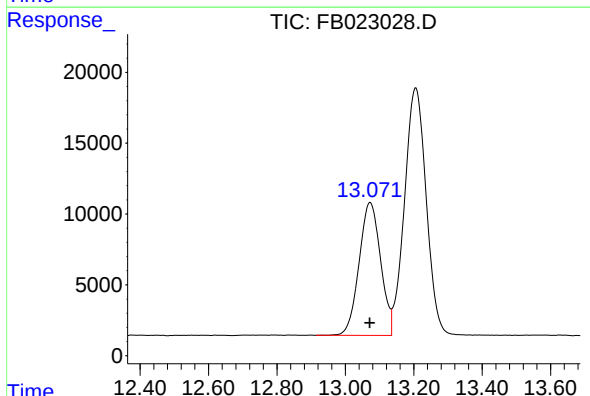


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.001 min
Response: 409648
Conc: 10.26 ng/ml

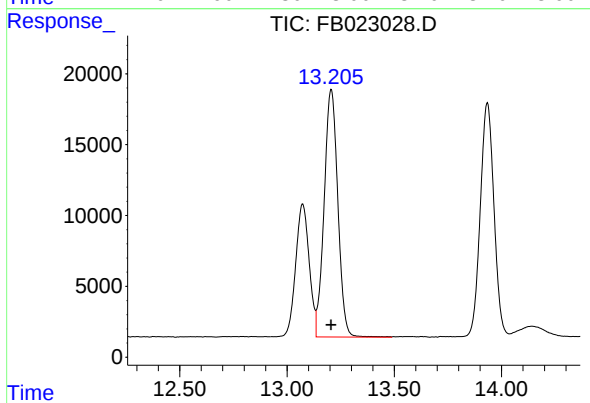


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.001 min
Response: 775341
Conc: 20.53 ng/ml

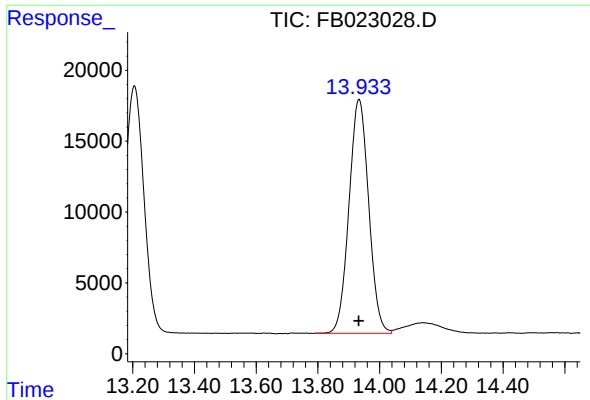

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.002 min
Response: 731931
Conc: 20.54 ng/ml

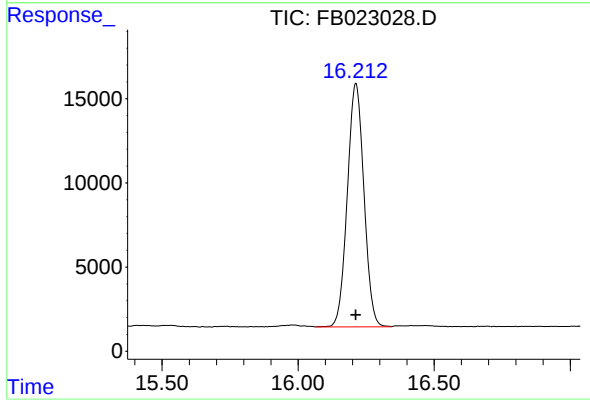

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.001 min
Response: 613557
Conc: 21.64 ng/ml