

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111824\
 Data File : FB031238.D
 Signal(s) : FID2B.CH
 Acq On : 18 Nov 2024 12:40
 Operator : YP/AJ
 Sample : BSF1118S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1118S1

Integration File: Calibration.e
 Quant Time: Nov 18 23:56:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	499856	18.109 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	1105575	28.150 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	1357726	28.989 ng/ml
3) t n-Heptane	7.755	405399	8.945 ng/ml
4) t Benzene	7.894	522360	9.772 ng/ml
6) t Toluene	10.623	1449910	29.035 ng/ml
7) t Ethylbenzene	13.060	420004	9.383 ng/ml
8) t m-Xylene	13.193	895441	18.410 ng/ml
9) t O-Xylene	13.921	834433	18.306 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	660688	17.756 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111824\
Data File : FB031238.D
Signal(s) : FID2B.CH
Acq On : 18 Nov 2024 12:40
Operator : YP/AJ
Sample : BSF1118S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1118S1

Integration File: Calibration.e
Quant Time: Nov 18 23:56:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

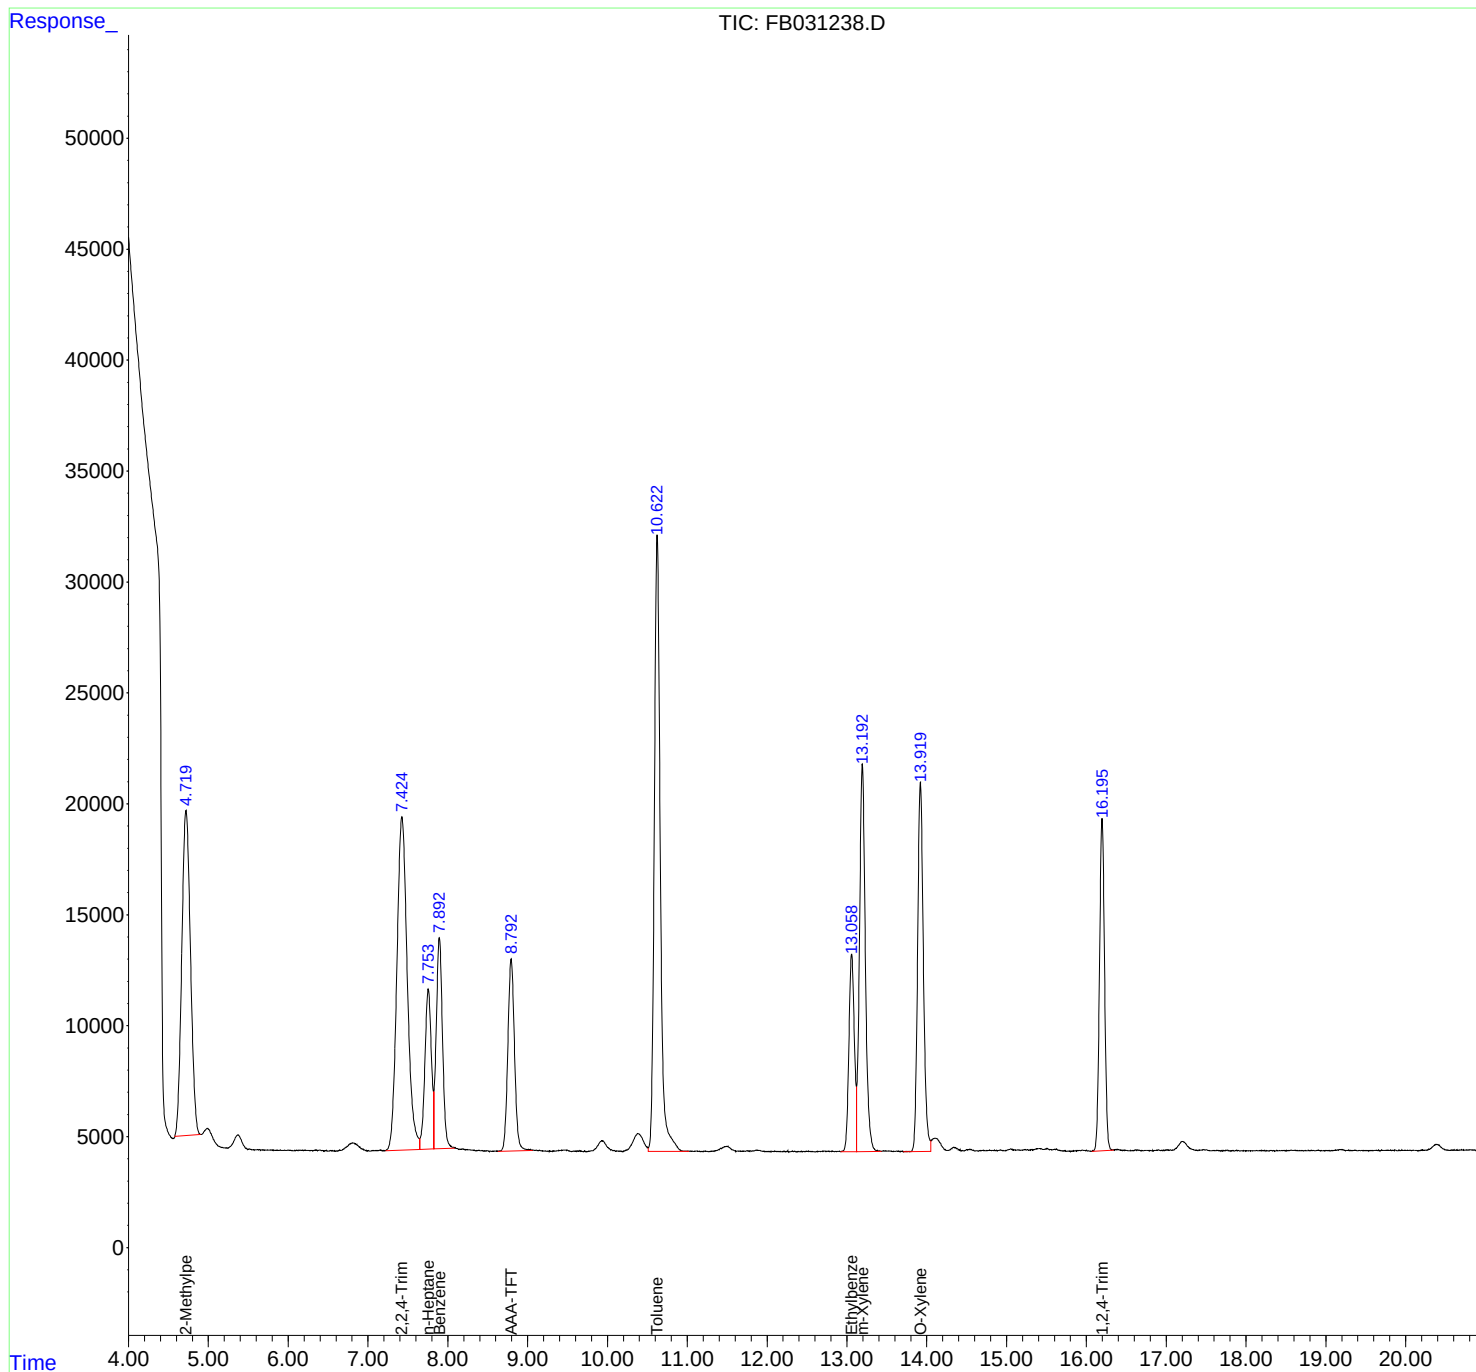


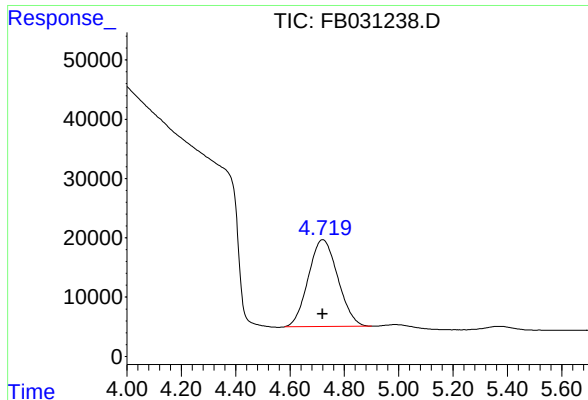

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 1105575
Conc: 28.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1118S1

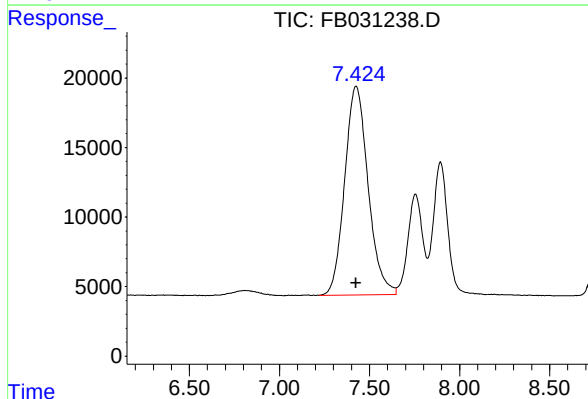


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 1357726
Conc: 28.99 ng/ml

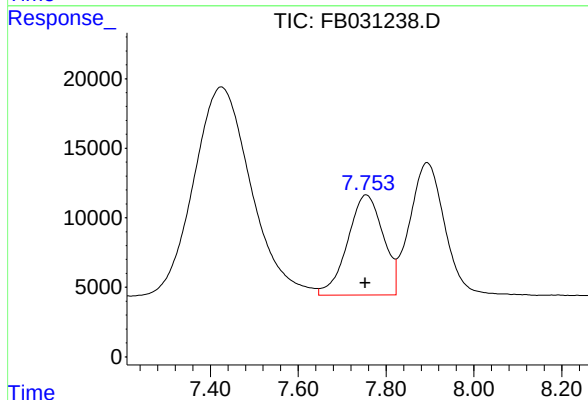


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.002 min
Response: 405399
Conc: 8.95 ng/ml

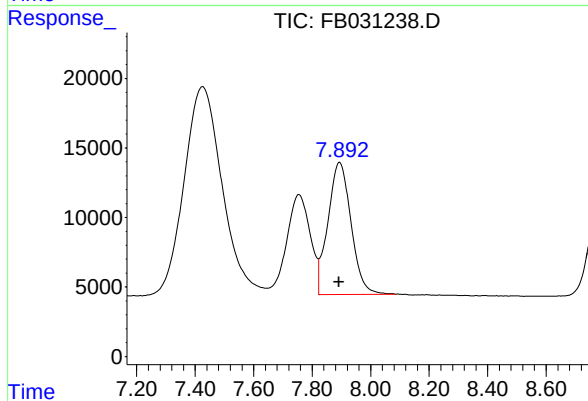

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 522360
Conc: 9.77 ng/ml

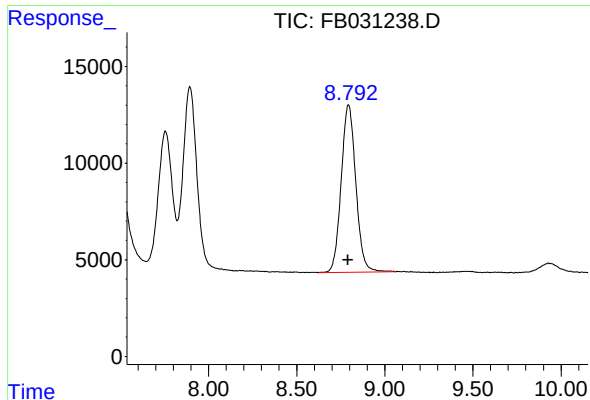

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 499856
Conc: 18.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1118S1

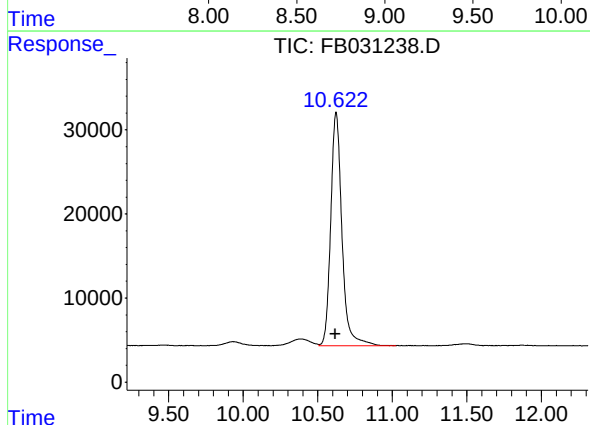


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 1449910
Conc: 29.03 ng/ml

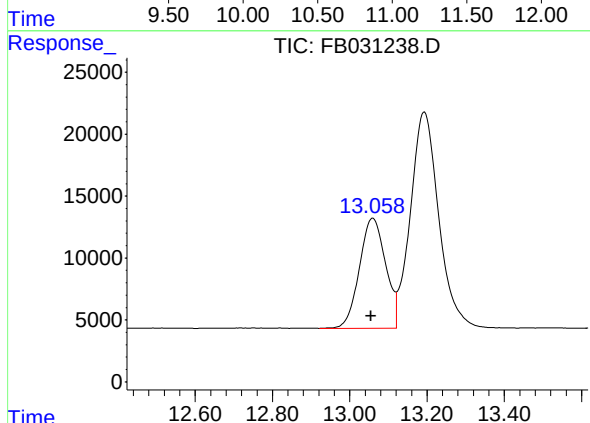


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 420004
Conc: 9.38 ng/ml

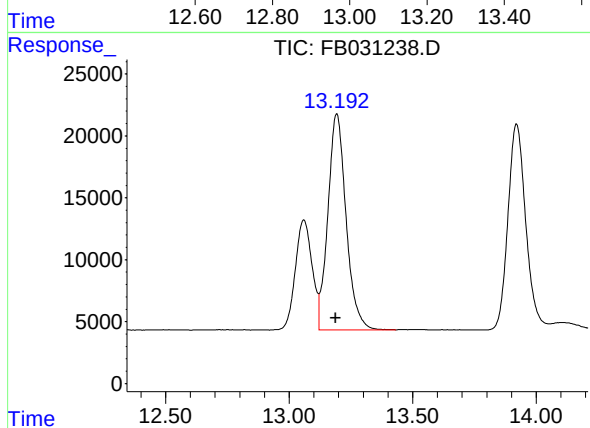

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.005 min
Response: 895441
Conc: 18.41 ng/ml

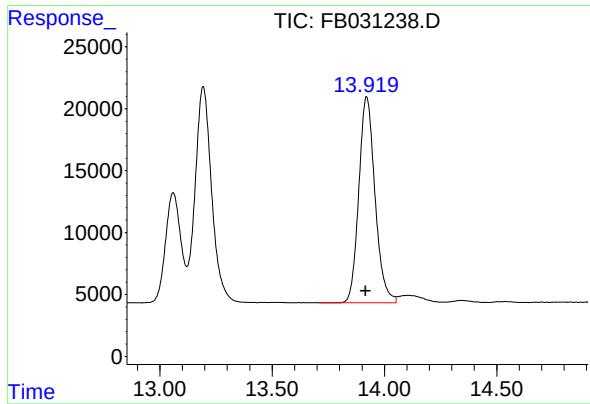

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.004 min
Response: 834433
Conc: 18.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1118S1

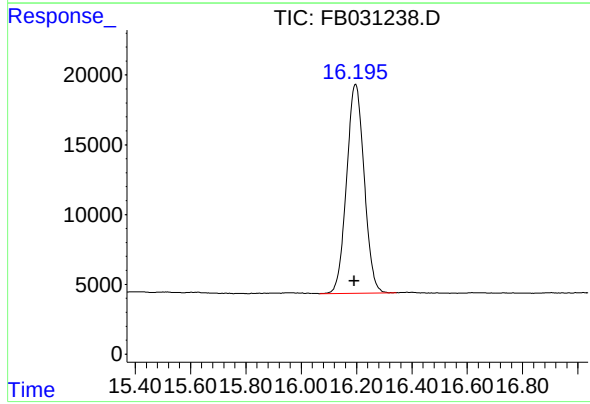

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.004 min
Response: 660688
Conc: 17.76 ng/ml