

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111824\
 Data File : FB031247.D
 Signal(s) : FID2B.CH
 Acq On : 18 Nov 2024 18:53
 Operator : YP/AJ
 Sample : BSF1118S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1118S3

Integration File: Calibration.e
 Quant Time: Nov 18 23:57:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
 Quant Title :
 QLast Update : Mon Oct 28 12:19:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	543316	19.683 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	1014018	25.819 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	1296736	27.687 ng/ml
3) t n-Heptane	7.752	379315	8.370 ng/ml
4) t Benzene	7.891	508310	9.509 ng/ml
6) t Toluene	10.621	1400742	28.050 ng/ml
7) t Ethylbenzene	13.058	406439	9.080 ng/ml
8) t m-Xylene	13.191	868730	17.861 ng/ml
9) t O-Xylene	13.920	813201	17.840 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	648752	17.436 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111824\
Data File : FB031247.D
Signal(s) : FID2B.CH
Acq On : 18 Nov 2024 18:53
Operator : YP/AJ
Sample : BSF1118S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1118S3

Integration File: Calibration.e
Quant Time: Nov 18 23:57:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102824.M
Quant Title :
QLast Update : Mon Oct 28 12:19:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

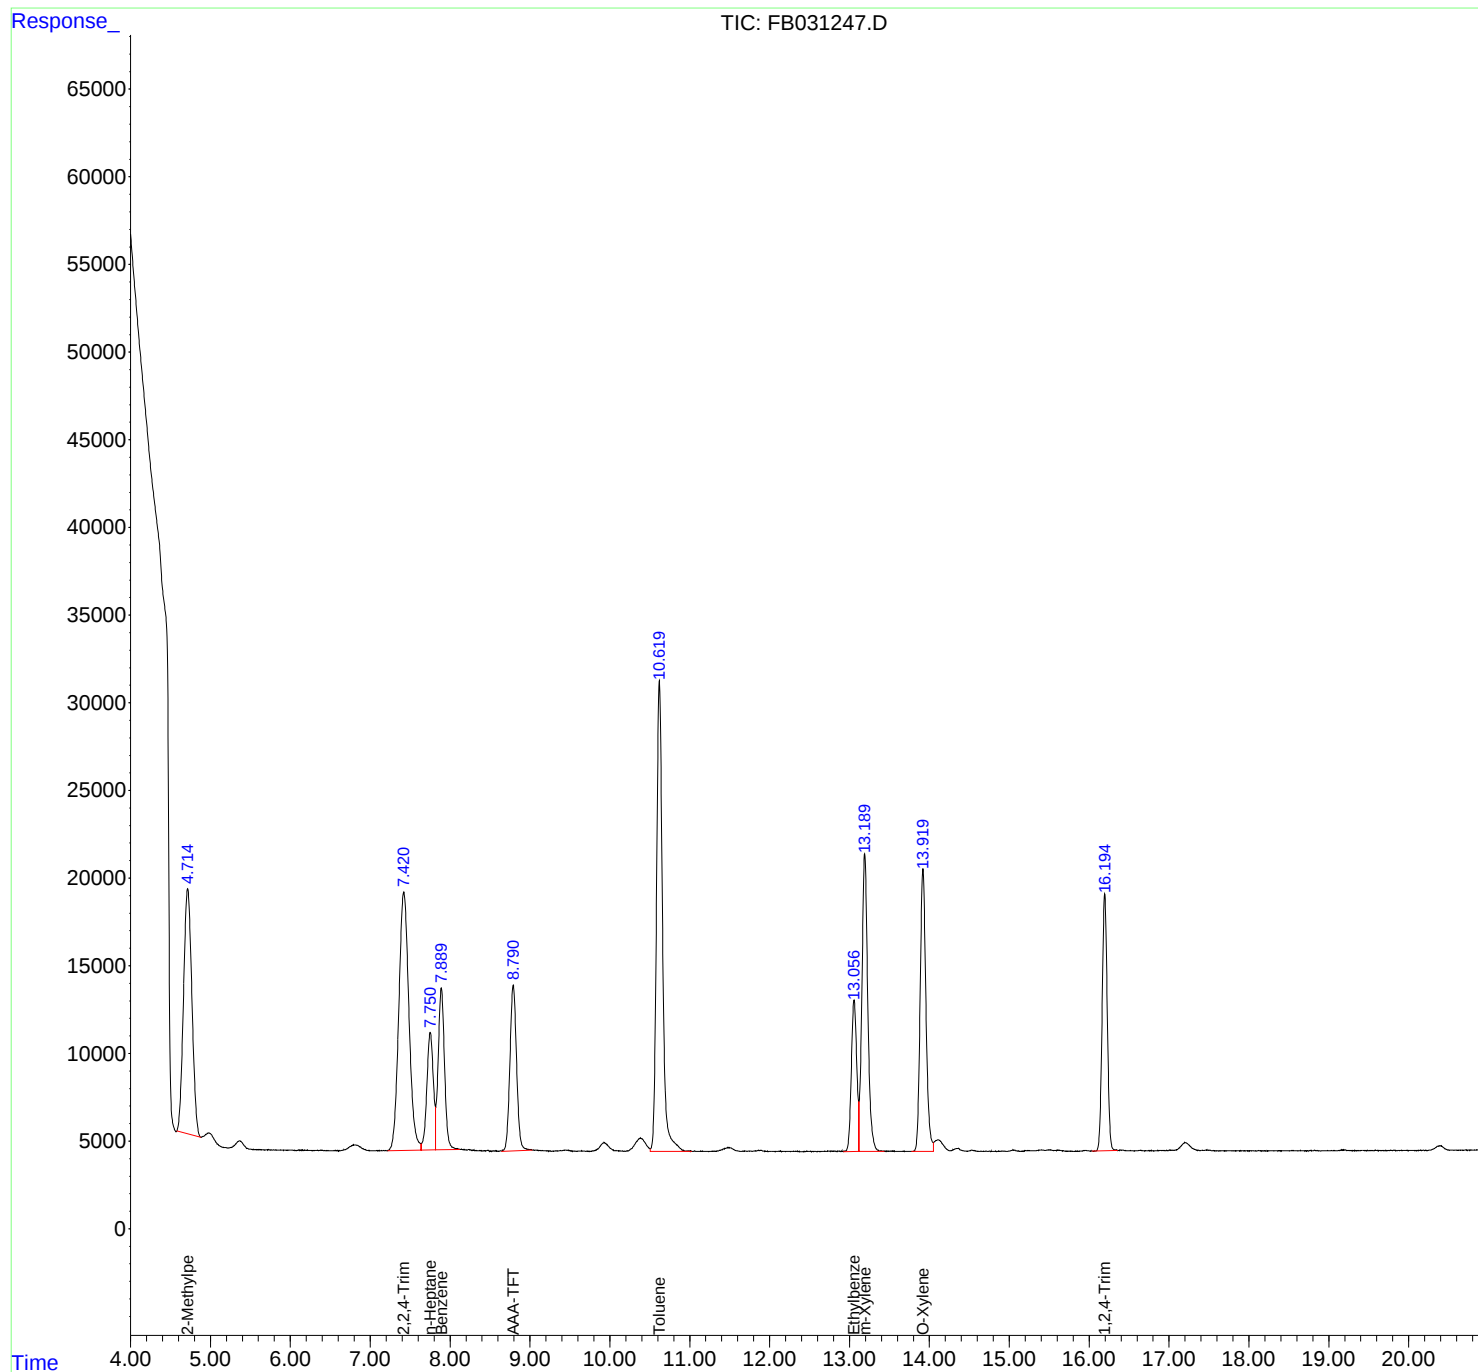


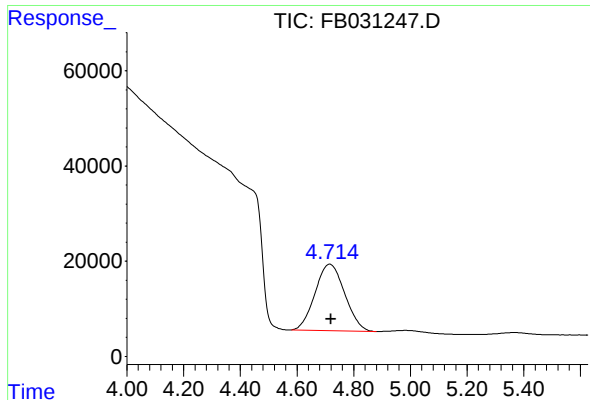

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: -0.004 min
Response: 1014018
Conc: 25.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1118S3

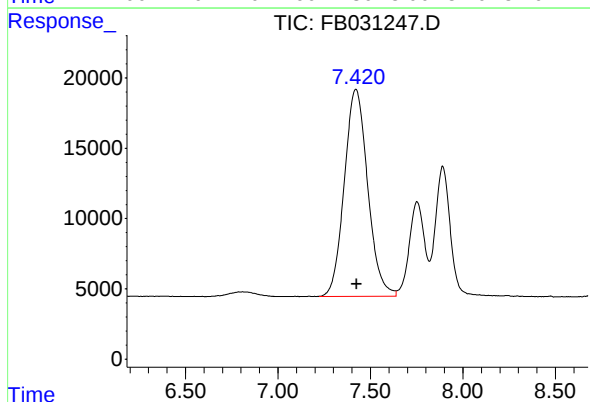


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.003 min
Response: 1296736
Conc: 27.69 ng/ml

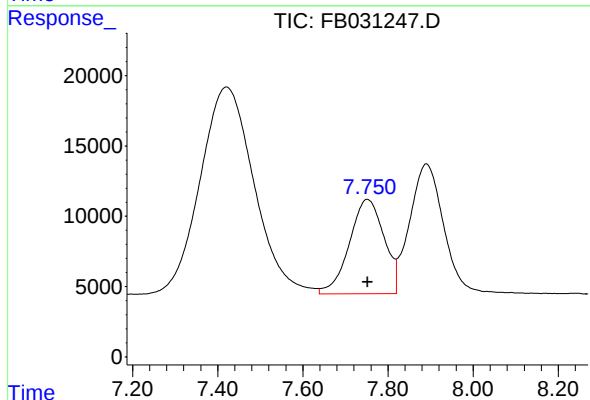


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 379315
Conc: 8.37 ng/ml

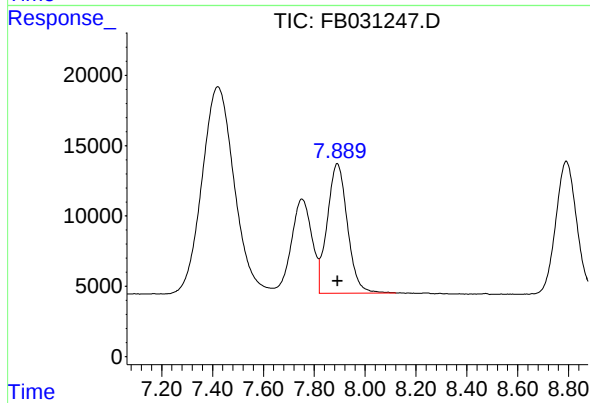

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 508310
Conc: 9.51 ng/ml

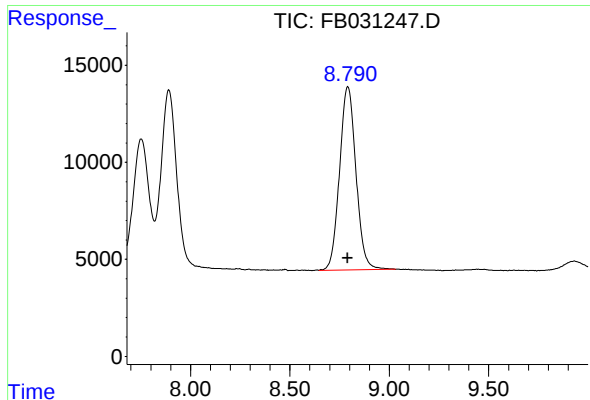

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 543316
Conc: 19.68 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1118S3

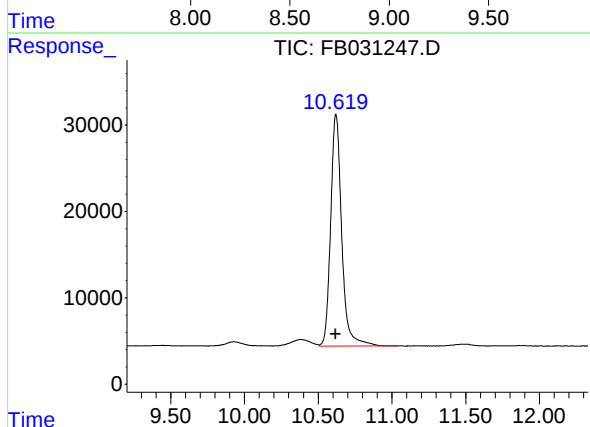


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.001 min
Response: 1400742
Conc: 28.05 ng/ml

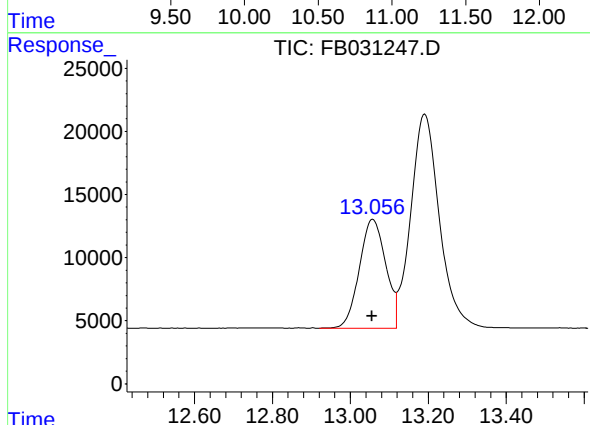


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.003 min
Response: 406439
Conc: 9.08 ng/ml

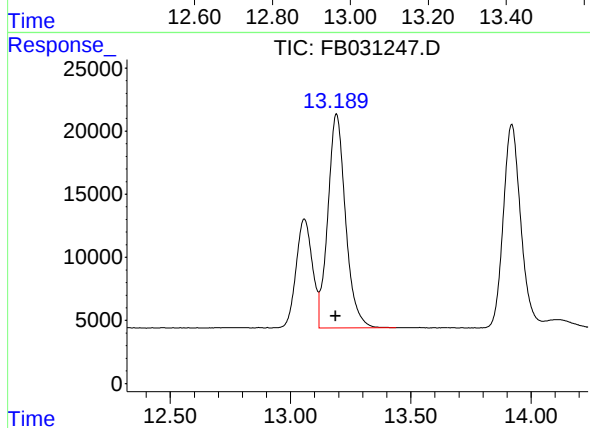

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.003 min
Response: 868730
Conc: 17.86 ng/ml

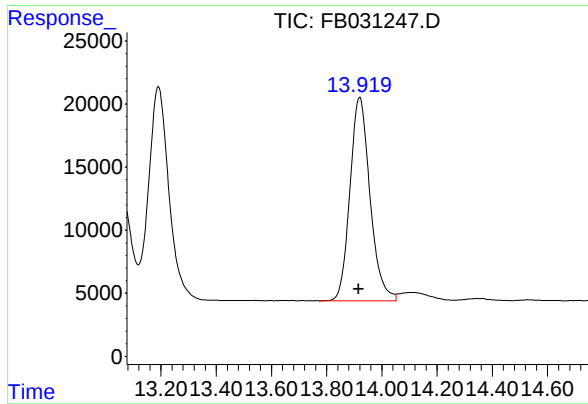

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.003 min
Response: 813201
Conc: 17.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1118S3

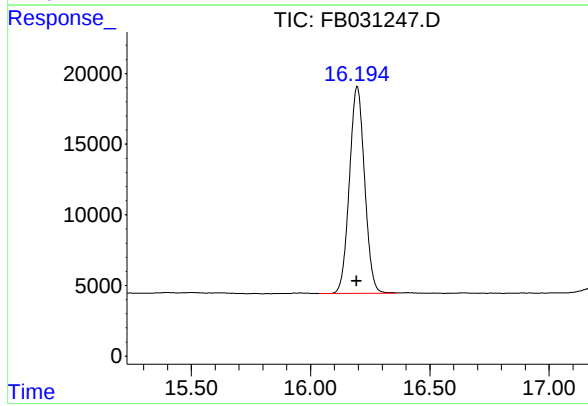

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 648752
Conc: 17.44 ng/ml