

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111918\
 Data File : FB018812.D
 Signal(s) : FID2B.CH
 Acq On : 19 Nov 2018 10:55
 Operator : MJ/SJ
 Sample : VBF1119S2
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 19 15:49:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
 Quant Title :
 QLast Update : Fri Nov 09 10:53:13 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.108	161453	18.718 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.965	734	0.050 ng/ml
2) t	2,2,4-Trimethylpentane	7.711	677	0.046 ng/ml
3) t	n-Heptane	8.056	1444	0.100 ng/ml
4) t	Benzene	8.180	4772	0.263 ng/ml
6) t	Toluene	10.948	2324	0.154 ng/ml
7) t	Ethylbenzene	13.405	2064	0.132 ng/ml
8) t	m-Xylene	13.545	768	0.046 ng/ml
9) t	O-Xylene	14.263	1558	0.091 ng/ml
10) t	1,2,4-Trimethylbenzene	16.534	452	0.023 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111918\
Data File : FB018812.D
Signal(s) : FID2B.CH
Acq On : 19 Nov 2018 10:55
Operator : MJ/SJ
Sample : VBF1119S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 19 15:49:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110918.M
Quant Title :
QLast Update : Fri Nov 09 10:53:13 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

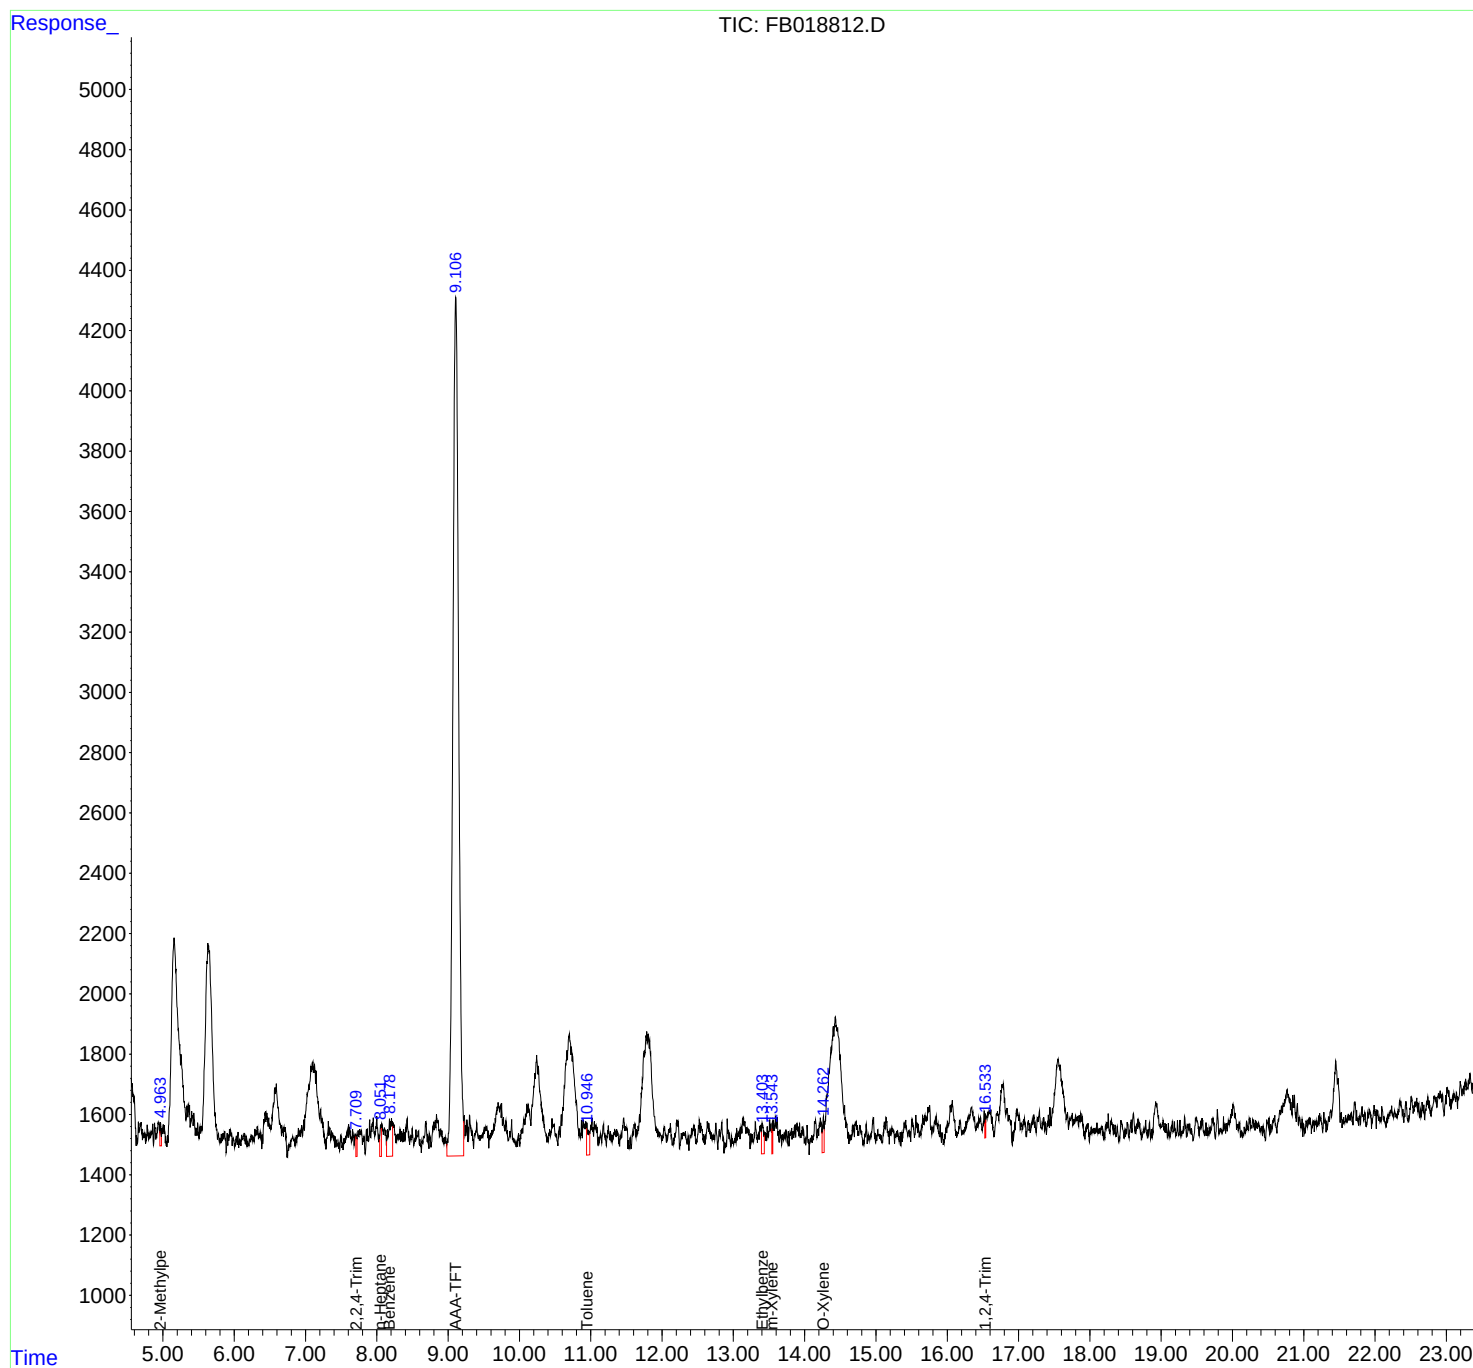

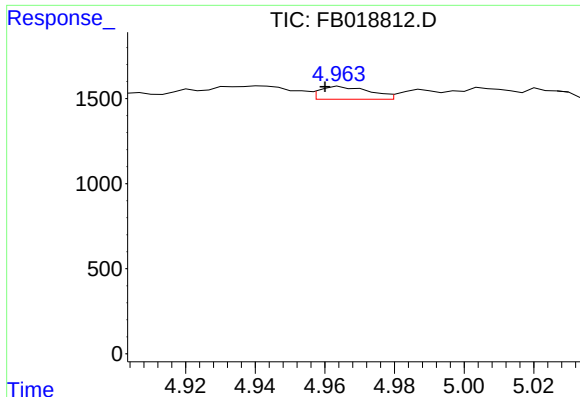


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: 0.005 min
Response: 734
Conc: 0.05 ng/ml

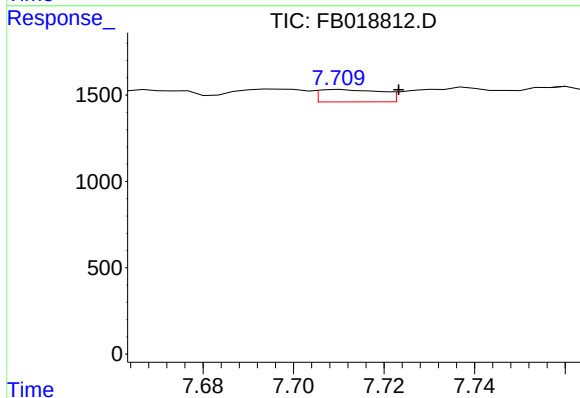


#2 2,2,4-Trimethylpentane

R.T.: 7.711 min
Delta R.T.: -0.013 min
Response: 677
Conc: 0.05 ng/ml

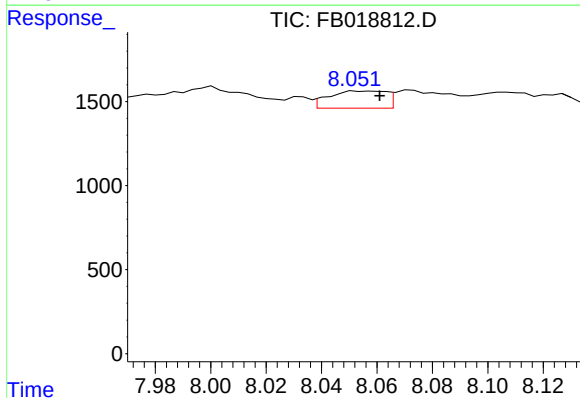


#3 n-Heptane

R.T.: 8.056 min
Delta R.T.: -0.005 min
Response: 1444
Conc: 0.10 ng/ml

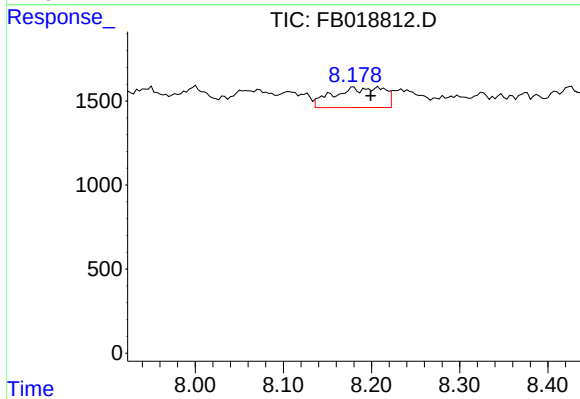


#4 Benzene

R.T.: 8.180 min
Delta R.T.: -0.020 min
Response: 4772
Conc: 0.26 ng/ml

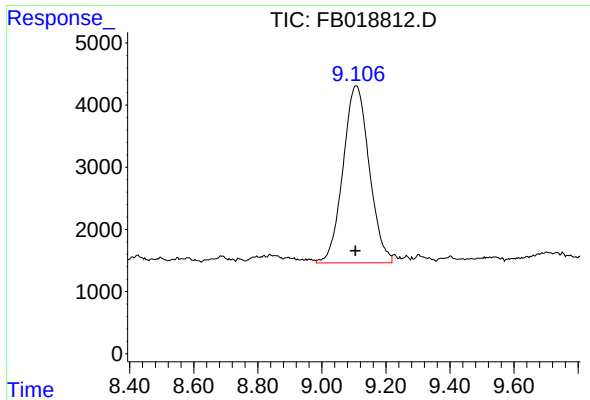


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: 0.003 min
Response: 161453
Conc: 18.72 ng/ml

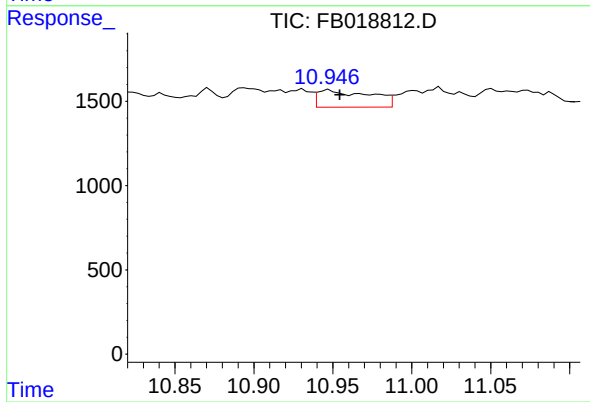


#6 Toluene

R.T.: 10.948 min
Delta R.T.: -0.007 min
Response: 2324
Conc: 0.15 ng/ml

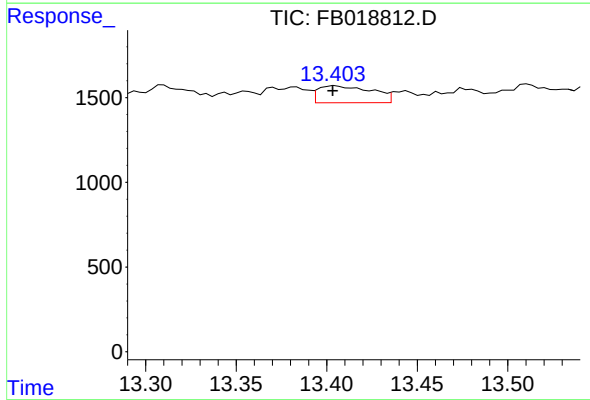


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: 0.002 min
Response: 2064
Conc: 0.13 ng/ml

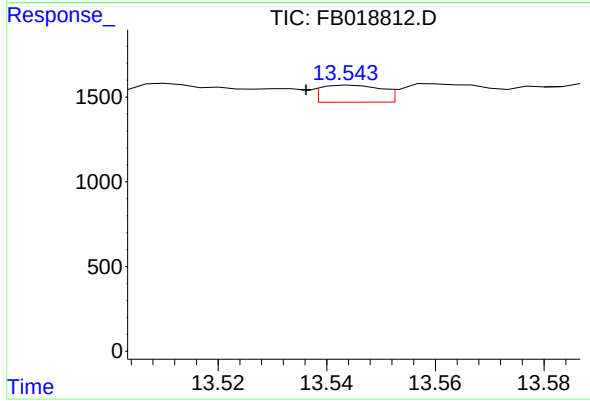


#8 m-Xylene

R.T.: 13.545 min
Delta R.T.: 0.009 min
Response: 768
Conc: 0.05 ng/ml

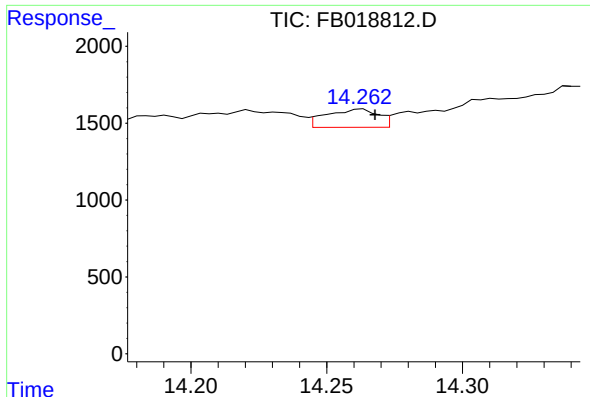

#9 O-Xylene

R.T.: 14.263 min
Delta R.T.: -0.005 min
Response: 1558
Conc: 0.09 ng/ml

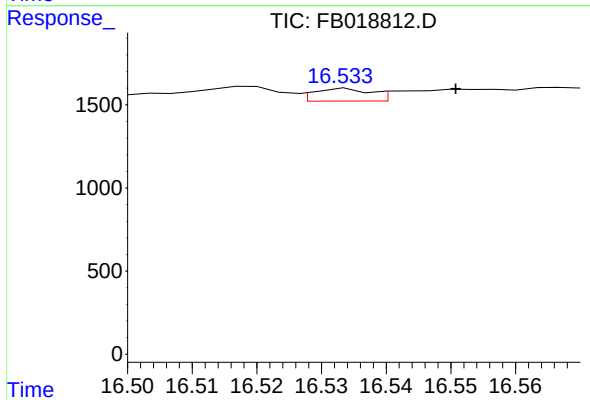

#10 1,2,4-Trimethylbenzene

R.T.: 16.534 min
Delta R.T.: -0.017 min
Response: 452
Conc: 0.02 ng/ml