

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111919\
 Data File : FB023038.D
 Signal(s) : FID2B.CH
 Acq On : 19 Nov 2019 15:30
 Operator : DD/AJ
 Sample : K5916-01MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 20 00:28:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.799	387234	17.201 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	687928	21.386 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	784307	22.218 ng/ml
3) t	n-Heptane	7.758	242045	6.958 ng/ml
4) t	Benzene	7.892	360756	8.329 ng/ml
6) t	Toluene	10.631	1056934	24.517 ng/ml
7) t	Ethylbenzene	13.071	330730	8.284 ng/ml
8) t	m-Xylene	13.204	621422	16.454 ng/ml
9) t	O-Xylene	13.932	601660	16.881 ng/ml
10) t	1,2,4-Trimethylbenzene	16.211	483553	17.051 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111919\
Data File : FB023038.D
Signal(s) : FID2B.CH
Acq On : 19 Nov 2019 15:30
Operator : DD/AJ
Sample : K5916-01MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 20 00:28:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

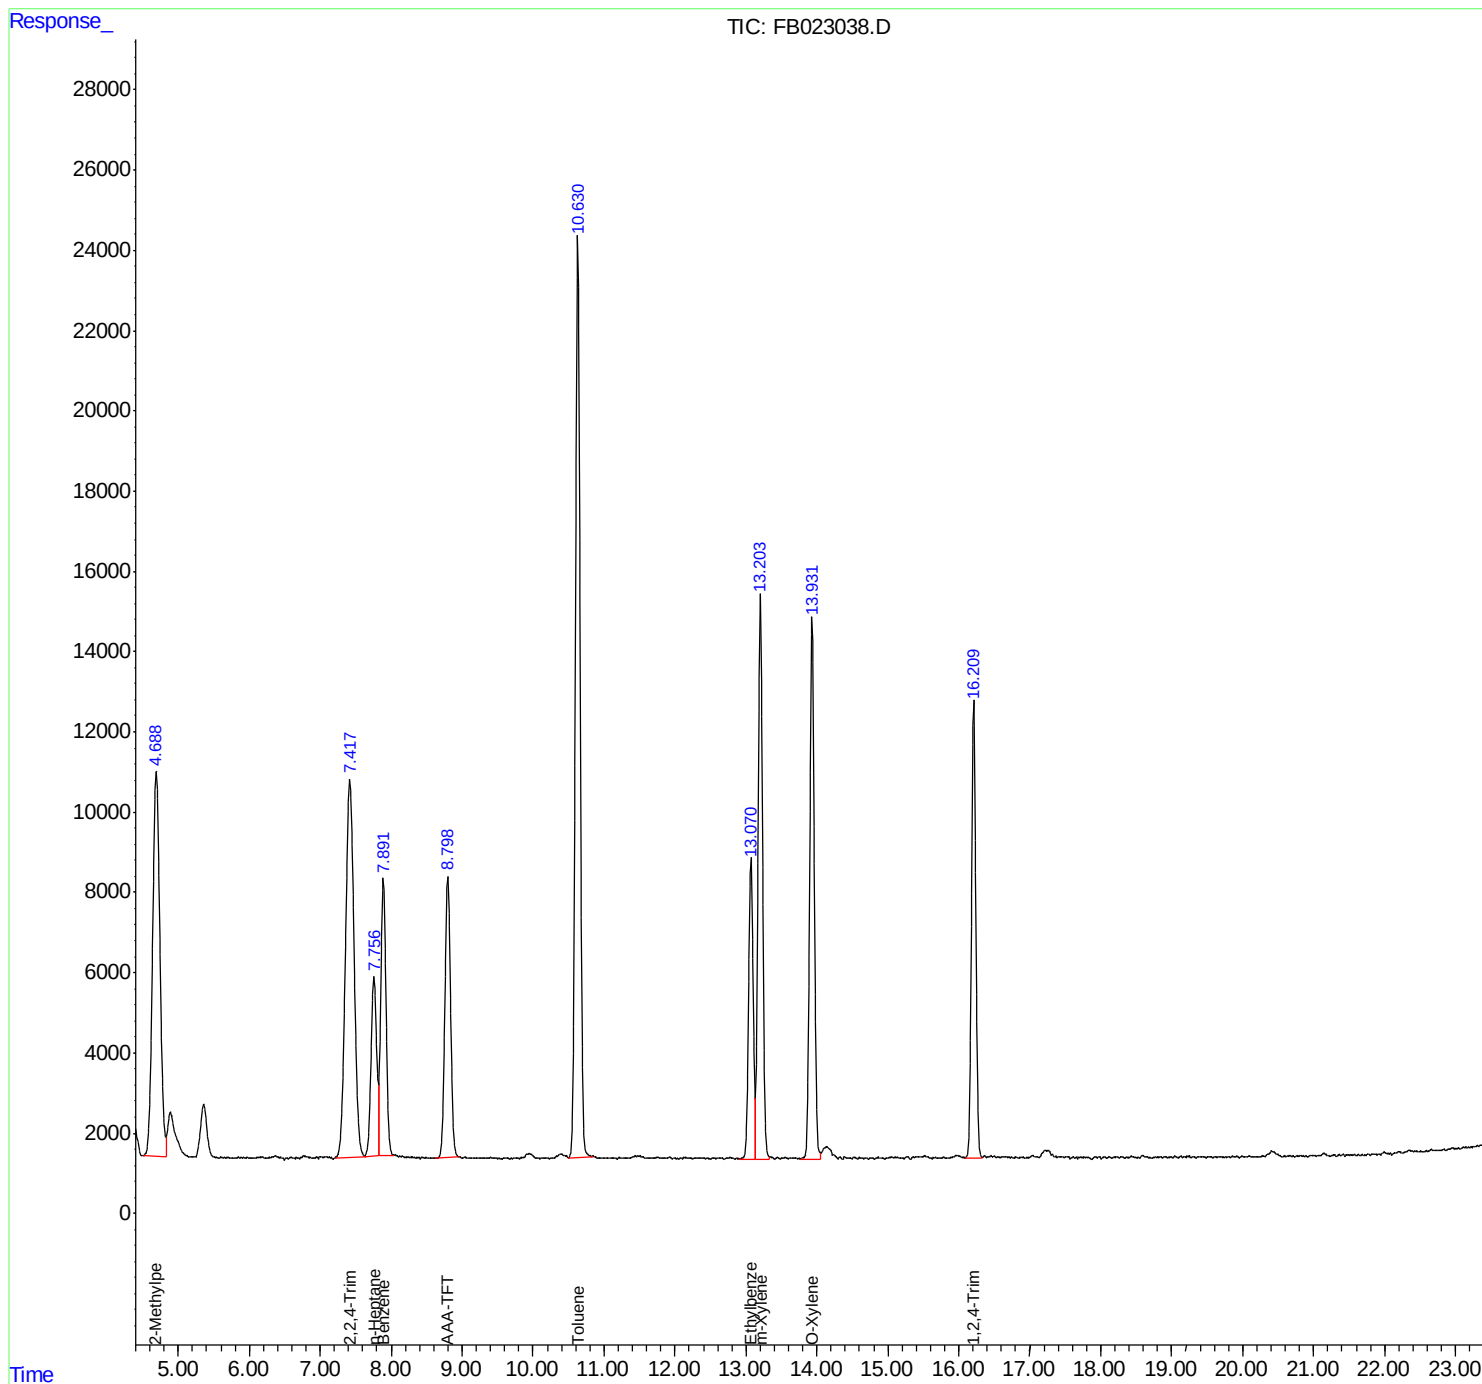

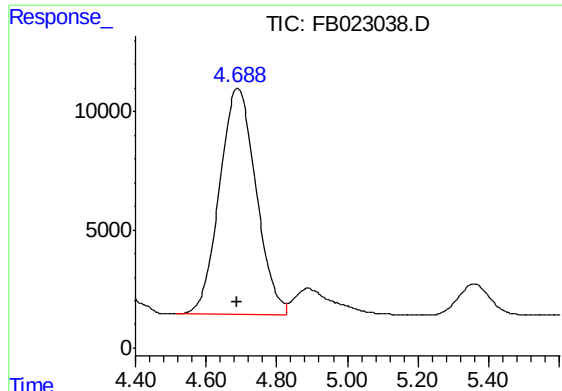


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 687928
Conc: 21.39 ng/ml

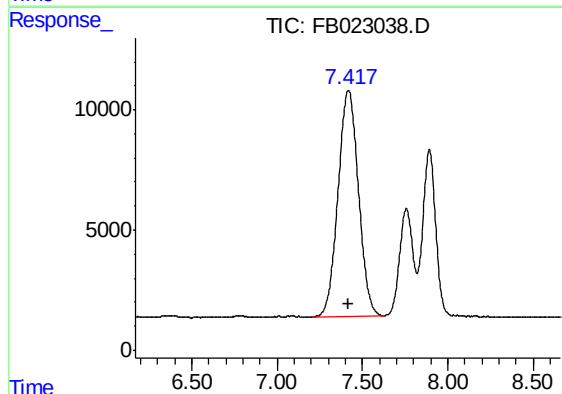


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 784307
Conc: 22.22 ng/ml

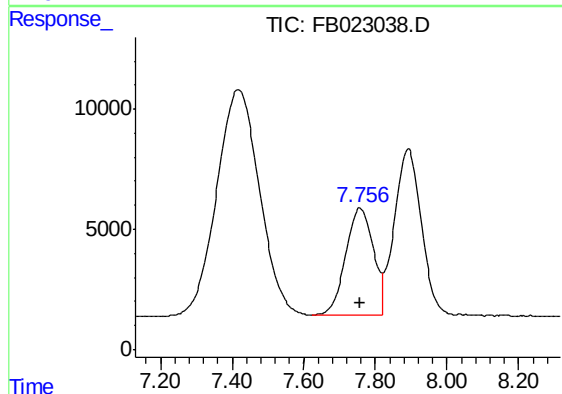


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 242045
Conc: 6.96 ng/ml

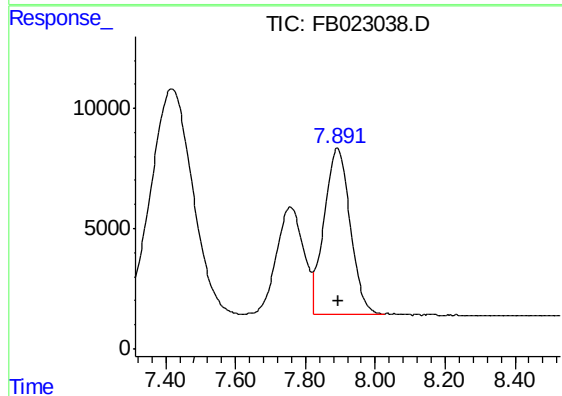


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.001 min
Response: 360756
Conc: 8.33 ng/ml

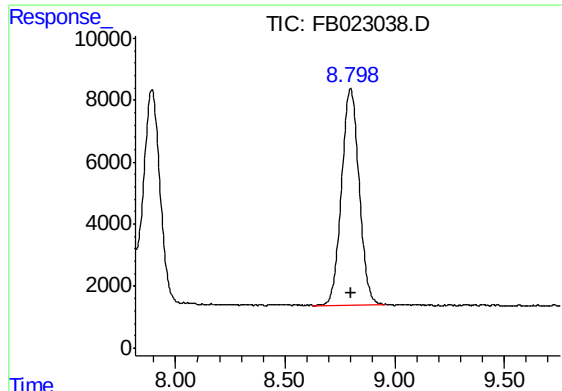


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 387234
Conc: 17.20 ng/ml

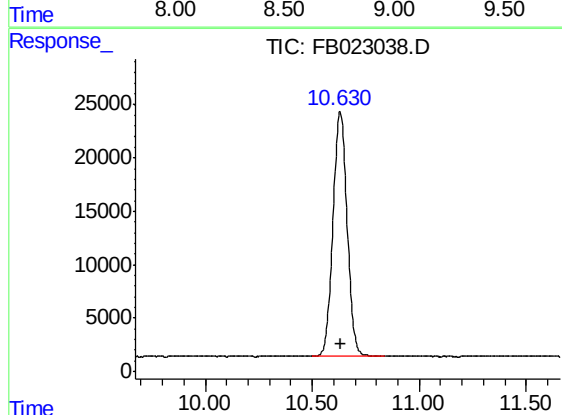


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1056934
Conc: 24.52 ng/ml

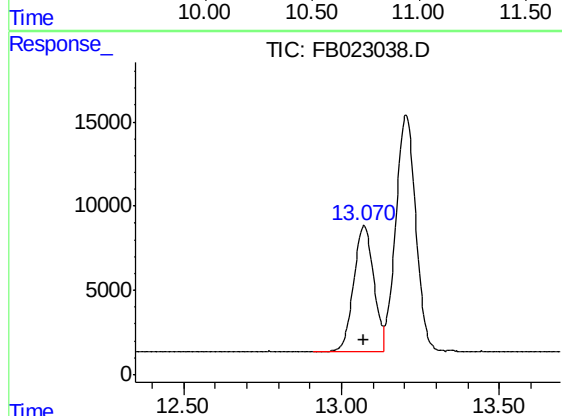


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 330730
Conc: 8.28 ng/ml

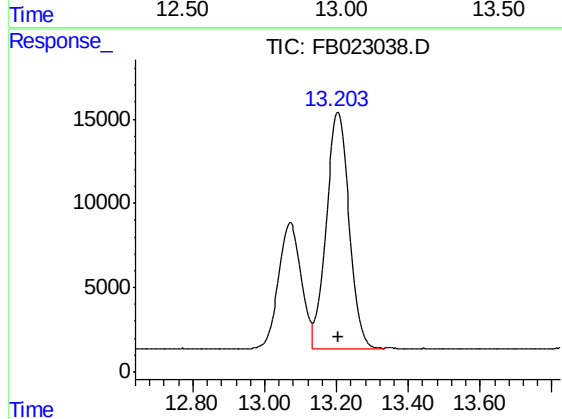


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 621422
Conc: 16.45 ng/ml

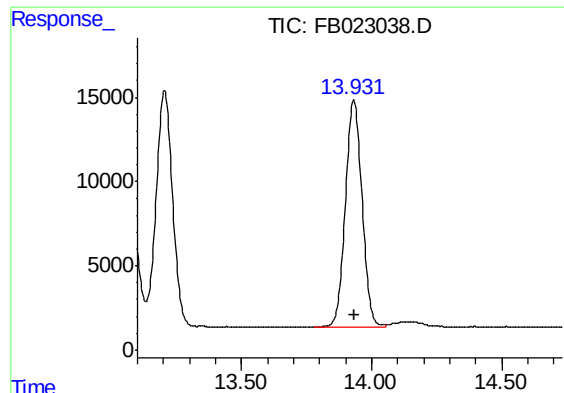

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 601660
Conc: 16.88 ng/ml

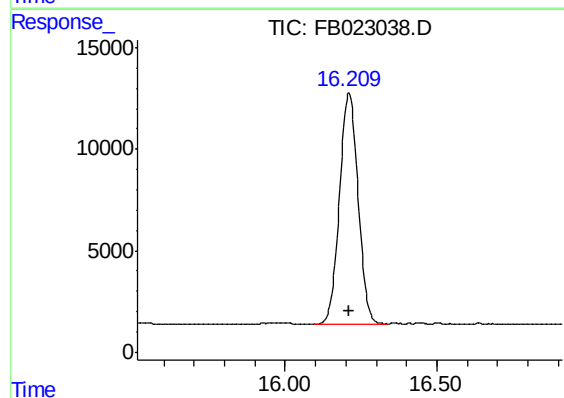

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 483553
Conc: 17.05 ng/ml