

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111919\
 Data File : FB023042.D
 Signal(s) : FID2B.CH
 Acq On : 19 Nov 2019 17:48
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 20 00:29:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	501253	22.266 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	960222	29.851 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1162162	32.922 ng/ml
3) t n-Heptane	7.758	368598	10.596 ng/ml
4) t Benzene	7.892	465985	10.758 ng/ml
6) t Toluene	10.631	1383098	32.083 ng/ml
7) t Ethylbenzene	13.071	432513	10.834 ng/ml
8) t m-Xylene	13.204	812346	21.509 ng/ml
9) t O-Xylene	13.932	772727	21.681 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	655453	23.113 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111919\
Data File : FB023042.D
Signal(s) : FID2B.CH
Acq On : 19 Nov 2019 17:48
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 20 00:29:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

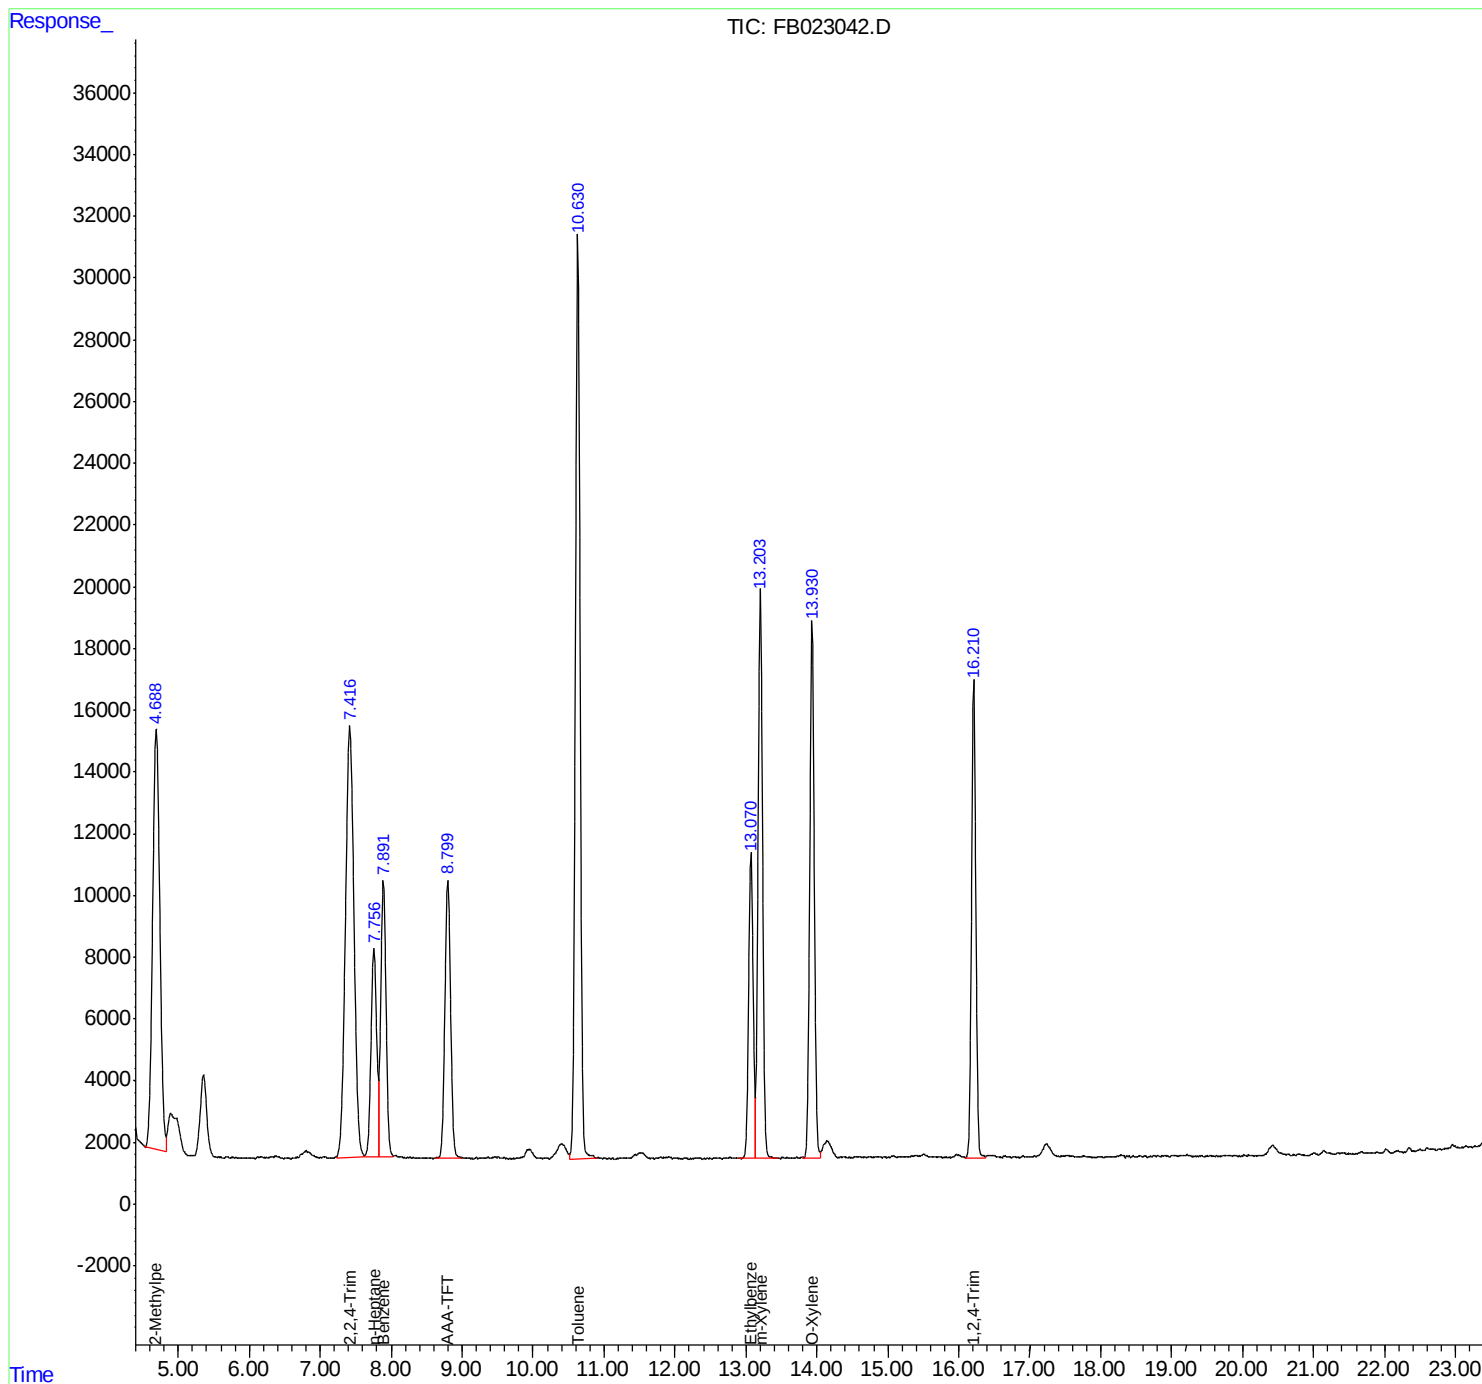

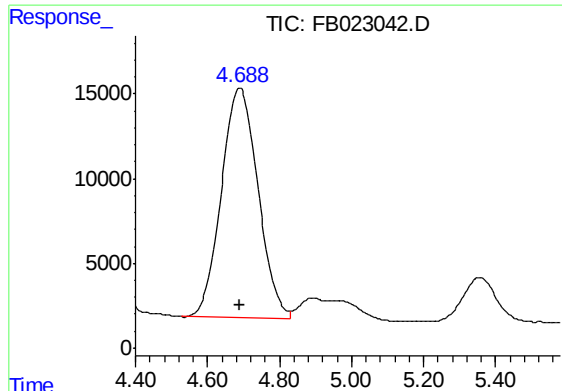


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 960222
Conc: 29.85 ng/ml

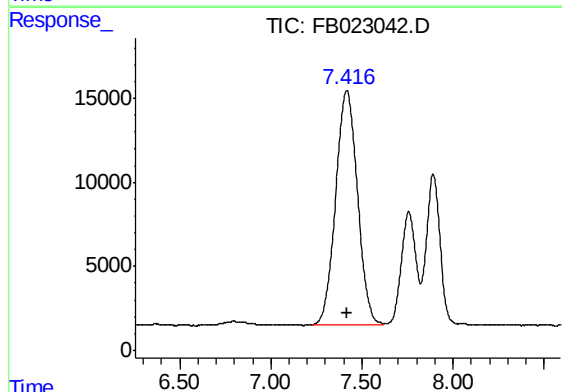


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 1162162
Conc: 32.92 ng/ml

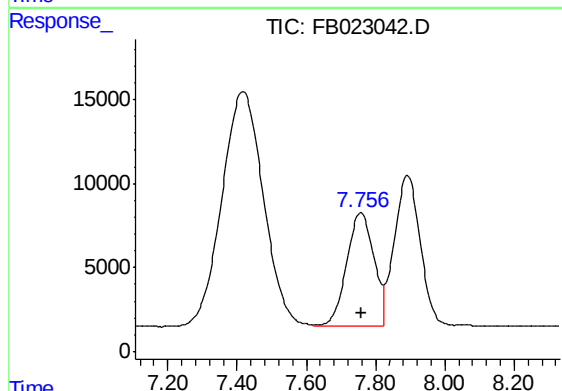


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 368598
Conc: 10.60 ng/ml

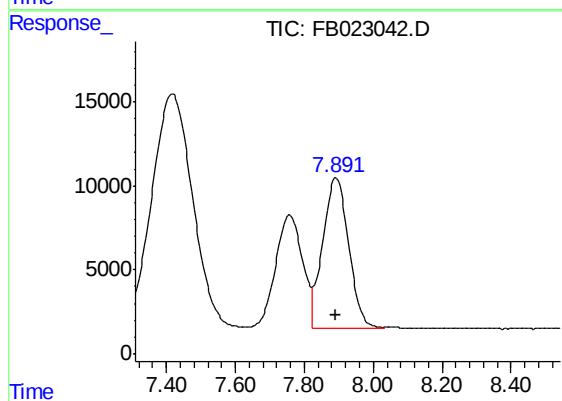


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 465985
Conc: 10.76 ng/ml

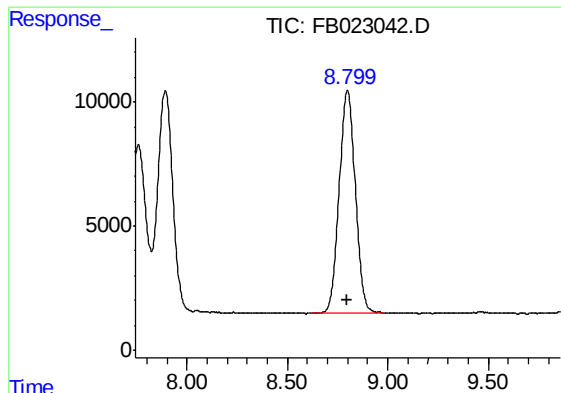


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 501253
Conc: 22.27 ng/ml

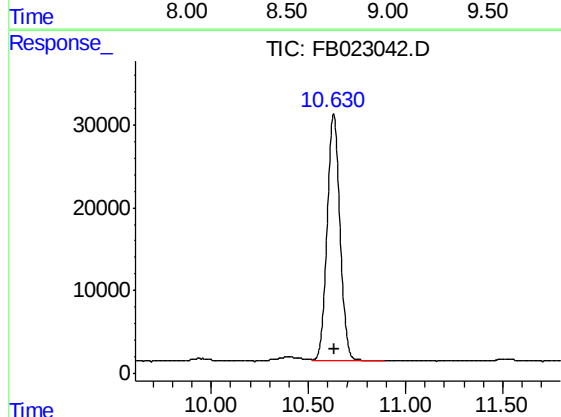


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1383098
Conc: 32.08 ng/ml

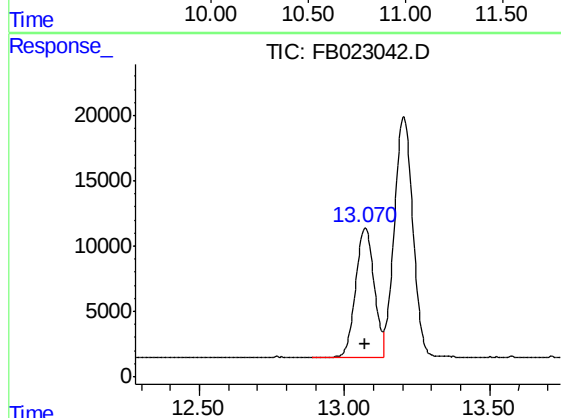


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 432513
Conc: 10.83 ng/ml

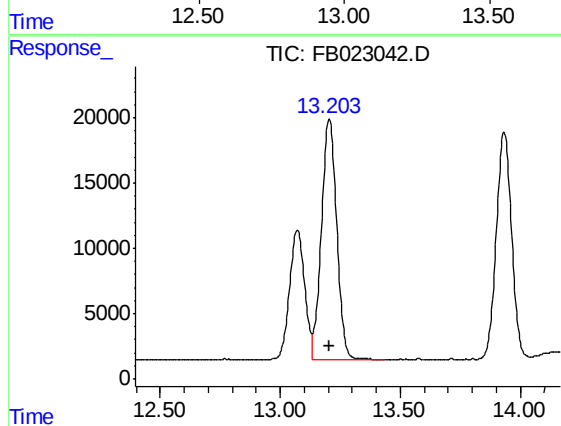


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 812346
Conc: 21.51 ng/ml

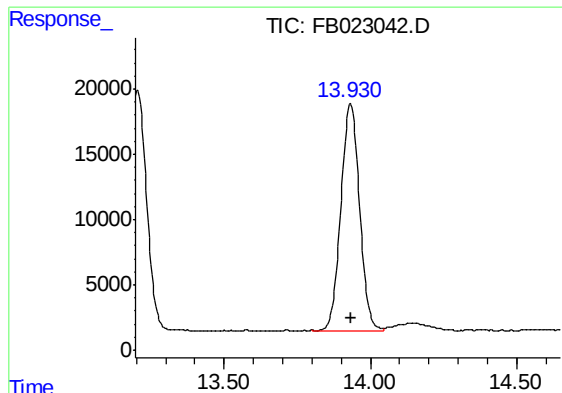

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 772727
Conc: 21.68 ng/ml

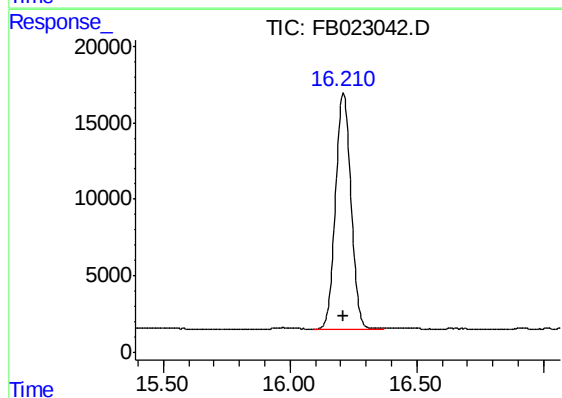

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 655453
Conc: 23.11 ng/ml