

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111919\
 Data File : FB023037.D
 Signal(s) : FID2B.CH
 Acq On : 19 Nov 2019 15:00
 Operator : DD/AJ
 Sample : K5916-01MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Nov 20 00:28:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
 Quant Title :
 QLast Update : Thu Oct 31 14:57:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	412673	18.331 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	737424	22.925 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	835277	23.662 ng/ml
3) t n-Heptane	7.757	264815	7.613 ng/ml
4) t Benzene	7.891	400657	9.250 ng/ml
6) t Toluene	10.630	1150310	26.683 ng/ml
7) t Ethylbenzene	13.070	362778	9.087 ng/ml
8) t m-Xylene	13.204	683959	18.110 ng/ml
9) t O-Xylene	13.932	659142	18.494 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	537507	18.954 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111919\
Data File : FB023037.D
Signal(s) : FID2B.CH
Acq On : 19 Nov 2019 15:00
Operator : DD/AJ
Sample : K5916-01MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Nov 20 00:28:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB103119.M
Quant Title :
QLast Update : Thu Oct 31 14:57:42 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

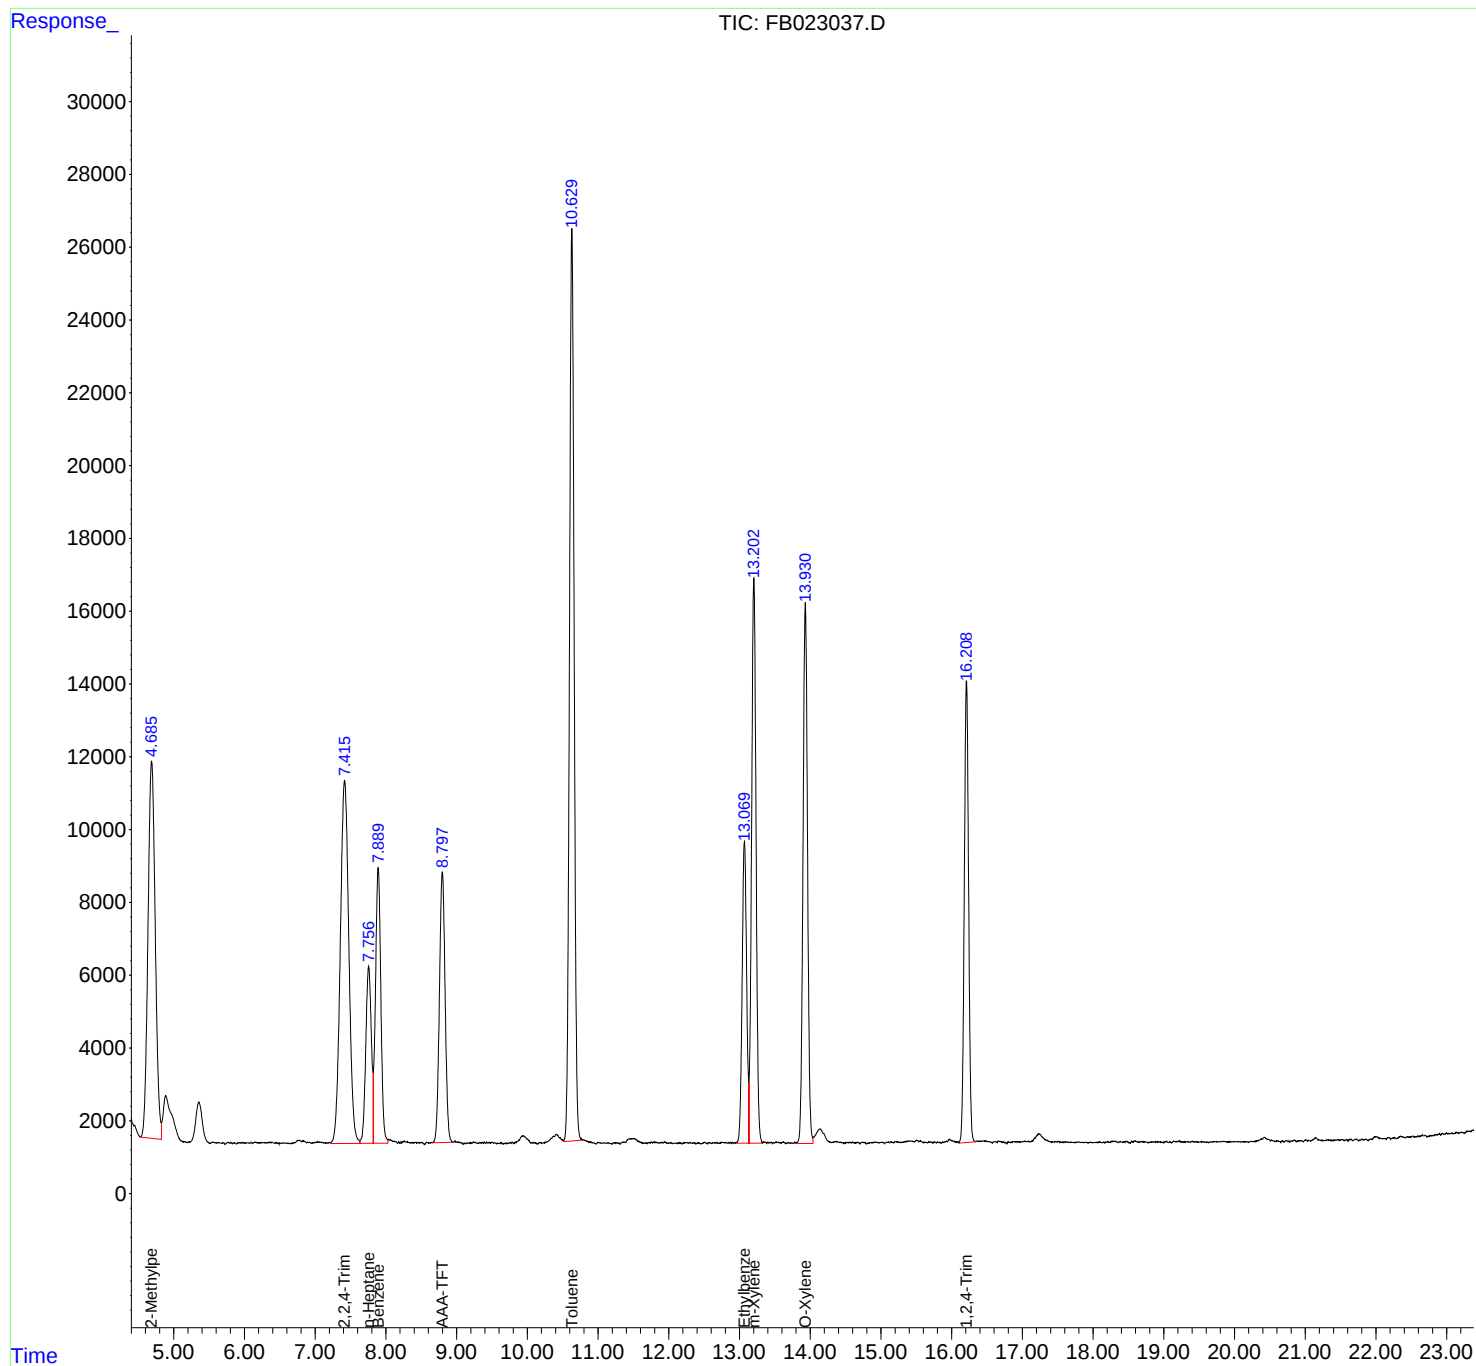

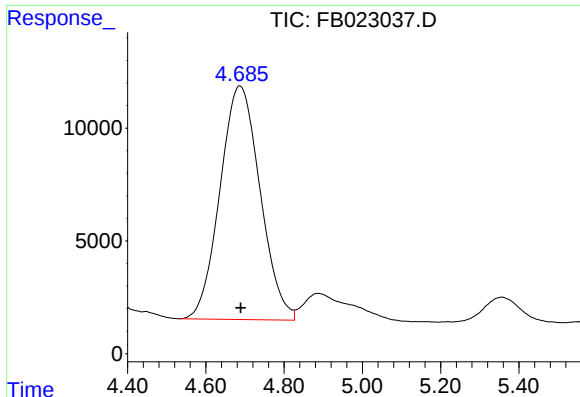


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 737424
Conc: 22.92 ng/ml

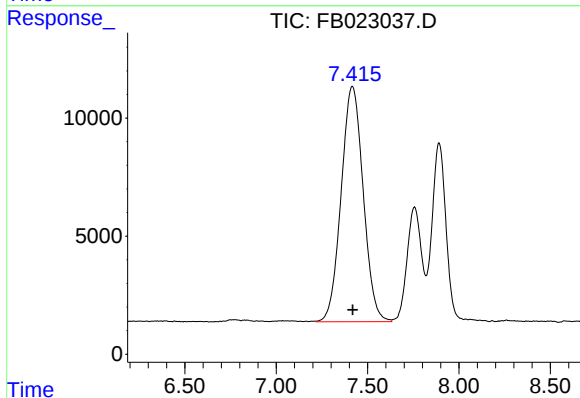


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 835277
Conc: 23.66 ng/ml

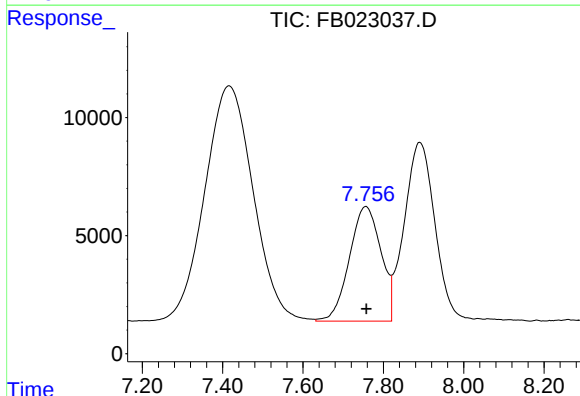


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 264815
Conc: 7.61 ng/ml

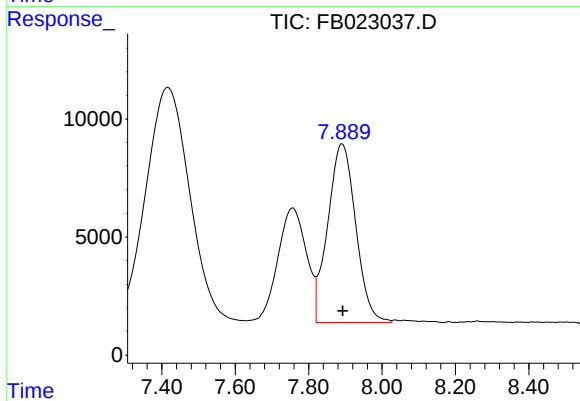


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 400657
Conc: 9.25 ng/ml

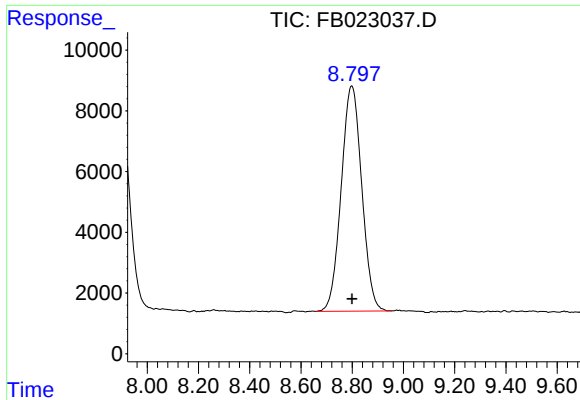


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 412673
Conc: 18.33 ng/ml

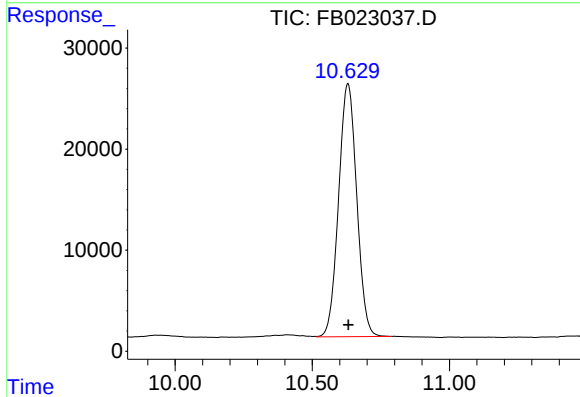


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.001 min
Response: 1150310
Conc: 26.68 ng/ml

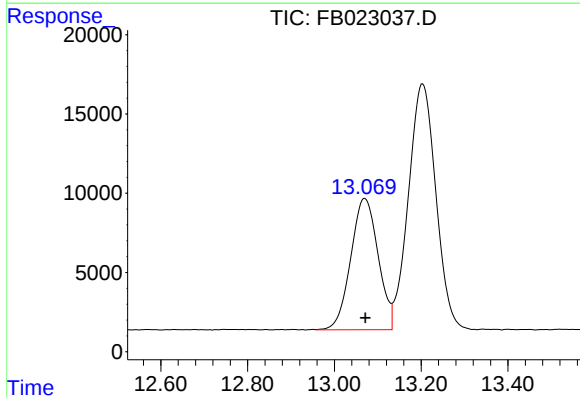


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.001 min
Response: 362778
Conc: 9.09 ng/ml

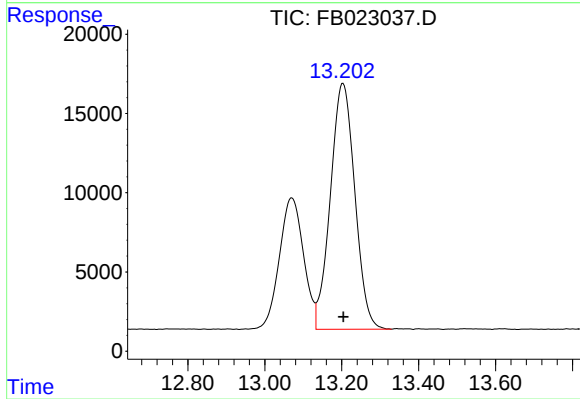


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: -0.001 min
Response: 683959
Conc: 18.11 ng/ml

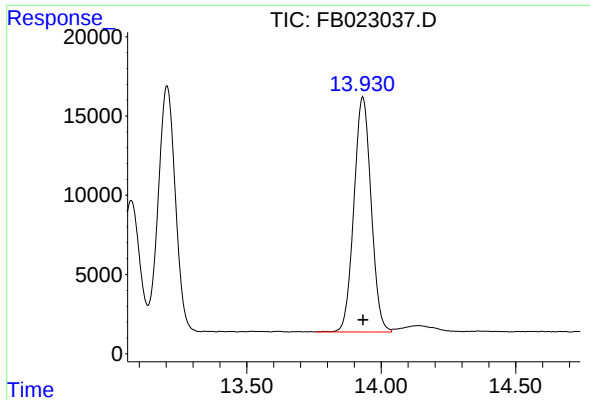

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 659142
Conc: 18.49 ng/ml

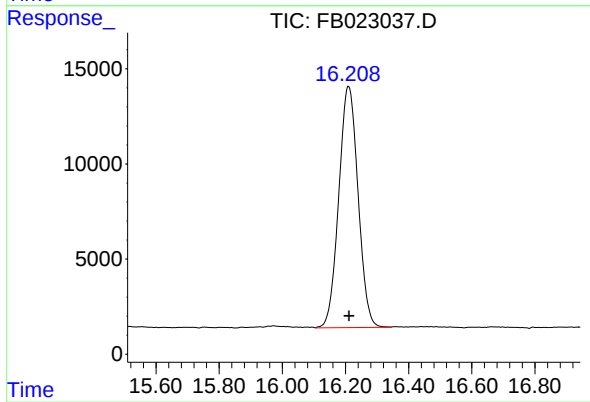

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 537507
Conc: 18.95 ng/ml