

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB112018\  
Data File : FB018823.D  
Signal(s) : FID2B.CH  
Acq On : 20 Nov 2018 8:43  
Operator : MJ/SJ  
Sample : VBF1120S1  
Misc : 5.00g/5.00ml DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Nov 20 11:06:37 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB110918.M  
Quant Title :  
QLast Update : Fri Nov 09 10:53:13 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 9.110  | 157656   | 18.277 ng/ml |
| Target Compounds            |        |          |              |
| 2) t 2,2,4-Trimethylpentane | 7.702  | 4168     | 0.284 ng/ml  |
| 4) t Benzene                | 8.189  | 4588     | 0.253 ng/ml  |
| 8) t m-Xylene               | 13.581 | 3887     | 0.234 ng/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB112018\  
Data File : FB018823.D  
Signal(s) : FID2B.CH  
Acq On : 20 Nov 2018 8:43  
Operator : MJ/SJ  
Sample : VBF1120S1  
Misc : 5.00g/5.00ml DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Nov 20 11:06:37 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB110918.M  
Quant Title :  
QLast Update : Fri Nov 09 10:53:13 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

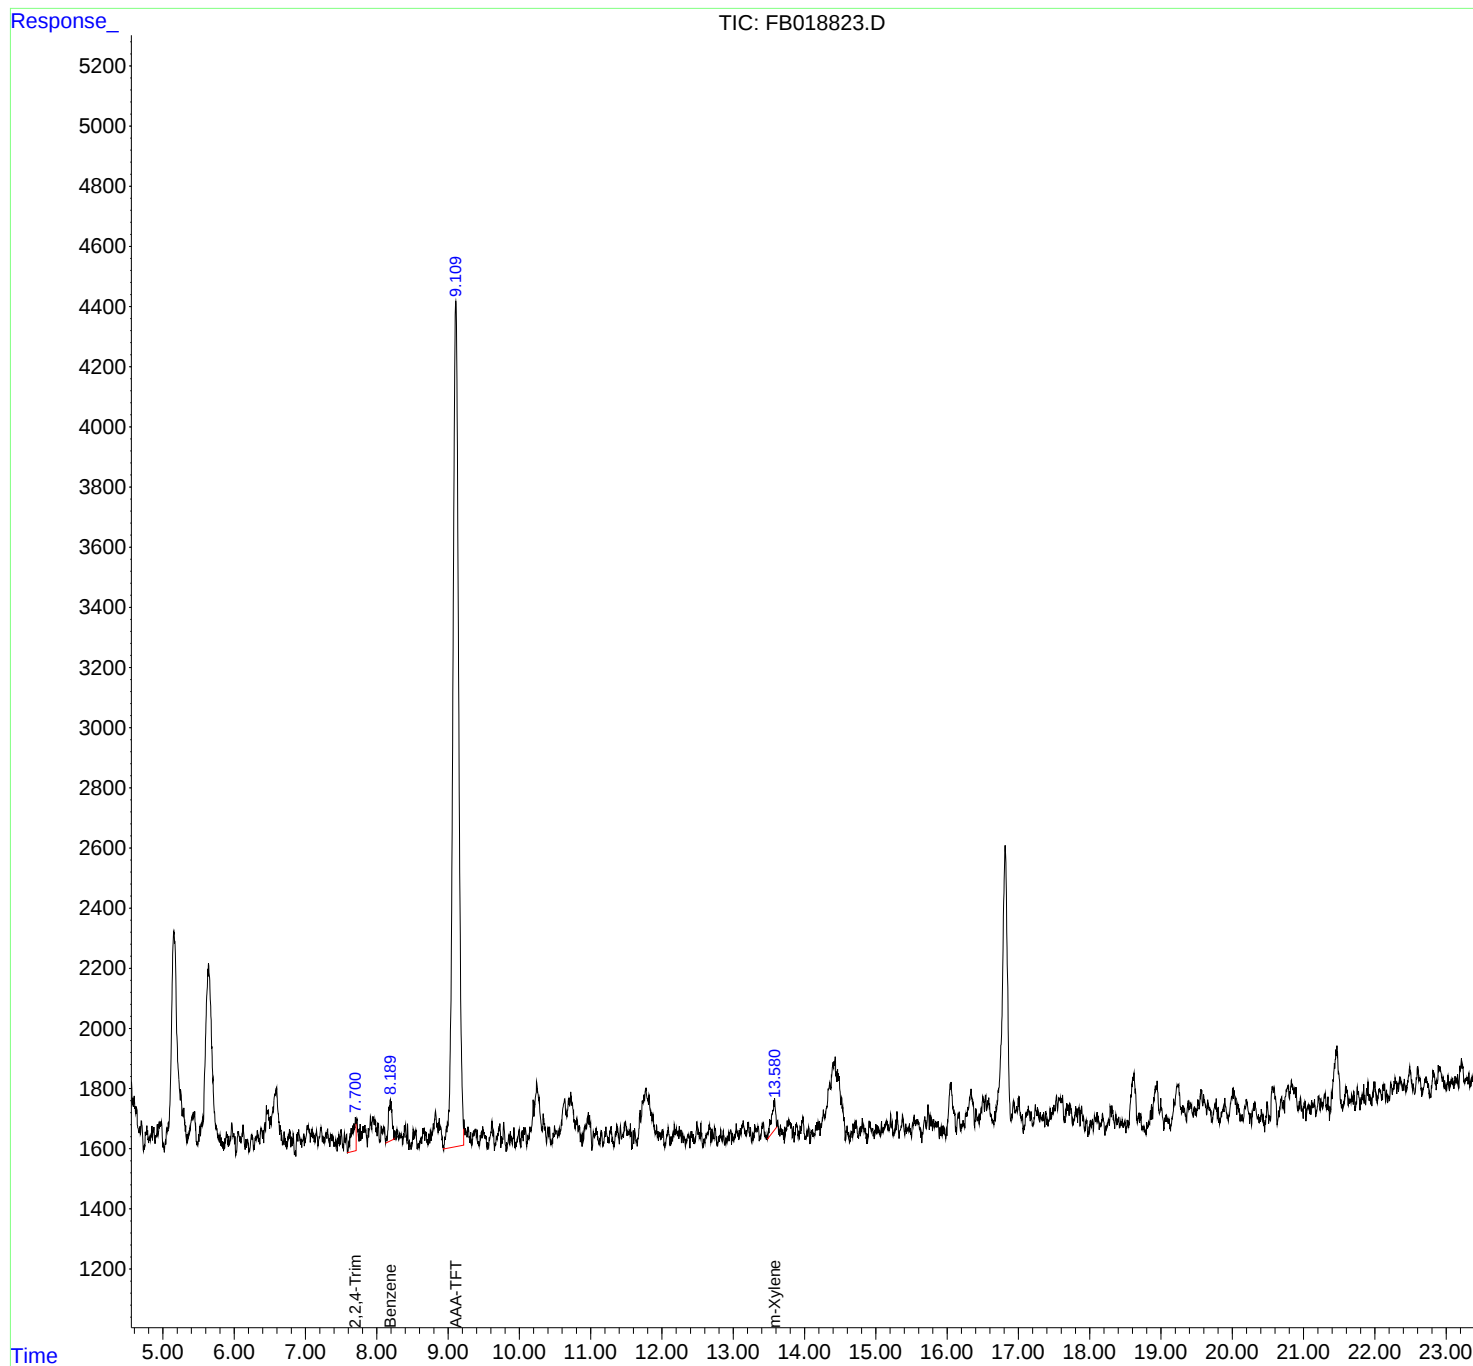

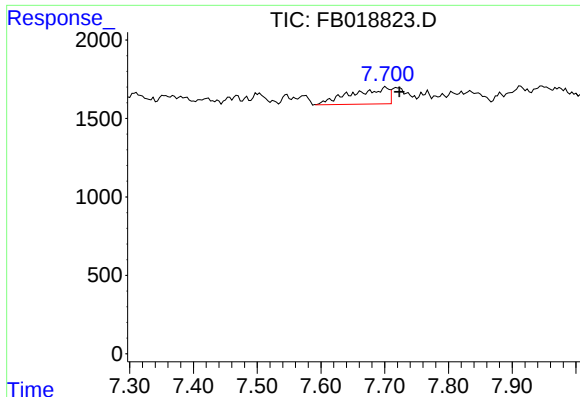


#2 2,2,4-Trimethylpentane

R.T.: 7.702 min  
Delta R.T.: -0.021 min  
Response: 4168  
Conc: 0.28 ng/ml

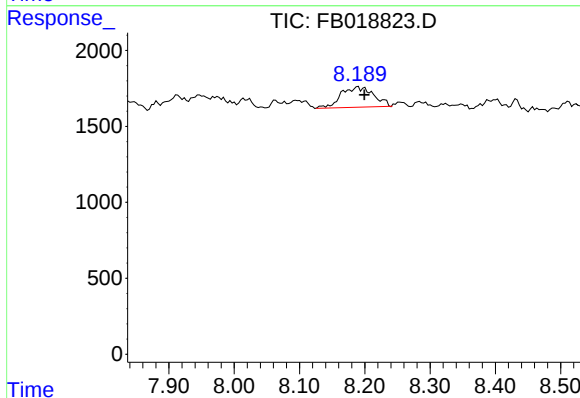


#4 Benzene

R.T.: 8.189 min  
Delta R.T.: -0.010 min  
Response: 4588  
Conc: 0.25 ng/ml

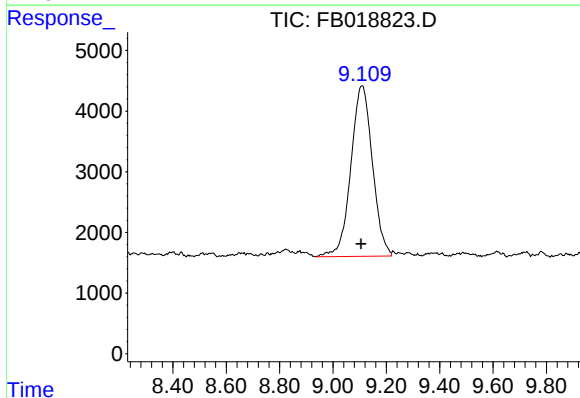

#5 AAA-TFT

R.T.: 9.110 min  
Delta R.T.: 0.005 min  
Response: 157656  
Conc: 18.28 ng/ml

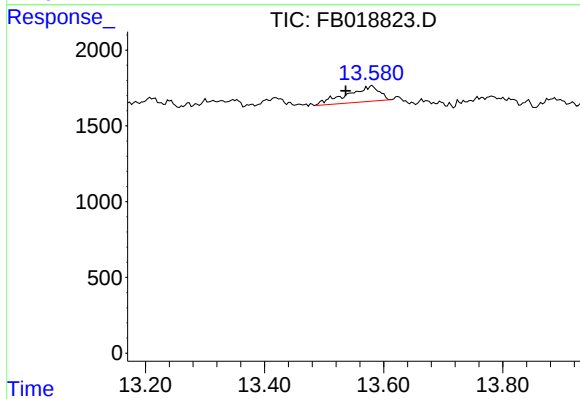

#8 m-Xylene

R.T.: 13.581 min  
Delta R.T.: 0.045 min  
Response: 3887  
Conc: 0.23 ng/ml