

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023068.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2019 17:12
 Operator : DD/AJ
 Sample : K5668-09MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 HD-01-112119MSD

Integration File: Calibration.e
 Quant Time: Nov 22 20:47:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	468778	19.084 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	926838	28.363 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1015924	29.134 ng/ml
3) t n-Heptane	7.758	331593	9.644 ng/ml
4) t Benzene	7.892	389521	9.349 ng/ml
6) t Toluene	10.630	1147905	28.495 ng/ml
7) t Ethylbenzene	13.071	370598	9.604 ng/ml
8) t m-Xylene	13.204	703993	19.346 ng/ml
9) t O-Xylene	13.932	663395	19.107 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	536748	19.140 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023068.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 17:12
Operator : DD/AJ
Sample : K5668-09MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

Integration File: Calibration.e
Quant Time: Nov 22 20:47:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

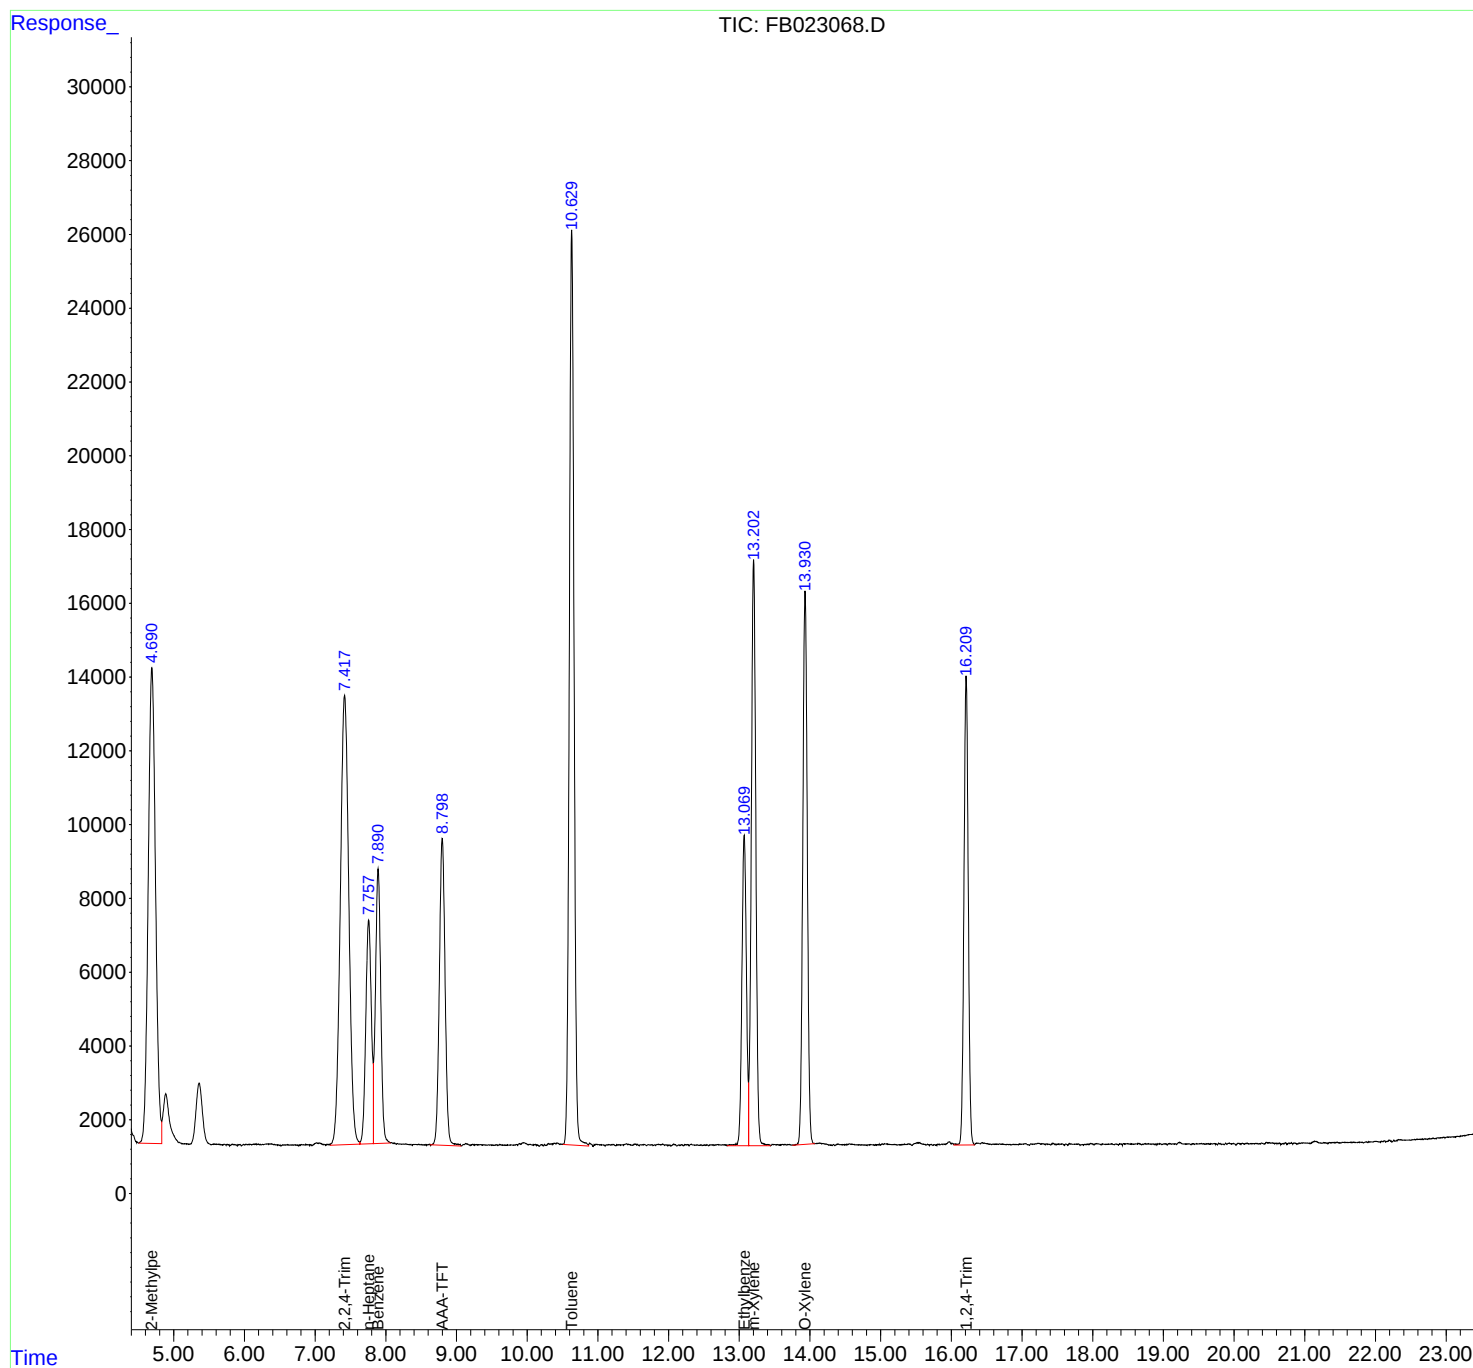


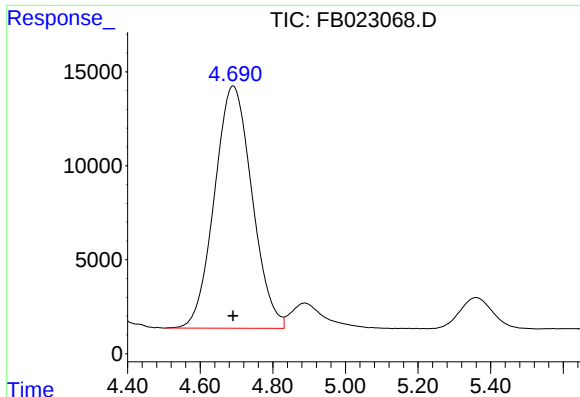

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 926838
Conc: 28.36 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

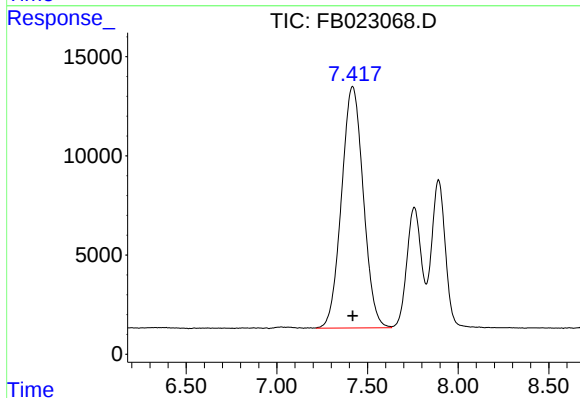


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1015924
Conc: 29.13 ng/ml

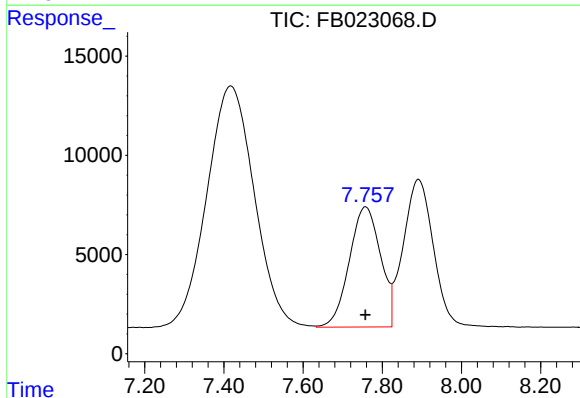


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 331593
Conc: 9.64 ng/ml

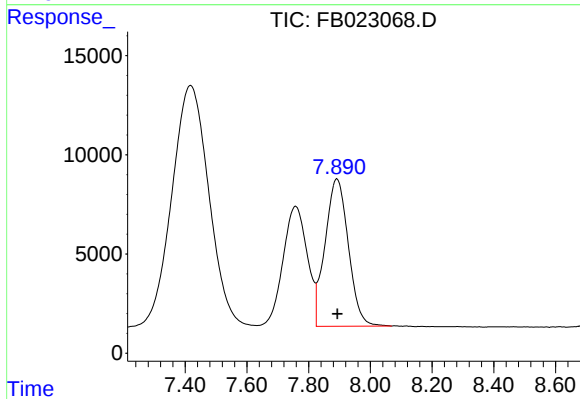

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 389521
Conc: 9.35 ng/ml

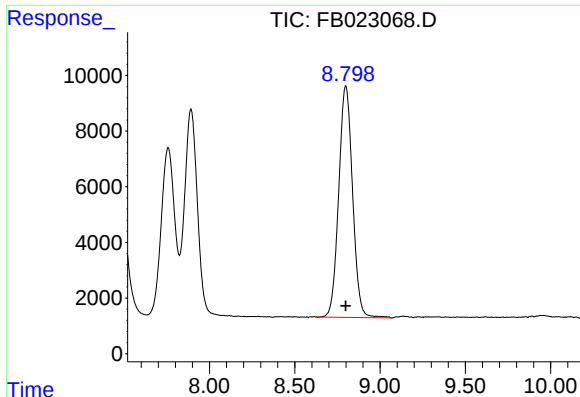

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 468778
Conc: 19.08 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

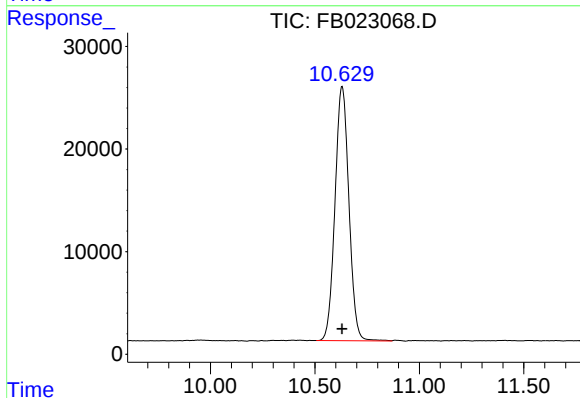


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1147905
Conc: 28.50 ng/ml

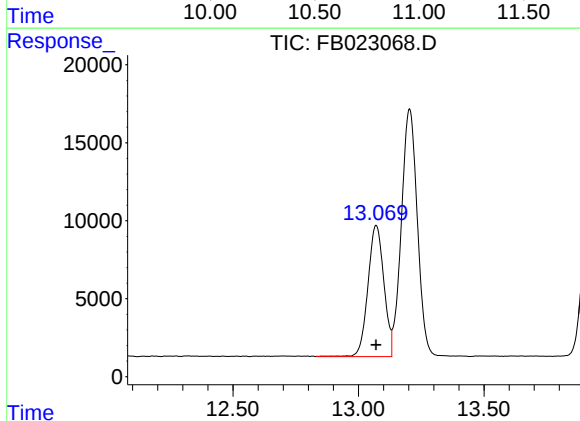


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 370598
Conc: 9.60 ng/ml

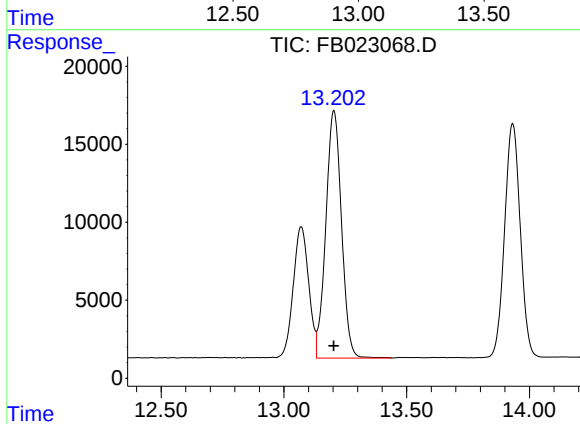

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 703993
Conc: 19.35 ng/ml

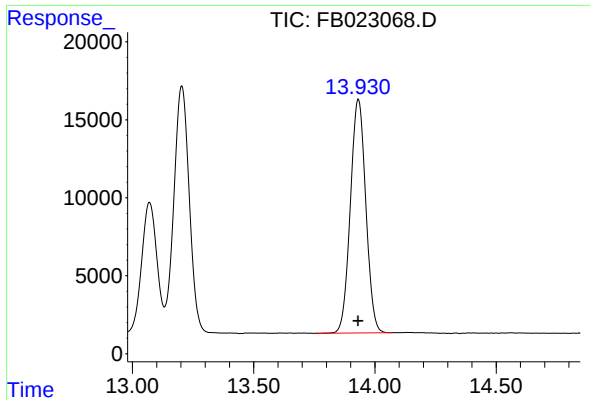

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 663395
Conc: 19.11 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

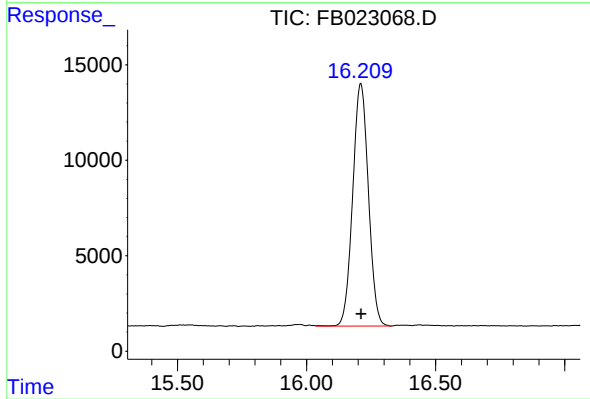

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 536748
Conc: 19.14 ng/ml