

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023070.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2019 18:13
 Operator : DD/AJ
 Sample : K5671-12
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-112119

Integration File: Calibration.e
 Quant Time: Nov 22 20:48:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	318497	12.966 ng/ml
Target Compounds			
6) t Toluene	10.632	3256	0.081 ng/ml
7) t Ethylbenzene	13.065	2982	0.077 ng/ml
8) t m-Xylene	13.201	4113	0.113 ng/ml
9) t O-Xylene	13.934	7505	0.216 ng/ml
10) t 1,2,4-Trimethylbenzene	16.214	5679	0.203 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023070.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 18:13
Operator : DD/AJ
Sample : K5671-12
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-112119

Integration File: Calibration.e
Quant Time: Nov 22 20:48:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

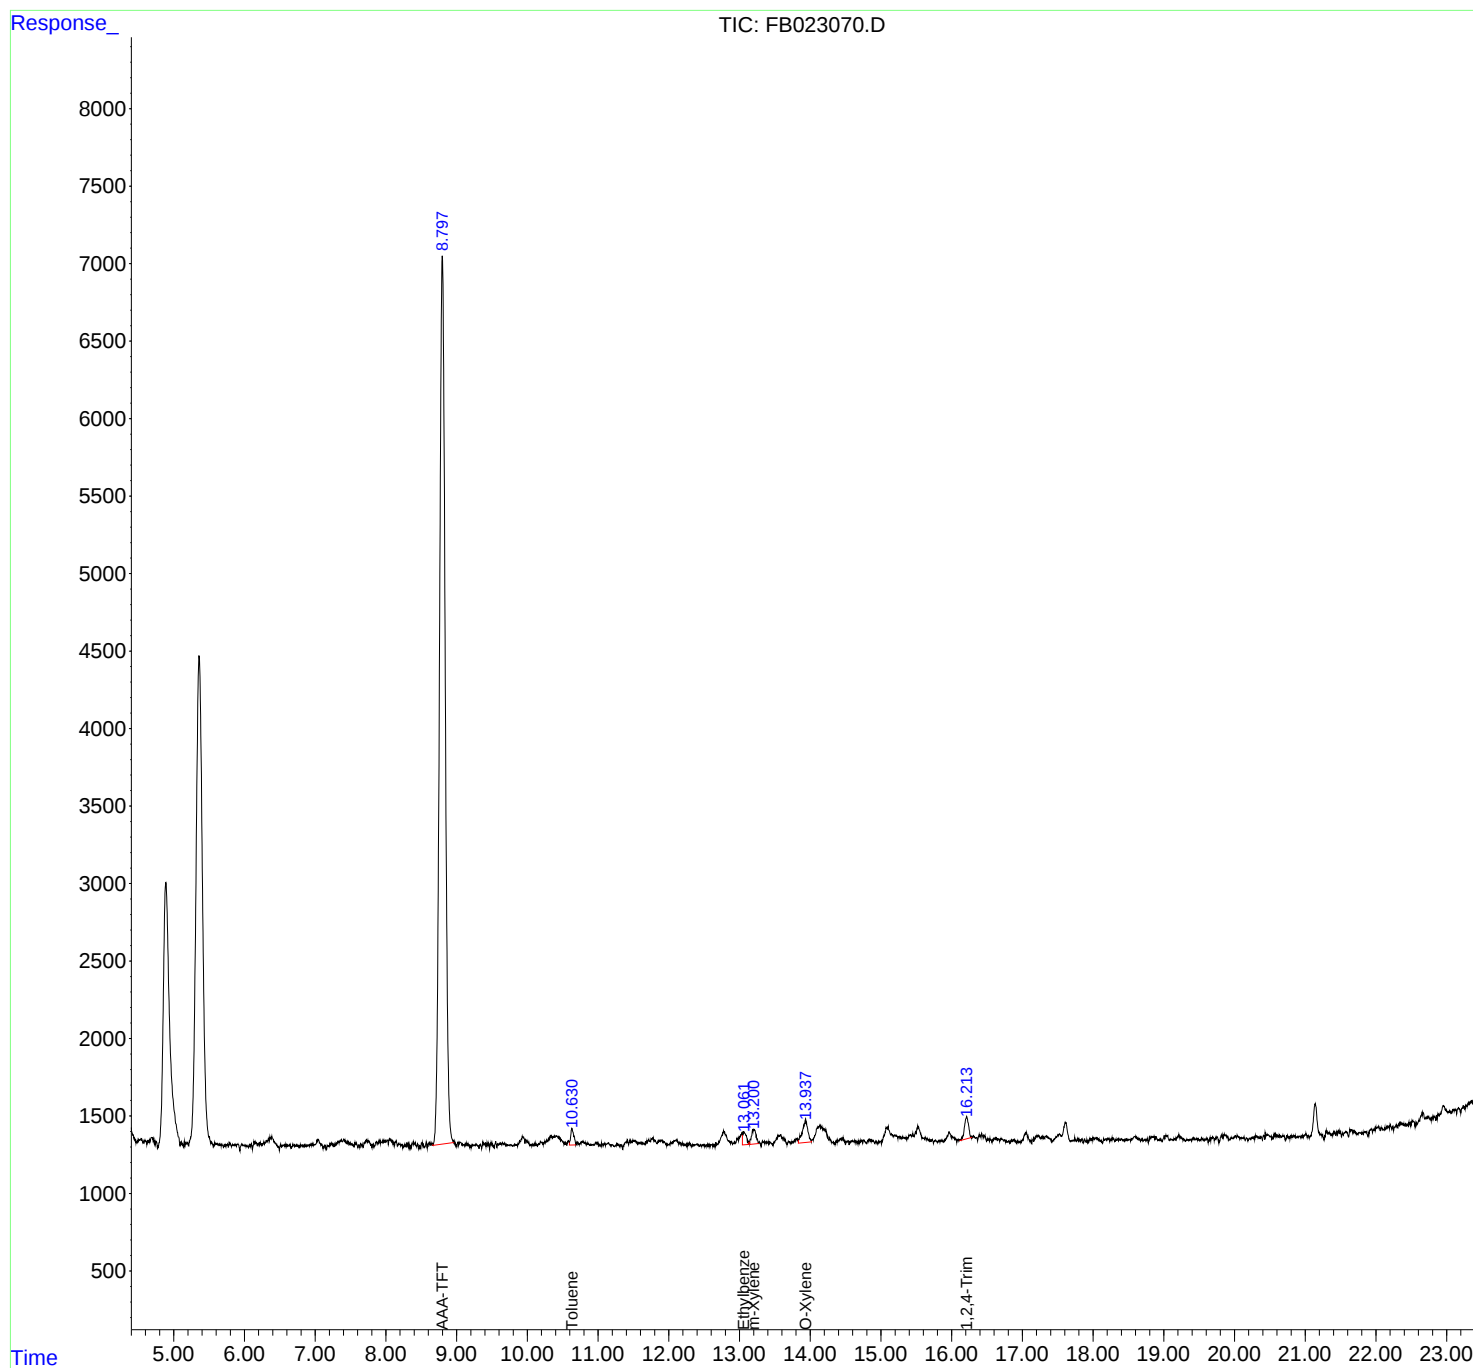


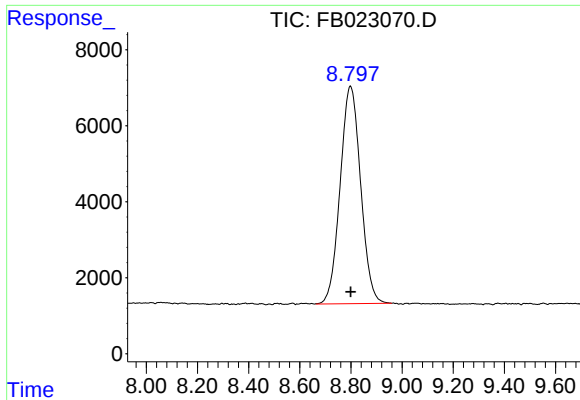

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 318497
Conc: 12.97 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-112119

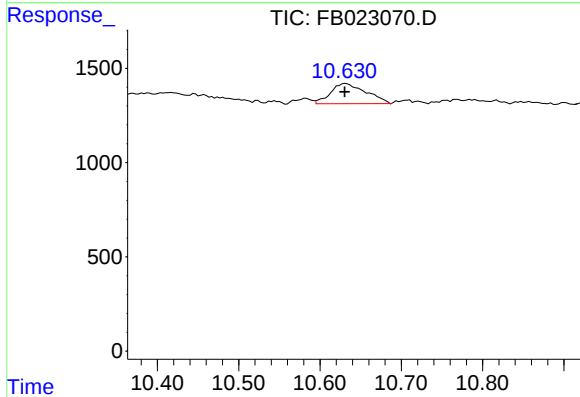


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.002 min
Response: 3256
Conc: 0.08 ng/ml

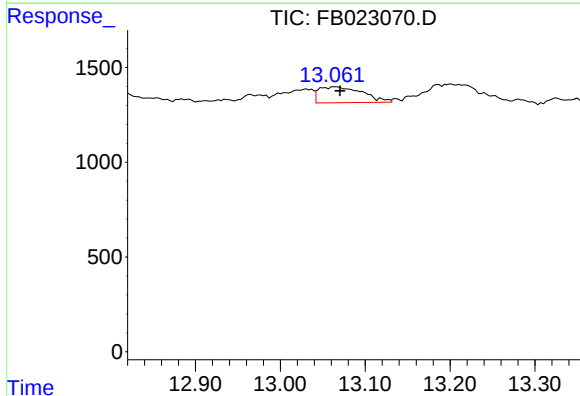


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.005 min
Response: 2982
Conc: 0.08 ng/ml

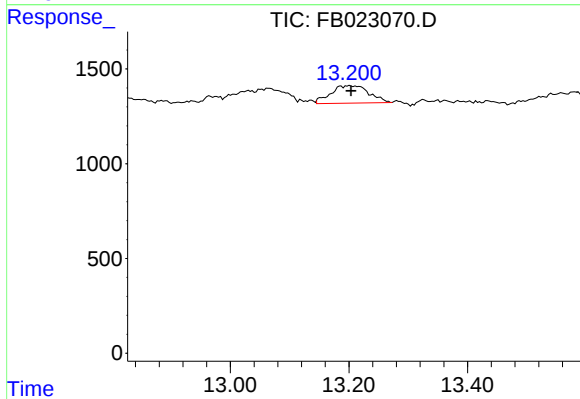

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 4113
Conc: 0.11 ng/ml

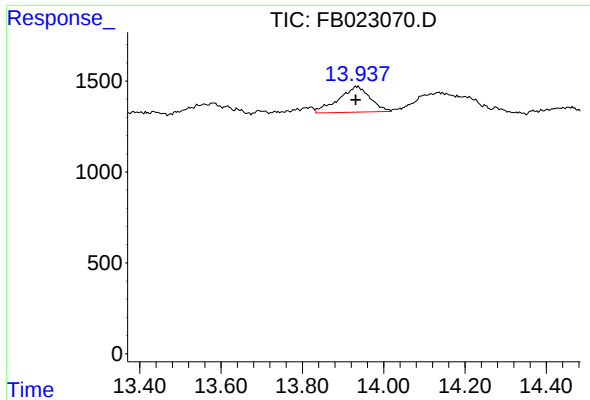

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.002 min
Response: 7505
Conc: 0.22 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-112119

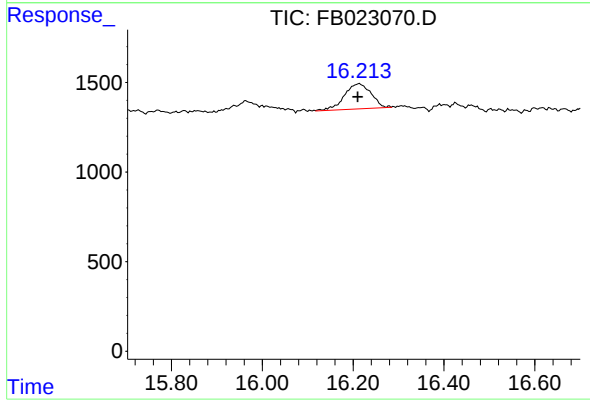

#10 1,2,4-Trimethylbenzene

R.T.: 16.214 min
Delta R.T.: 0.004 min
Response: 5679
Conc: 0.20 ng/ml