

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023071.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2019 18:43
 Operator : DD/AJ
 Sample : K5670-10
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-01-112119

Integration File: Calibration.e
 Quant Time: Nov 22 20:48:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	129822	5.285 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.388	1889	0.054 ng/ml
6) t Toluene	10.645	3839	0.095 ng/ml
7) t Ethylbenzene	13.055	7135	0.185 ng/ml
8) t m-Xylene	13.202	10887	0.299 ng/ml
9) t O-Xylene	13.925	2837	0.082 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	2441	0.087 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023071.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 18:43
Operator : DD/AJ
Sample : K5670-10
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-01-112119

Integration File: Calibration.e
Quant Time: Nov 22 20:48:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

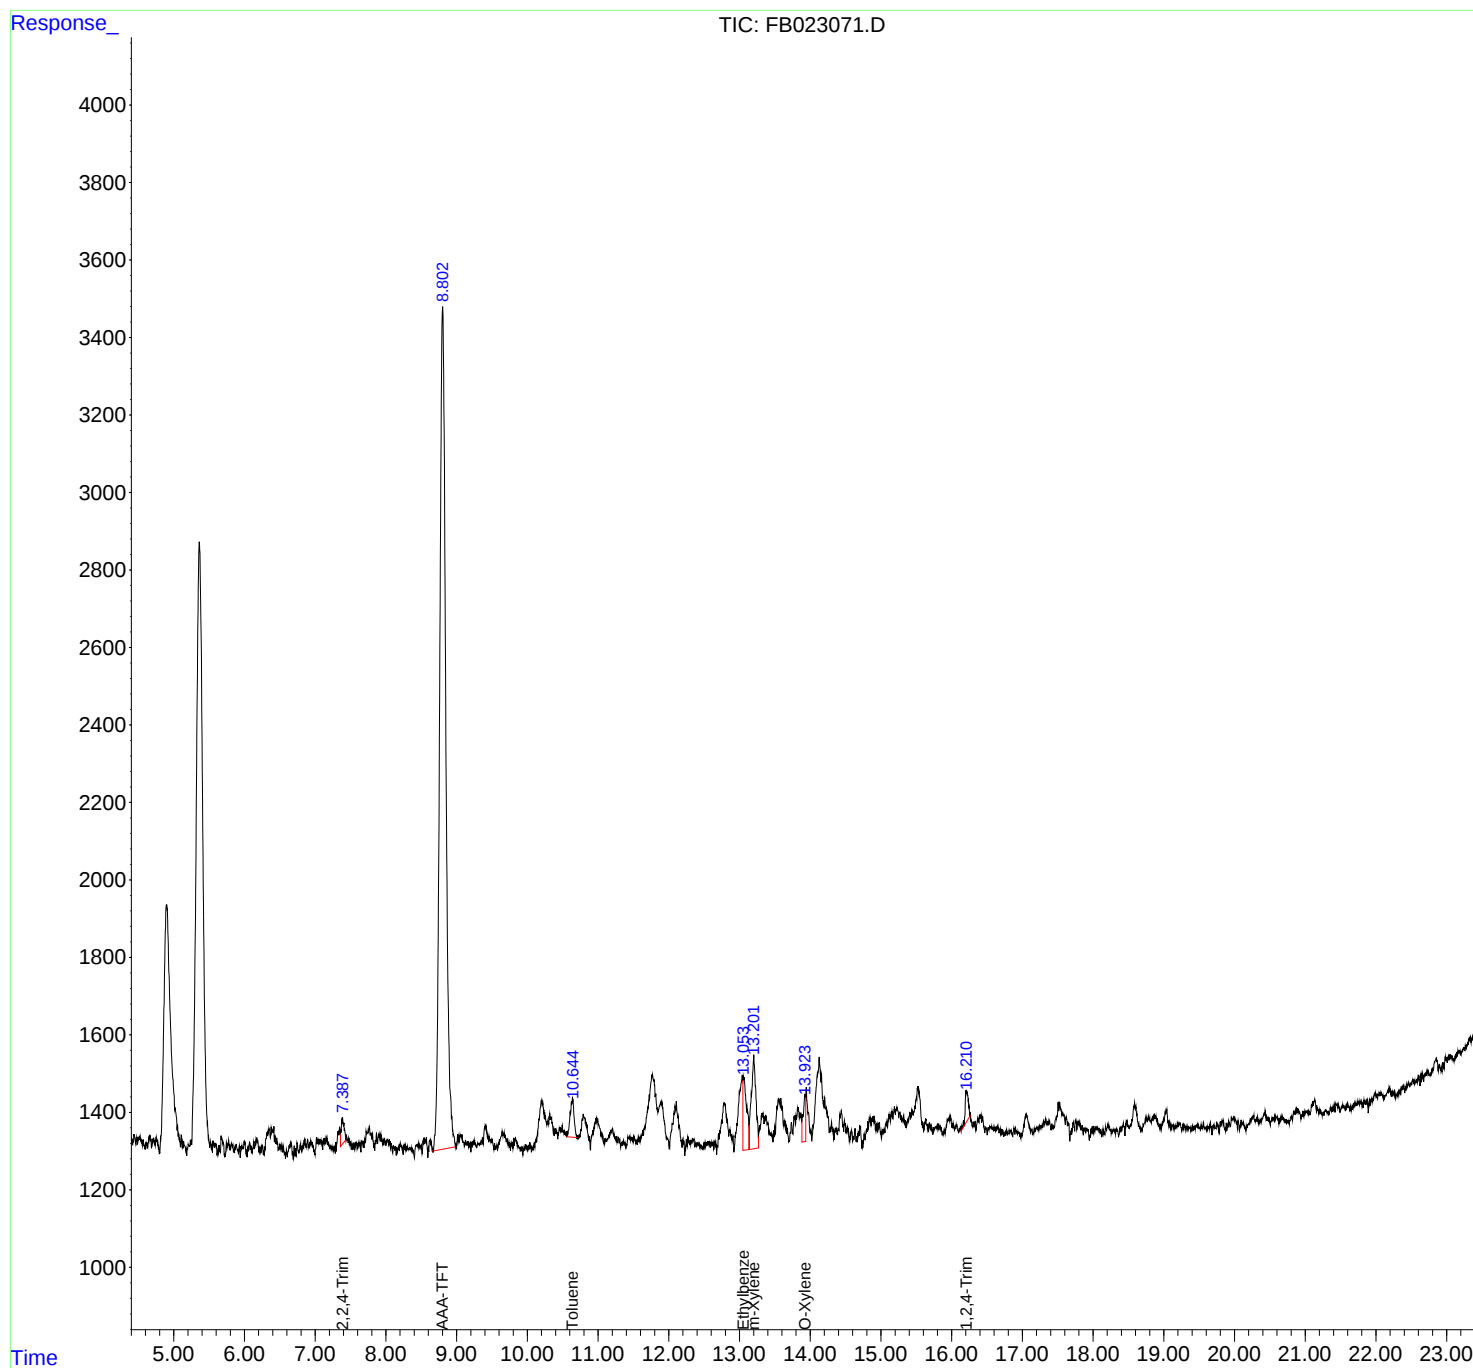


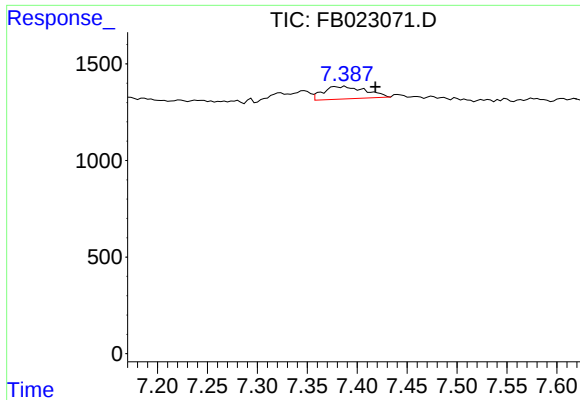

#2 2,2,4-Trimethylpentane


R.T.: 7.388 min
Delta R.T.: -0.030 min
Response: 1889
Conc: 0.05 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-01-112119

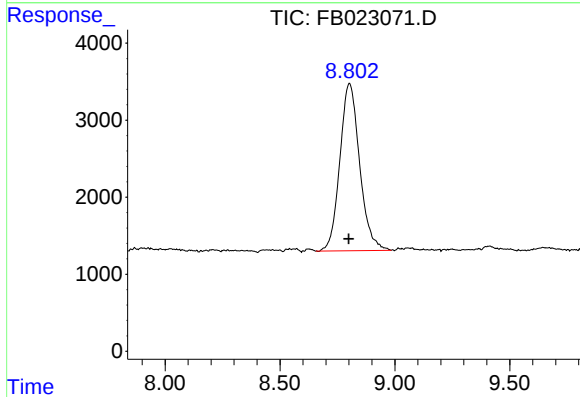


#5 AAA-TFT

R.T.: 8.803 min
Delta R.T.: 0.004 min
Response: 129822
Conc: 5.29 ng/ml

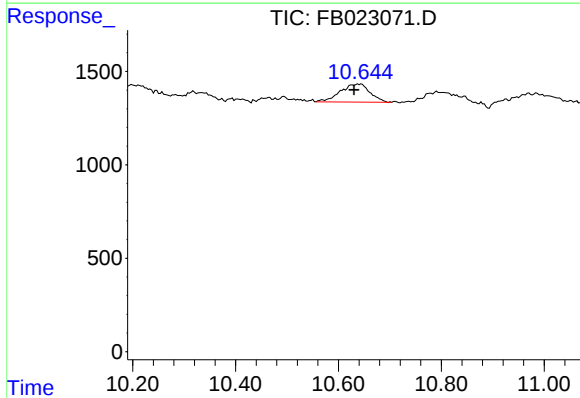


#6 Toluene

R.T.: 10.645 min
Delta R.T.: 0.015 min
Response: 3839
Conc: 0.10 ng/ml

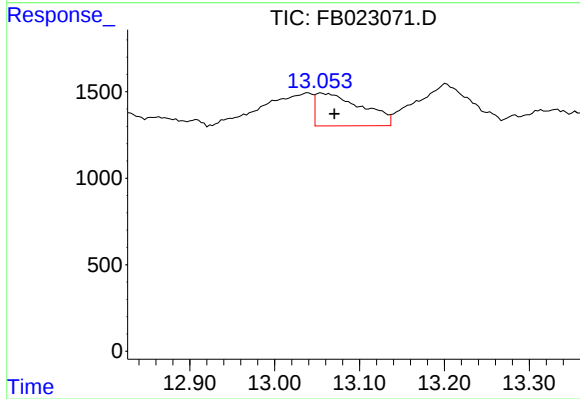

#7 Ethylbenzene


R.T.: 13.055 min
Delta R.T.: -0.015 min
Response: 7135
Conc: 0.18 ng/ml

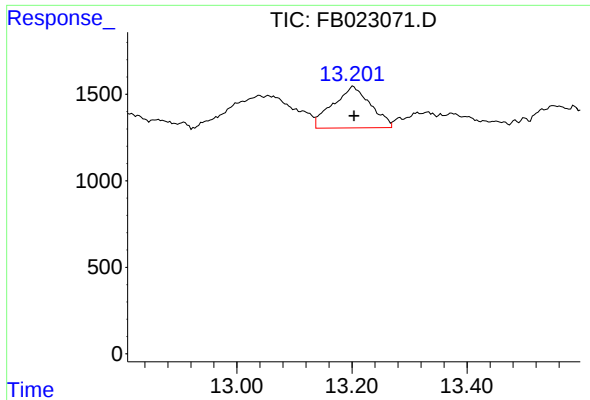

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 10887
Conc: 0.30 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-01-112119

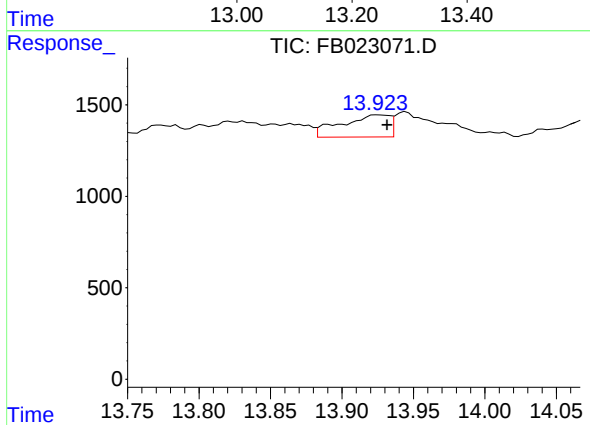

#9 o-Xylene

R.T.: 13.925 min
Delta R.T.: -0.006 min
Response: 2837
Conc: 0.08 ng/ml

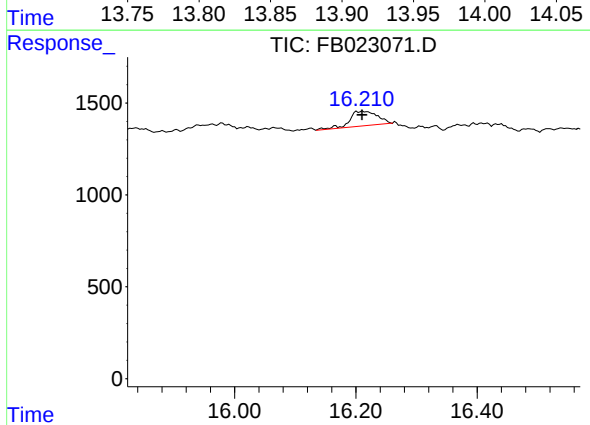

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.001 min
Response: 2441
Conc: 0.09 ng/ml