

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023073.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 19:44
Operator : DD/AJ
Sample : K5973-02
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 22 20:48:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	400032	16.285 ng/ml
Target Compounds			
6) t Toluene	10.636	1528	0.038 ng/ml
9) t O-Xylene	13.925	1581	0.046 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	2627	0.094 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023073.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 19:44
Operator : DD/AJ
Sample : K5973-02
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 22 20:48:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

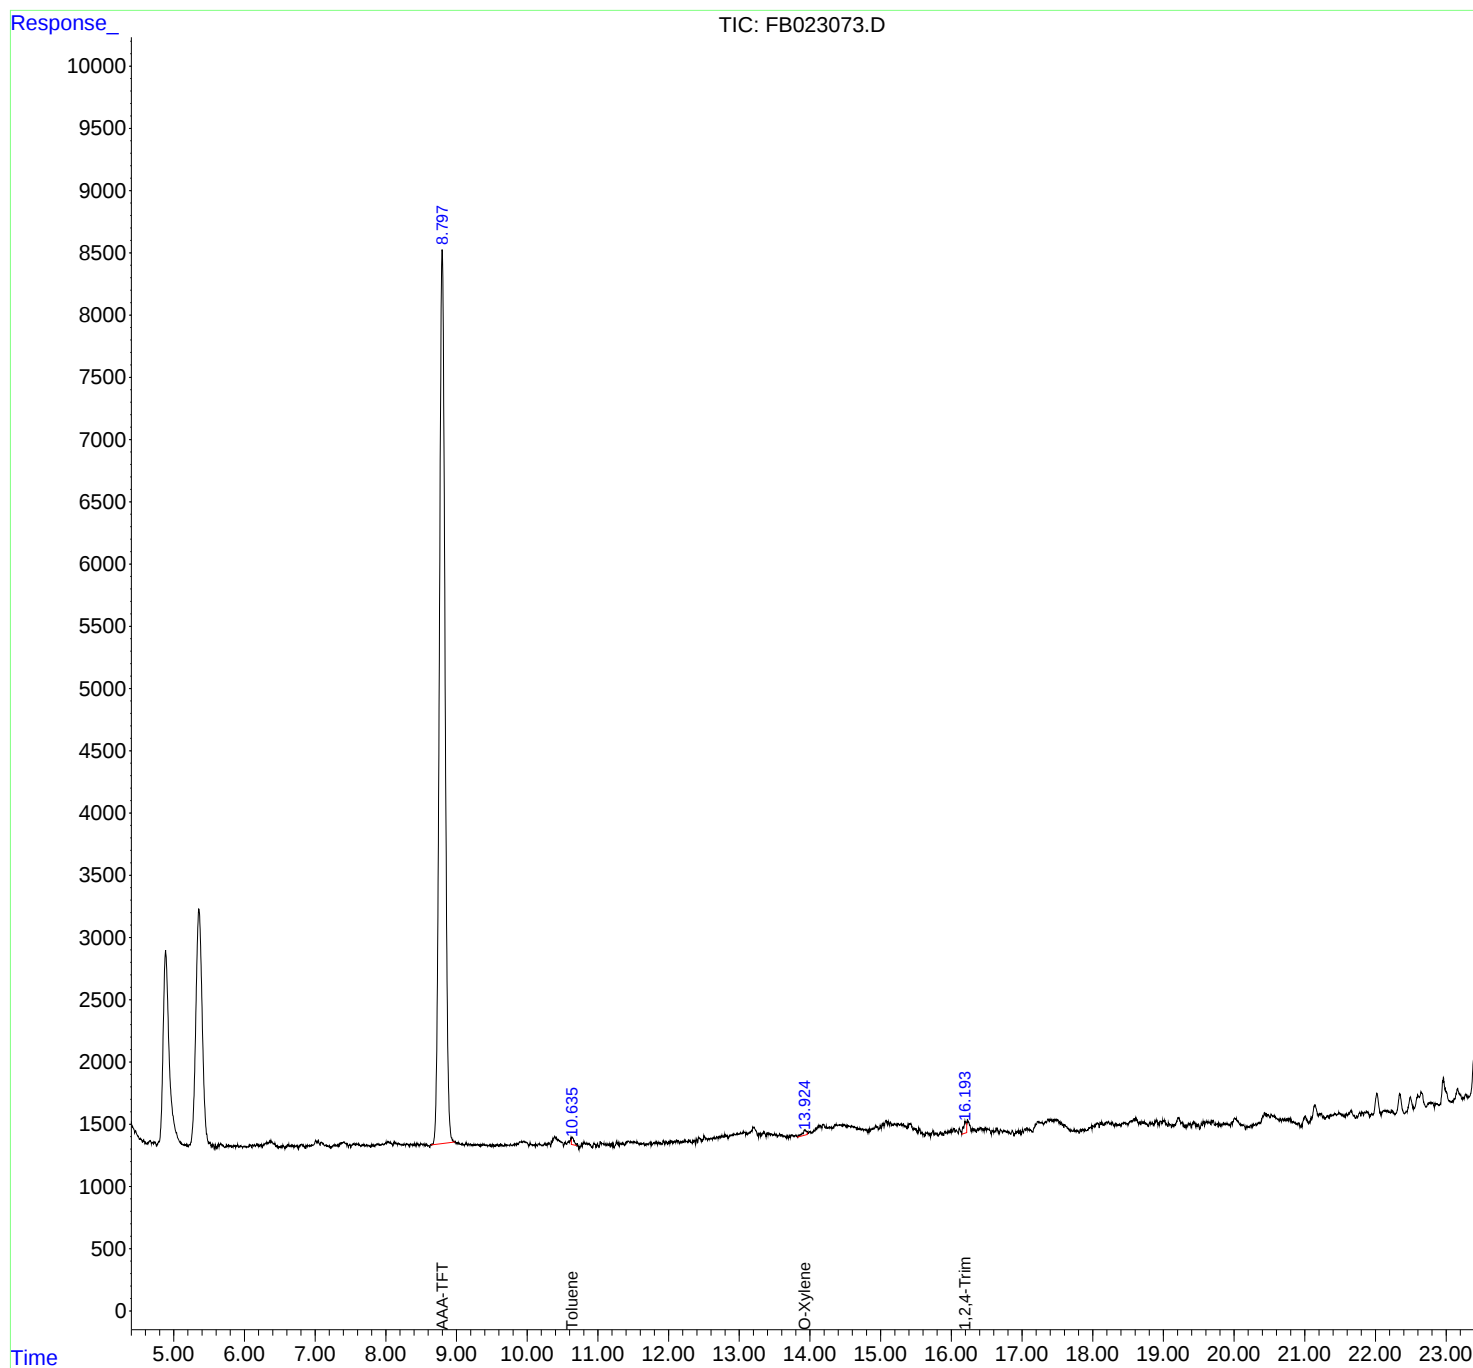


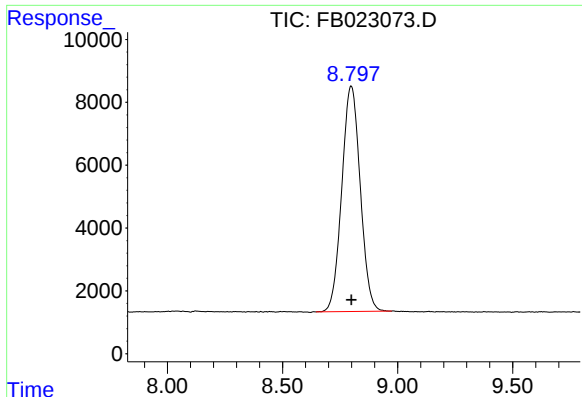

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 400032
Conc: 16.29 ng/ml

Instrument :
FID_B
ClientSampleId :

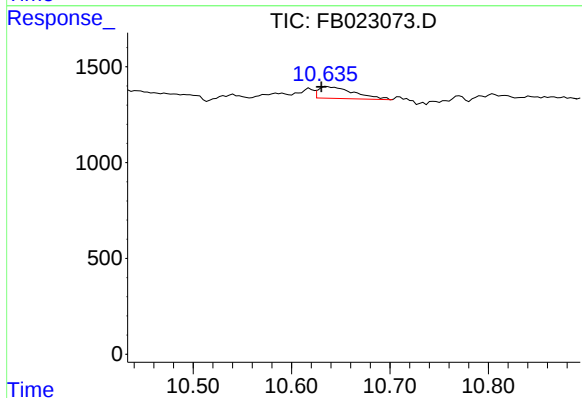


#6 Toluene

R.T.: 10.636 min
Delta R.T.: 0.006 min
Response: 1528
Conc: 0.04 ng/ml

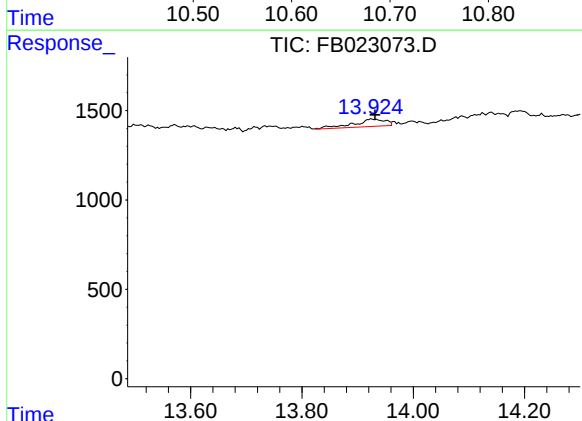

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.006 min
Response: 1581
Conc: 0.05 ng/ml

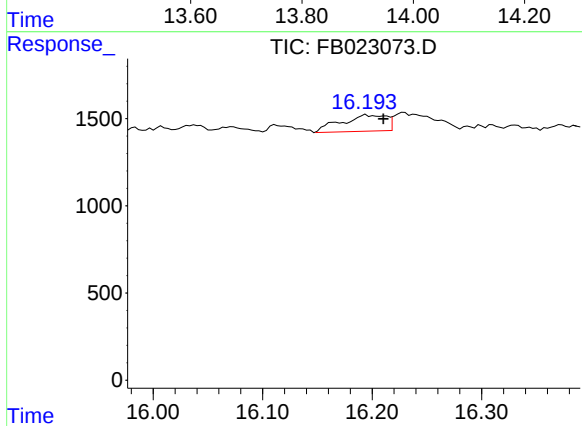

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.016 min
Response: 2627
Conc: 0.09 ng/ml