

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023076.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2019 21:15
 Operator : DD/AJ
 Sample : K5948-01
 Misc : 6.08g/5.00ml DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 B-1-0-6

Integration File: Calibration.e
 Quant Time: Nov 22 20:49:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.805	669828	27.269 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.677	113425	3.471 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	580108	16.636 ng/ml
4) t Benzene	7.889	616672	14.801 ng/ml
6) t Toluene	10.637	150368	3.733 ng/ml
8) t m-Xylene	13.199	50656	1.392 ng/ml
9) t O-Xylene	13.944	96006	2.765 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	87449	3.118 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023076.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 21:15
Operator : DD/AJ
Sample : K5948-01
Misc : 6.08g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B-1-0-6

Integration File: Calibration.e
Quant Time: Nov 22 20:49:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

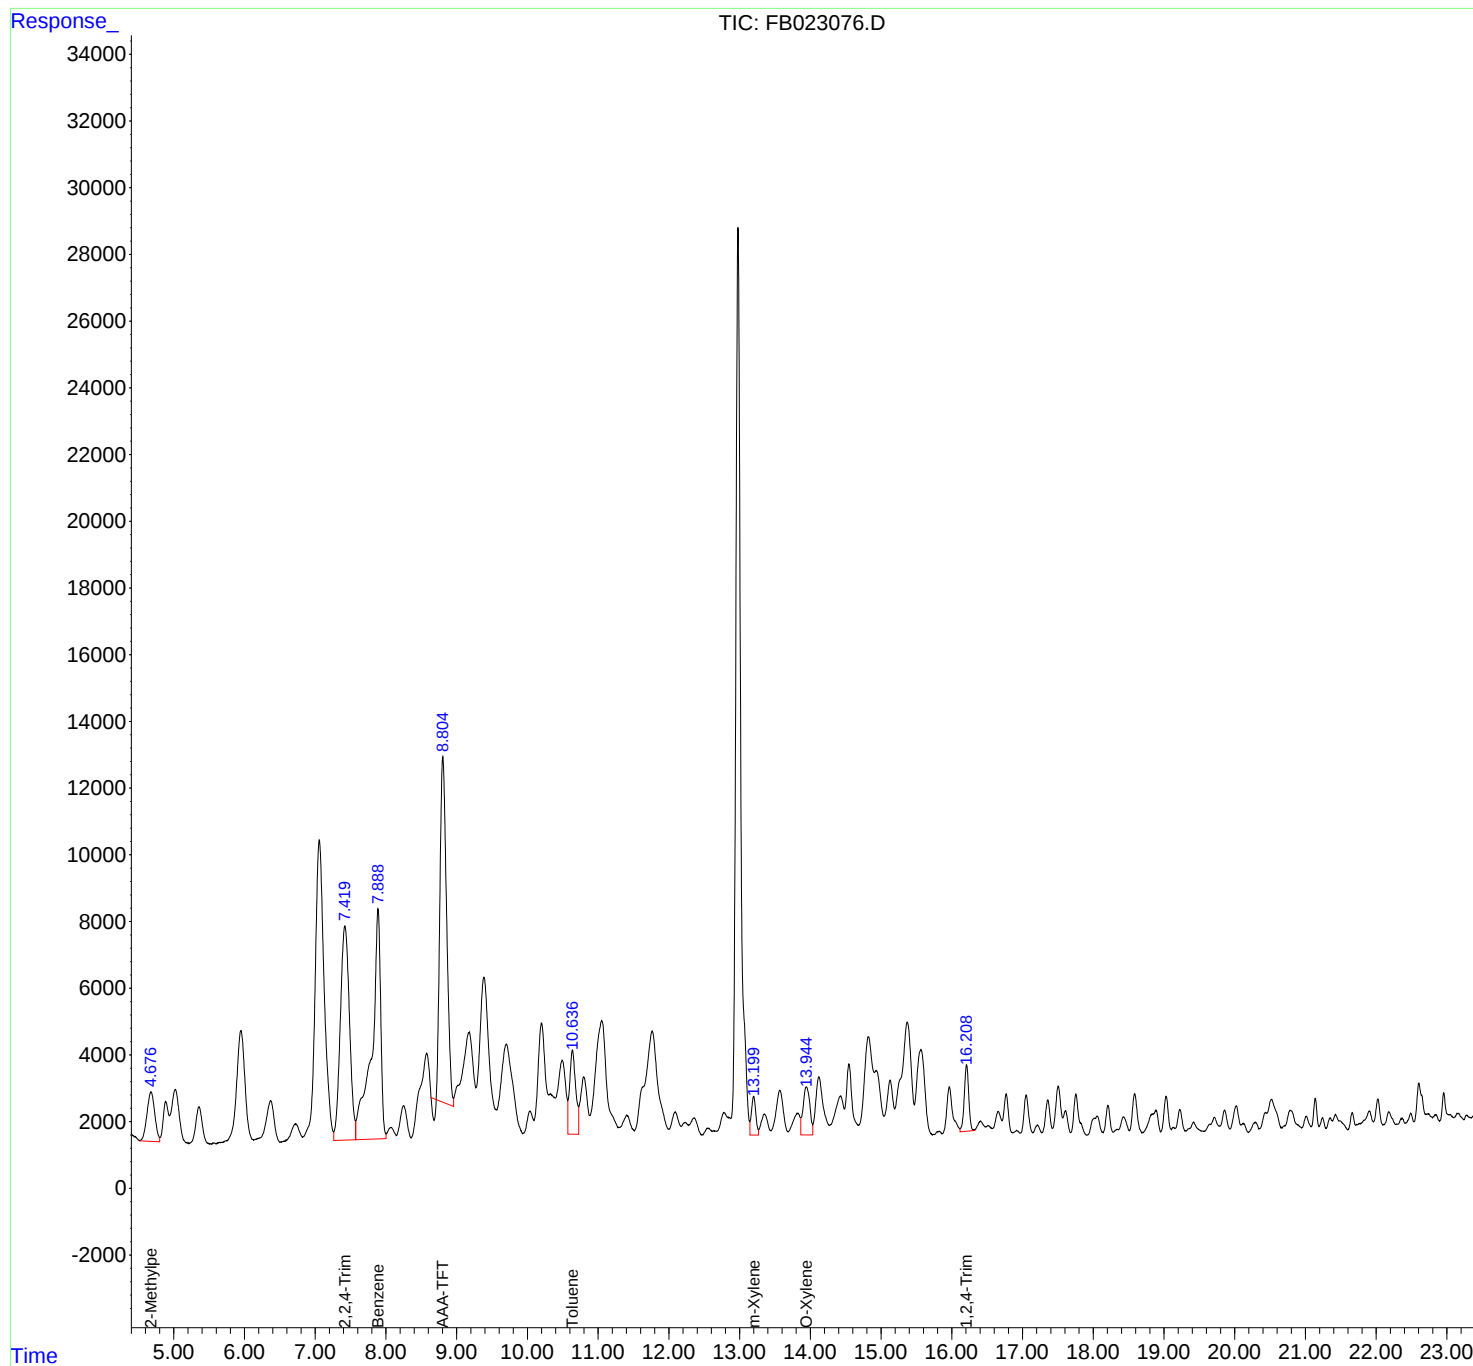


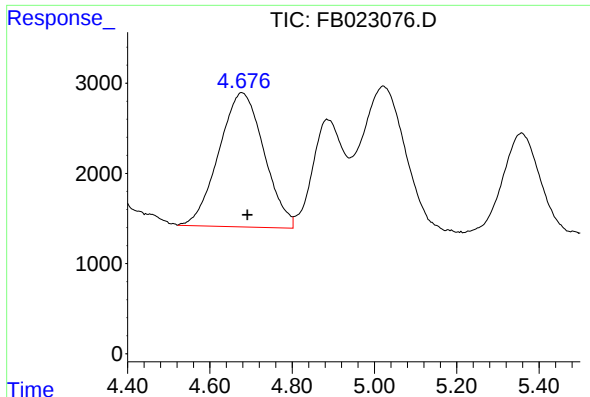

#1 2-Methylpentane


R.T.: 4.677 min
Delta R.T.: -0.014 min
Response: 113425
Conc: 3.47 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1-0-6

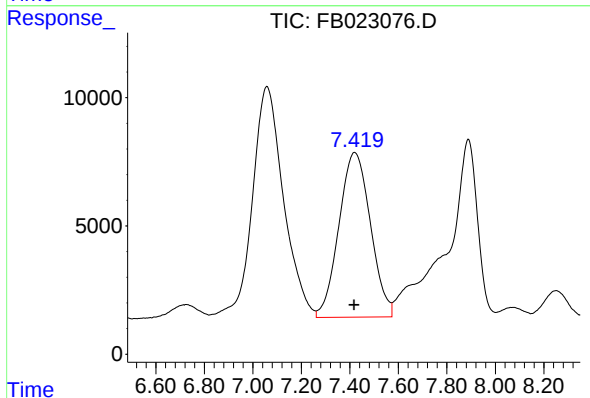


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.002 min
Response: 580108
Conc: 16.64 ng/ml

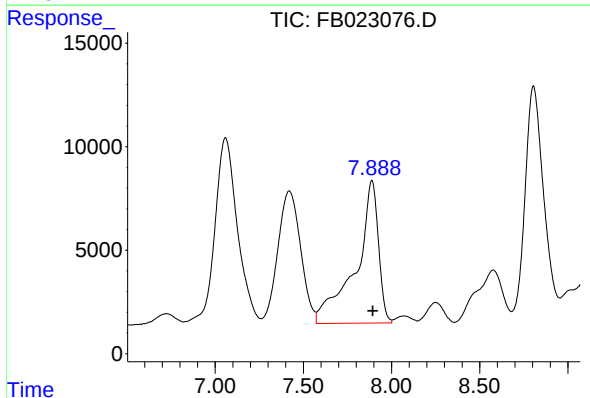


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 616672
Conc: 14.80 ng/ml

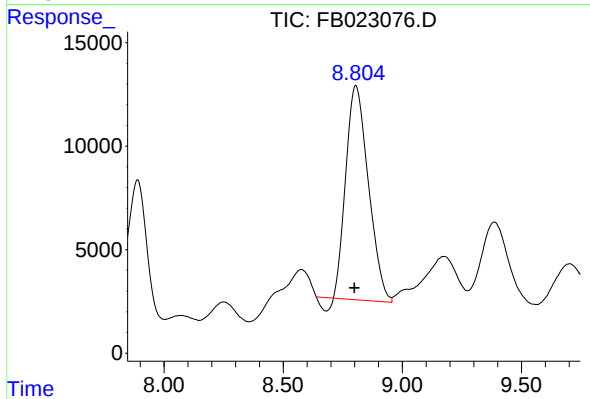

#5 AAA-TFT


R.T.: 8.805 min
Delta R.T.: 0.006 min
Response: 669828
Conc: 27.27 ng/ml

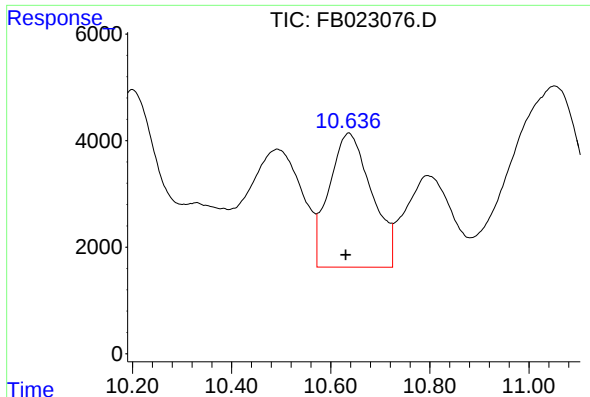

#6 Toluene


R.T.: 10.637 min
Delta R.T.: 0.007 min
Response: 150368
Conc: 3.73 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1-0-6

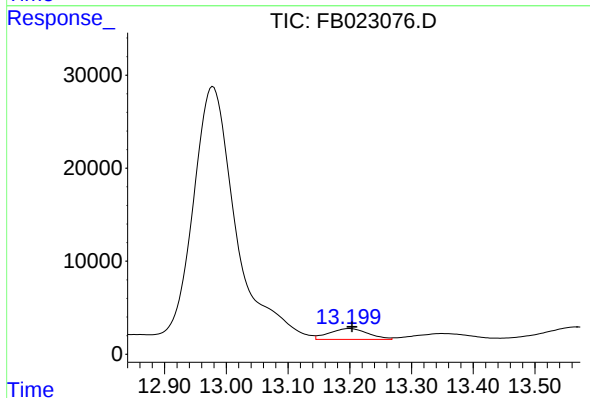


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 50656
Conc: 1.39 ng/ml

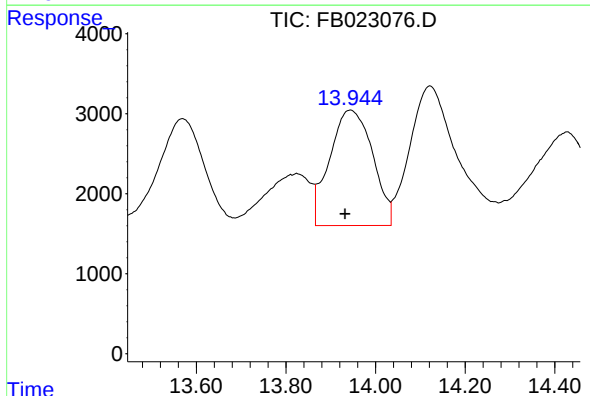

#9 o-Xylene

R.T.: 13.944 min
Delta R.T.: 0.013 min
Response: 96006
Conc: 2.77 ng/ml

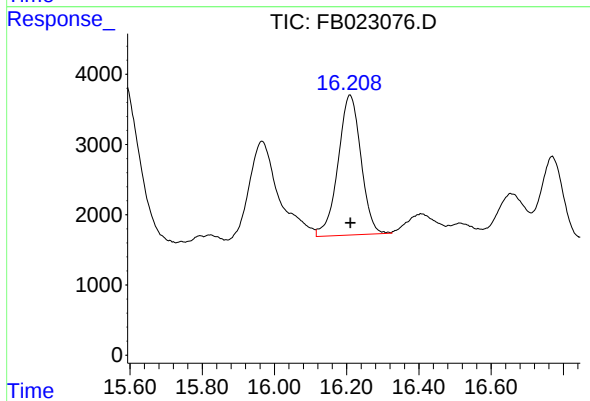

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 87449
Conc: 3.12 ng/ml