

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023079.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2019 22:46
 Operator : DD/AJ
 Sample : K5668-09MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 HD-01-112119MS

Integration File: Calibration.e
 Quant Time: Nov 22 23:00:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	383366	15.607 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	727644	22.267 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	813838	23.339 ng/ml
3) t n-Heptane	7.757	264777	7.701 ng/ml
4) t Benzene	7.891	355955	8.543 ng/ml
6) t Toluene	10.629	1028935	25.542 ng/ml
7) t Ethylbenzene	13.069	322164	8.349 ng/ml
8) t m-Xylene	13.202	609879	16.760 ng/ml
9) t O-Xylene	13.930	598073	17.225 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	504396	17.986 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023079.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 22:46
Operator : DD/AJ
Sample : K5668-09MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HD-01-112119MS

Integration File: Calibration.e
Quant Time: Nov 22 23:00:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

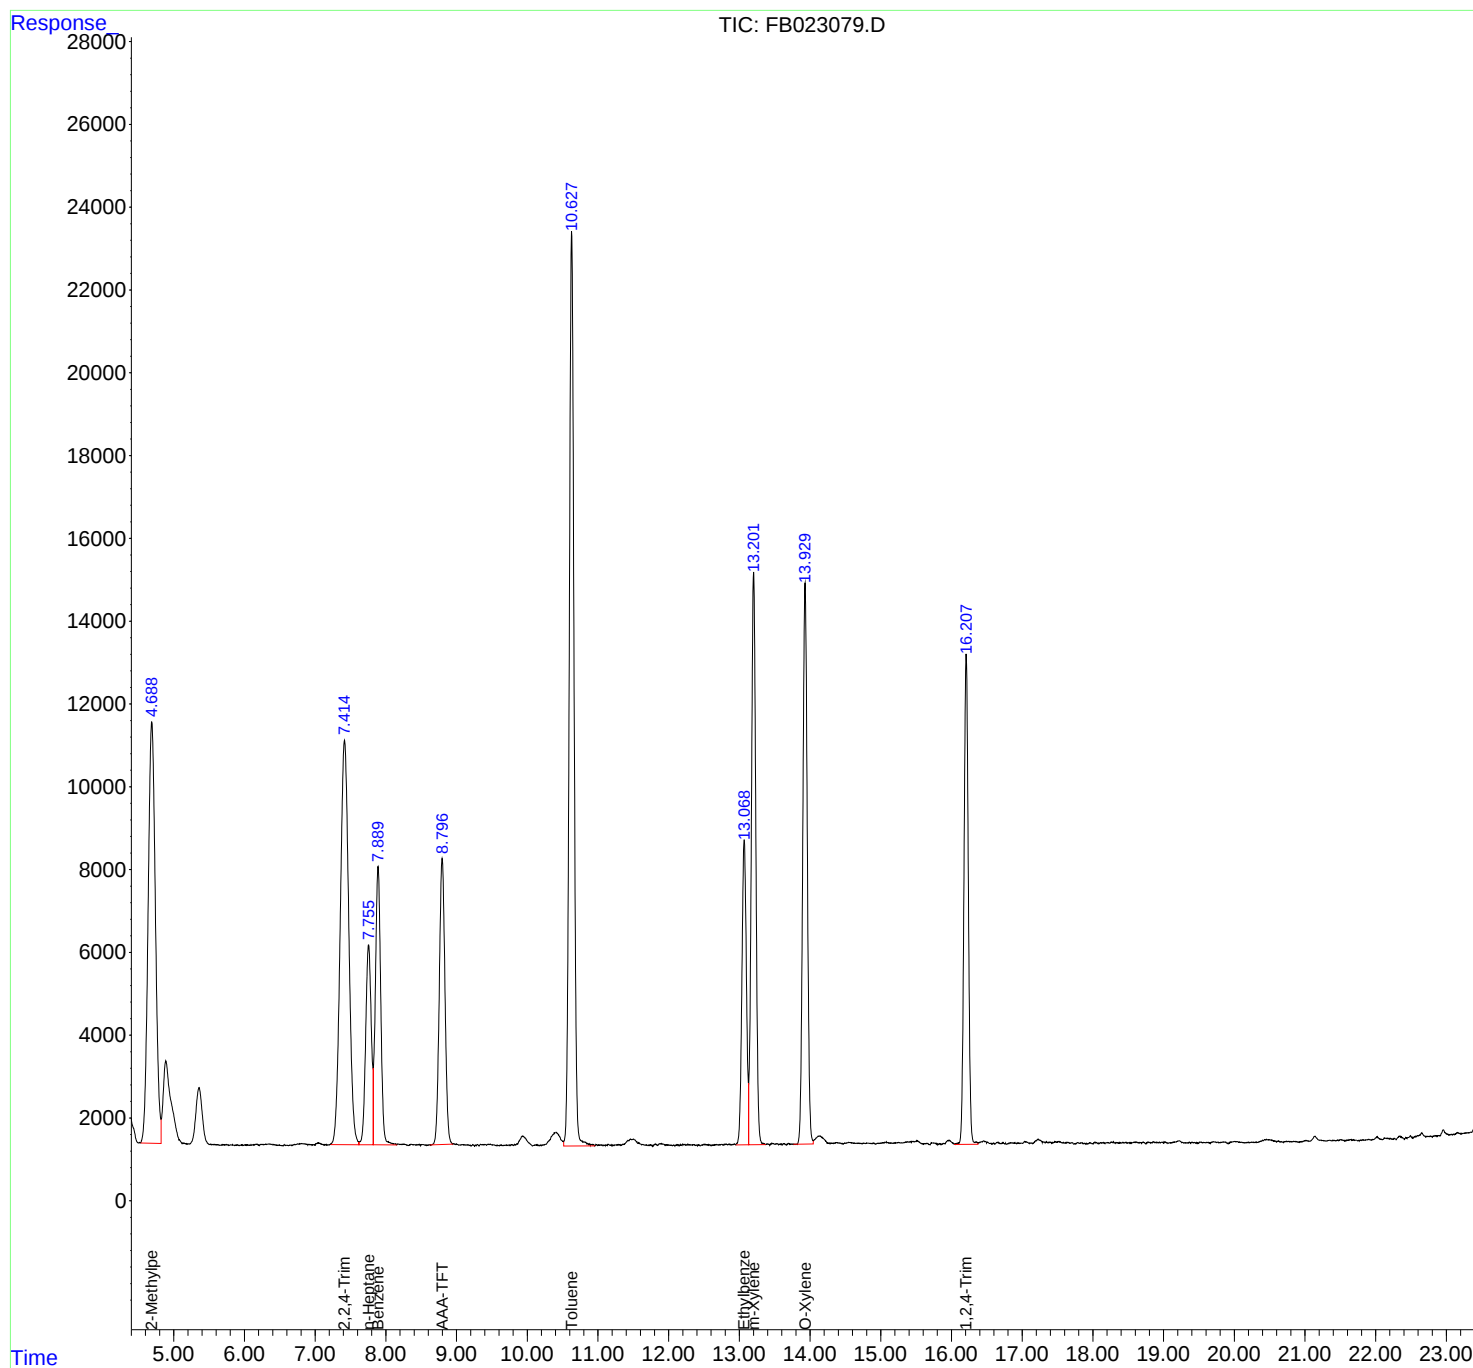


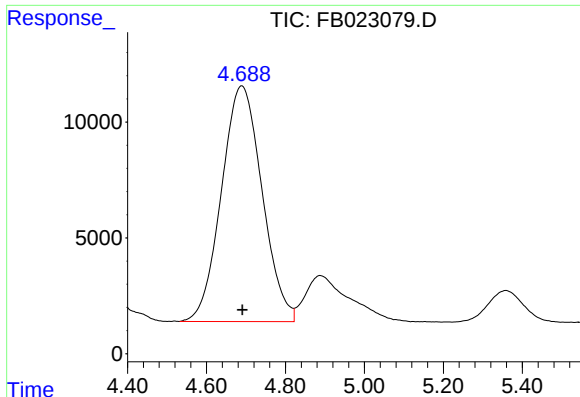

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 727644
Conc: 22.27 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MS

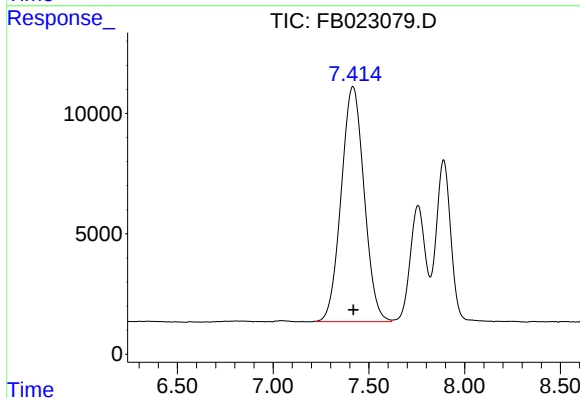


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.003 min
Response: 813838
Conc: 23.34 ng/ml

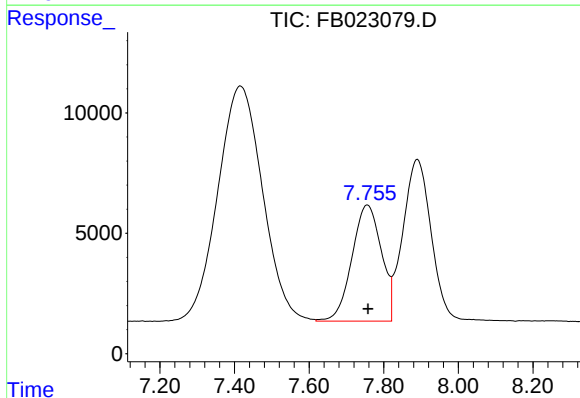


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 264777
Conc: 7.70 ng/ml

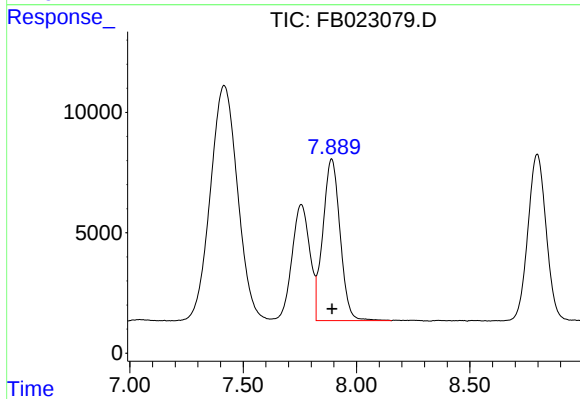

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 355955
Conc: 8.54 ng/ml

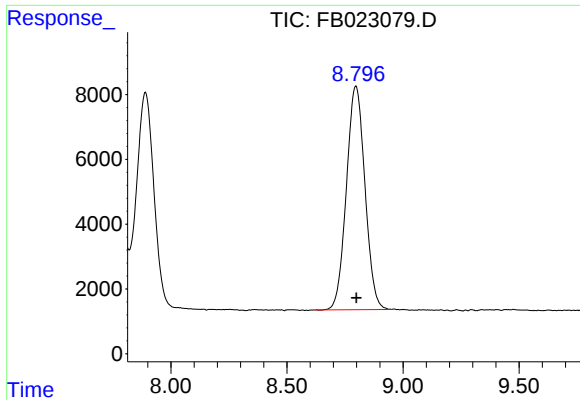

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 383366
Conc: 15.61 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MS

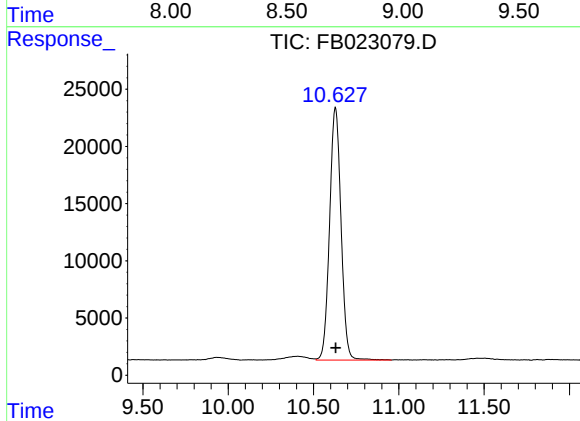


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 1028935
Conc: 25.54 ng/ml

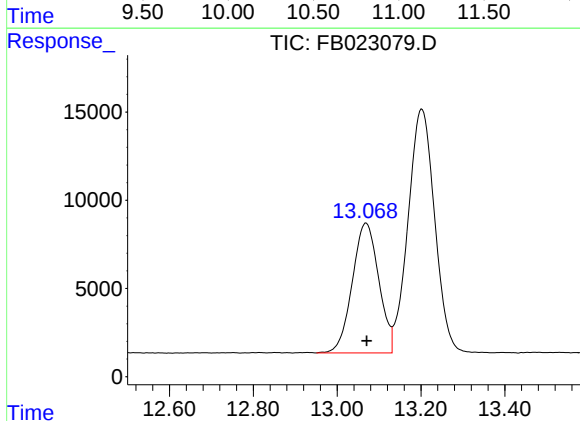


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 322164
Conc: 8.35 ng/ml

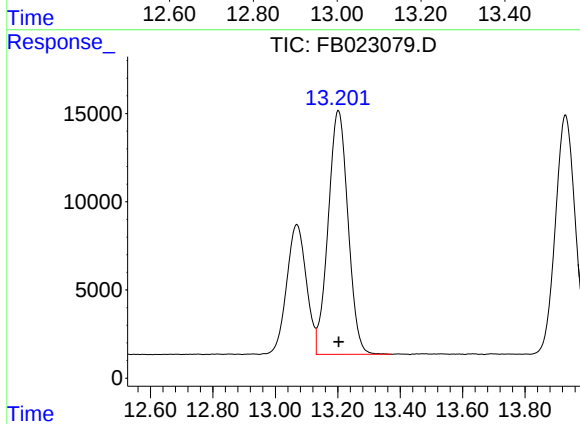

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 609879
Conc: 16.76 ng/ml

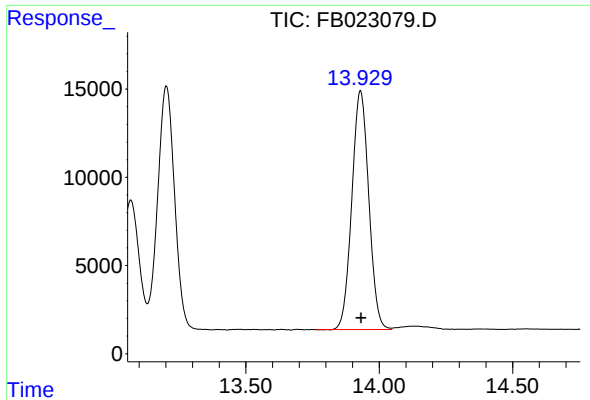

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 598073
Conc: 17.23 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MS

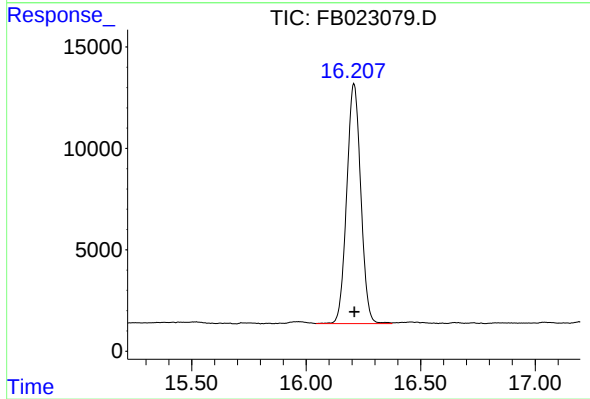

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 504396
Conc: 17.99 ng/ml