

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023080.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2019 23:16
 Operator : DD/AJ
 Sample : K5668-09MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 HD-01-112119MSD

Integration File: SAMPLE.e
 Quant Time: Nov 23 02:51:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	462962	18.847 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	880537	26.946 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	981028	28.133 ng/ml
3) t n-Heptane	7.755	317980	9.248 ng/ml
4) t Benzene	7.890	392722	9.426 ng/ml
6) t Toluene	10.628	1123162	27.881 ng/ml
7) t Ethylbenzene	13.069	350624	9.086 ng/ml
8) t m-Xylene	13.202	658919	18.107 ng/ml
9) t O-Xylene	13.930	637897	18.372 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	524797	18.714 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
Data File : FB023080.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2019 23:16
Operator : DD/AJ
Sample : K5668-09MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

Integration File: SAMPLE.e
Quant Time: Nov 23 02:51:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

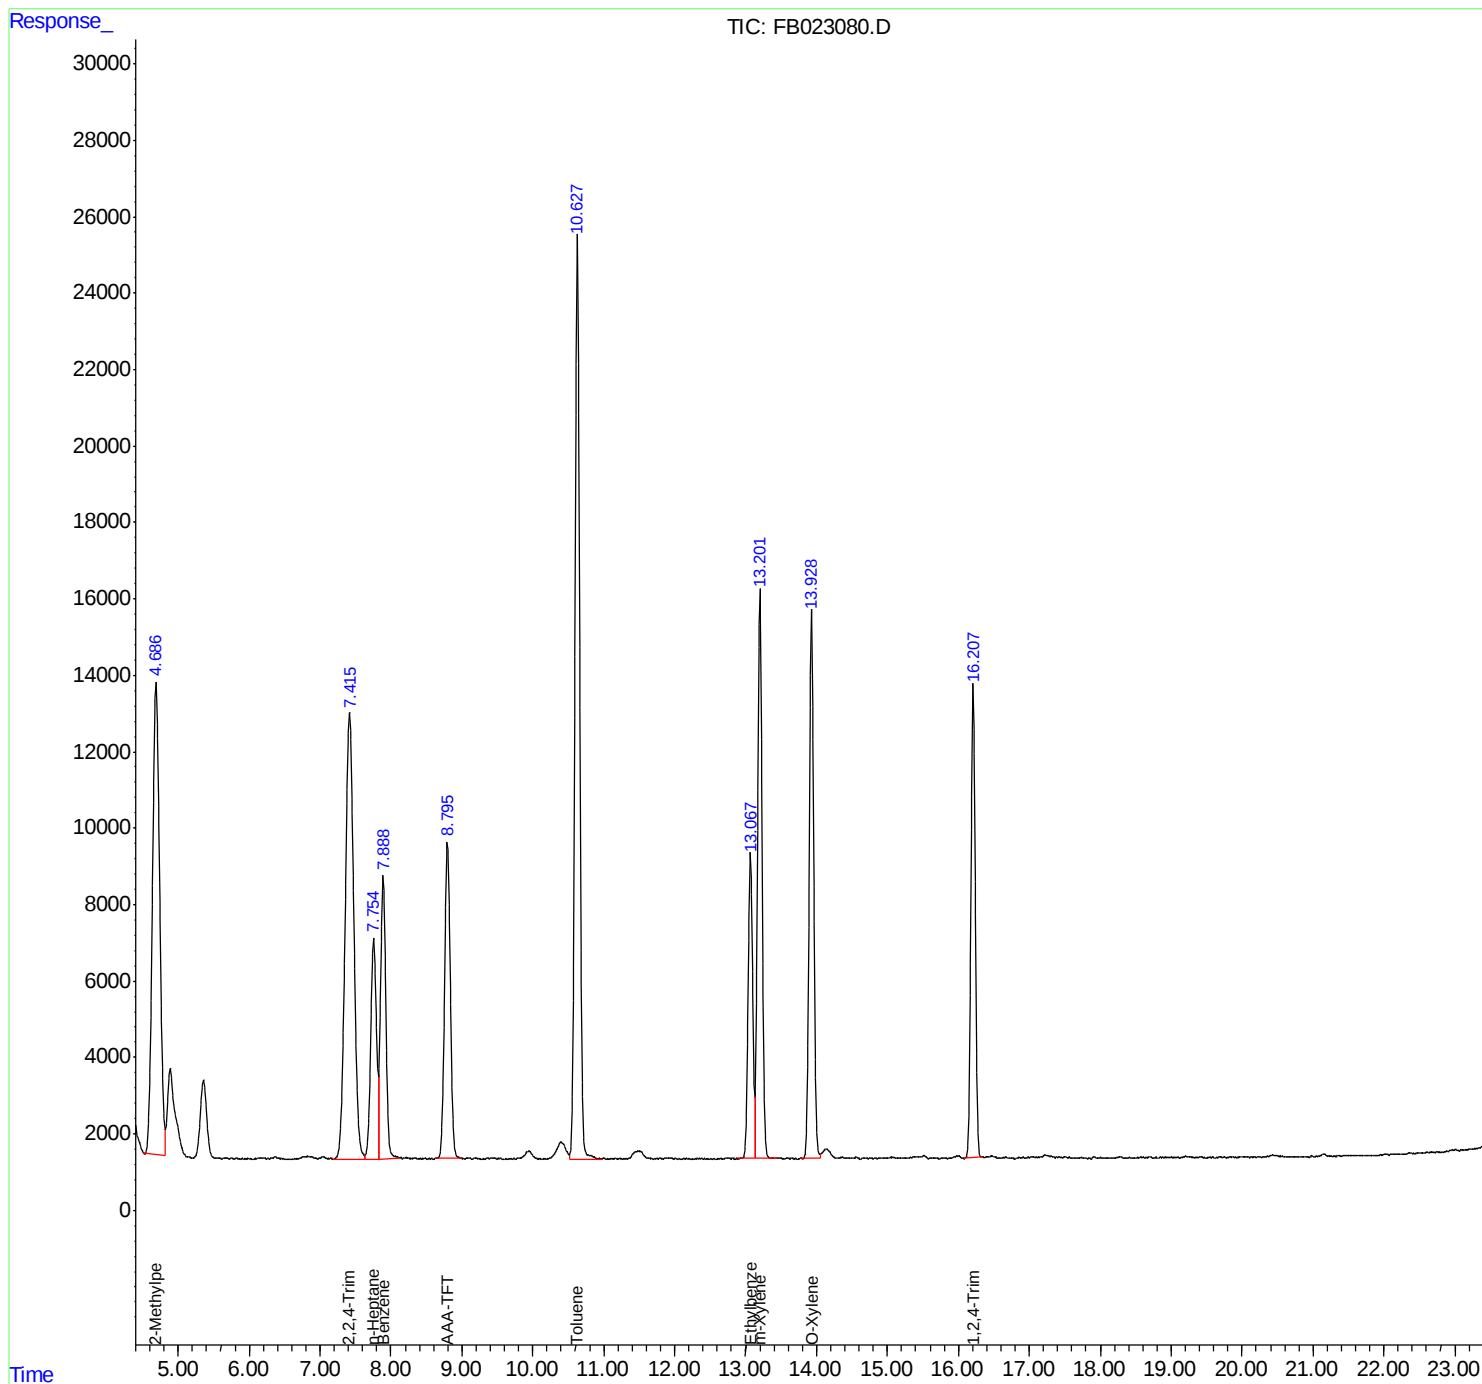


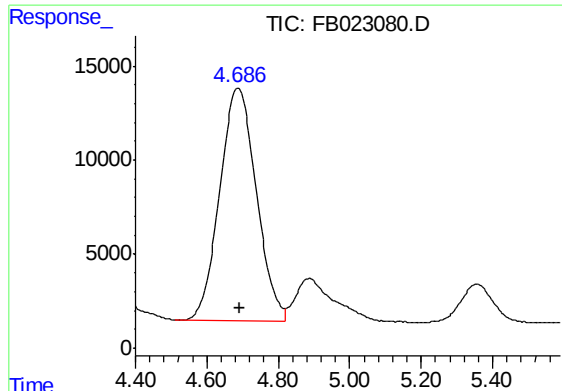

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 880537
Conc: 26.95 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

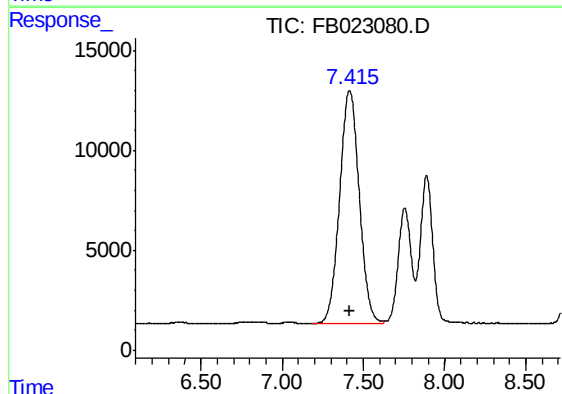


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 981028
Conc: 28.13 ng/ml

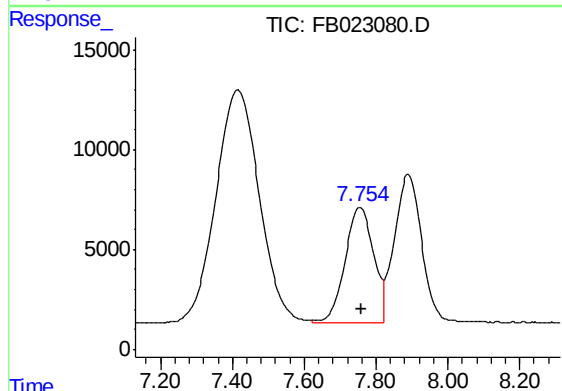


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.002 min
Response: 317980
Conc: 9.25 ng/ml

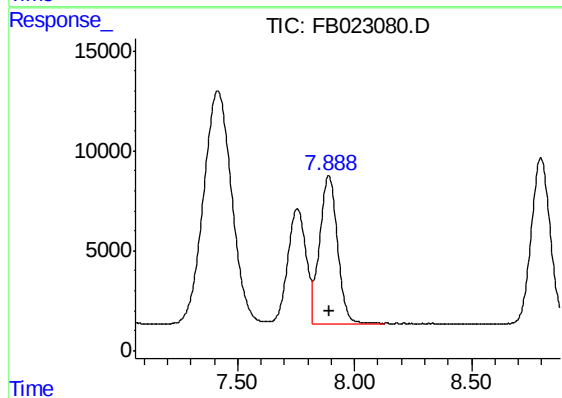

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 392722
Conc: 9.43 ng/ml

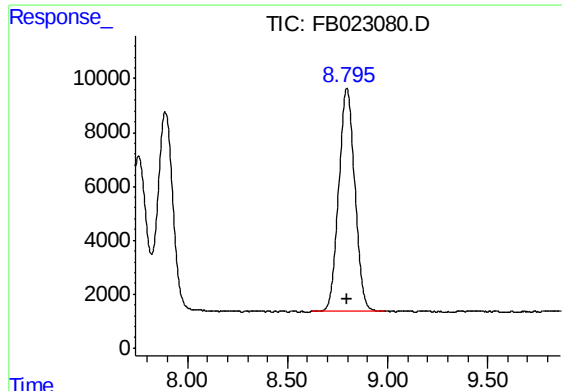

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 462962
Conc: 18.85 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

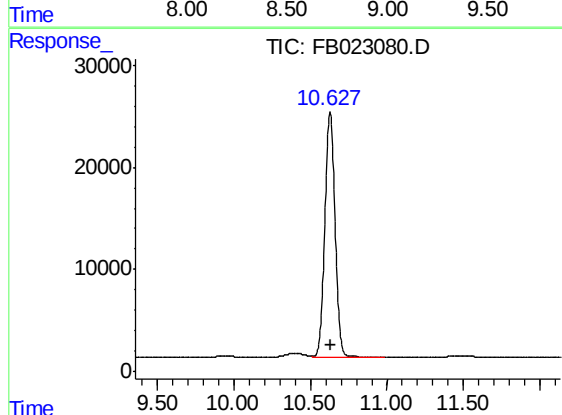


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1123162
Conc: 27.88 ng/ml

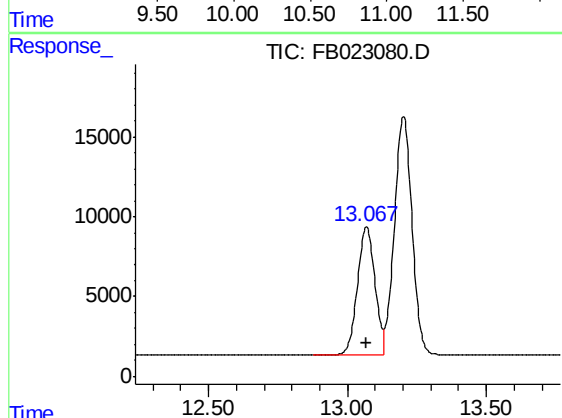


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 350624
Conc: 9.09 ng/ml

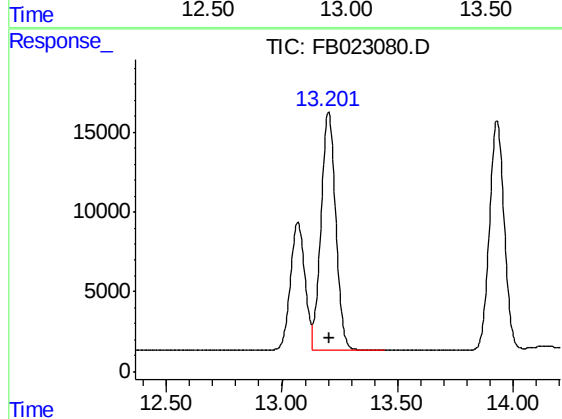

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 658919
Conc: 18.11 ng/ml

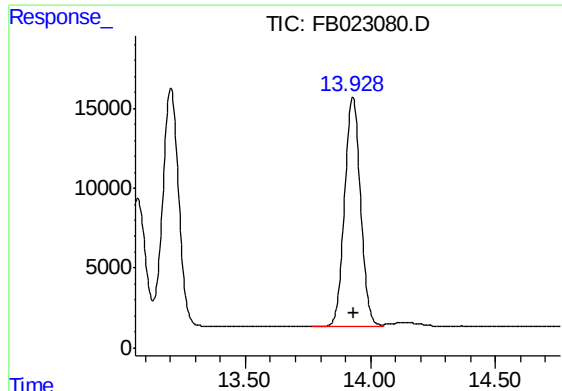

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 637897
Conc: 18.37 ng/ml

Instrument :
FID_B
ClientSampleId :
HD-01-112119MSD

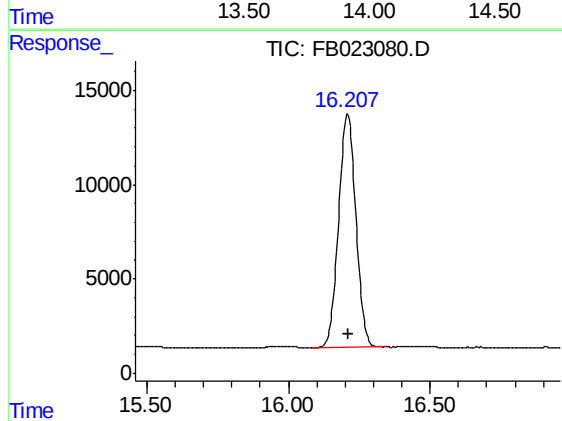

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 524797
Conc: 18.71 ng/ml