

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112224\
 Data File : FB031259.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2024 12:14
 Operator : YP/AJ
 Sample : BSF1122S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1122S1

Integration File: Calibration.e
 Quant Time: Nov 23 00:17:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
 Quant Title :
 QLast Update : Thu Nov 21 12:34:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	678417	24.102 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.723	1173208	29.748 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	1383262	29.252 ng/ml
3) t n-Heptane	7.757	444037	9.508 ng/ml
4) t Benzene	7.895	517504	9.548 ng/ml
6) t Toluene	10.624	1446115	28.918 ng/ml
7) t Ethylbenzene	13.061	413631	9.428 ng/ml
8) t m-Xylene	13.195	889972	18.877 ng/ml
9) t O-Xylene	13.923	826587	18.978 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	655540	18.364 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112224\
Data File : FB031259.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2024 12:14
Operator : YP/AJ
Sample : BSF1122S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1122S1

Integration File: Calibration.e
Quant Time: Nov 23 00:17:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

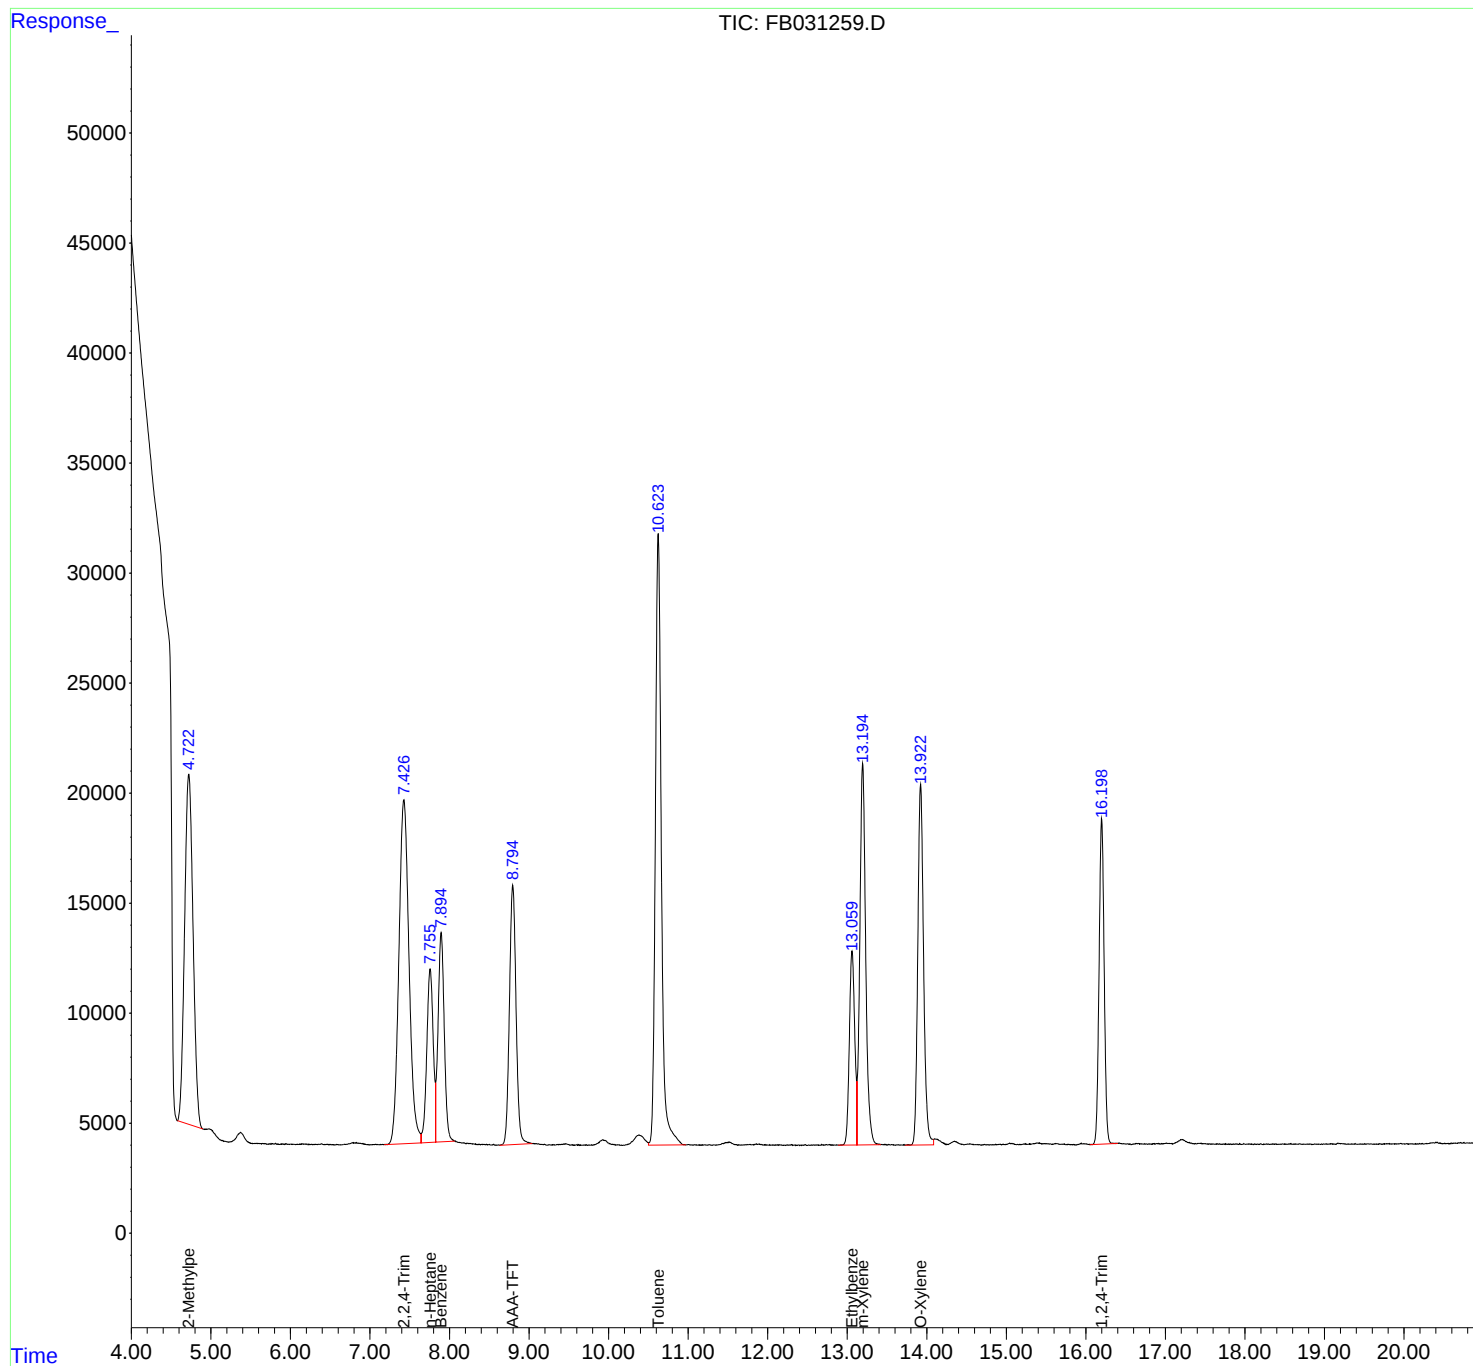


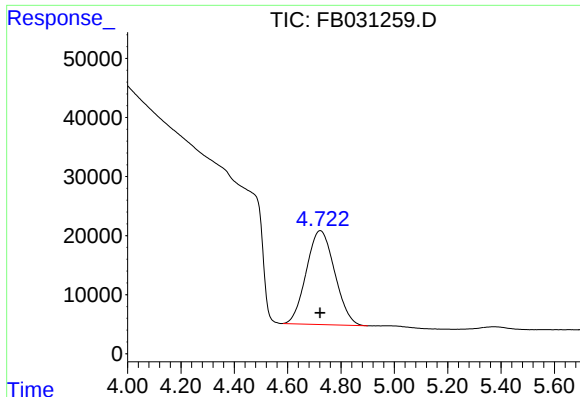

#1 2-Methylpentane


R.T.: 4.723 min
Delta R.T.: 0.000 min
Response: 1173208
Conc: 29.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1122S1

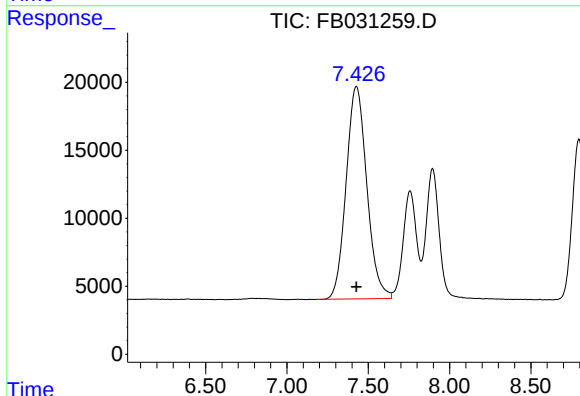


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 1383262
Conc: 29.25 ng/ml

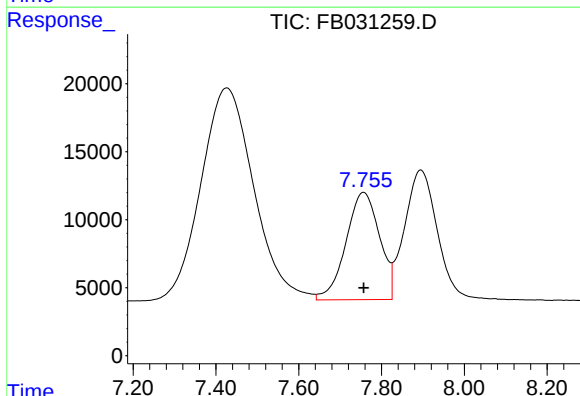


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 444037
Conc: 9.51 ng/ml

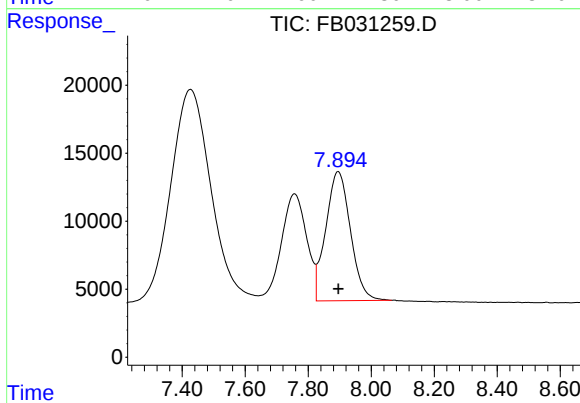

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 517504
Conc: 9.55 ng/ml

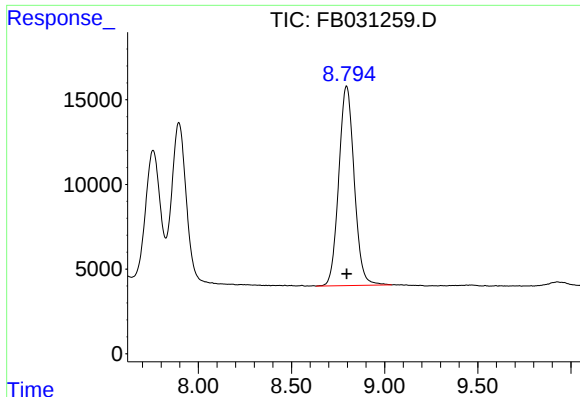

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 678417
Conc: 24.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1122S1

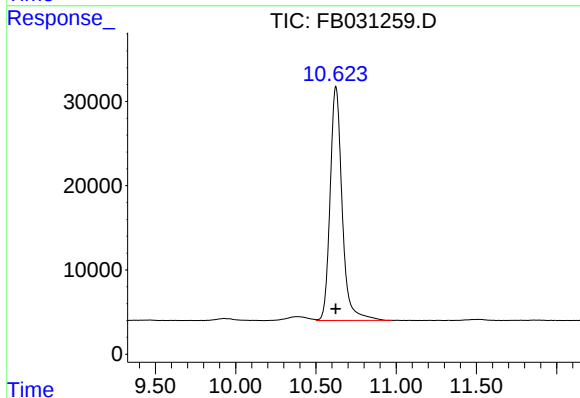


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 1446115
Conc: 28.92 ng/ml

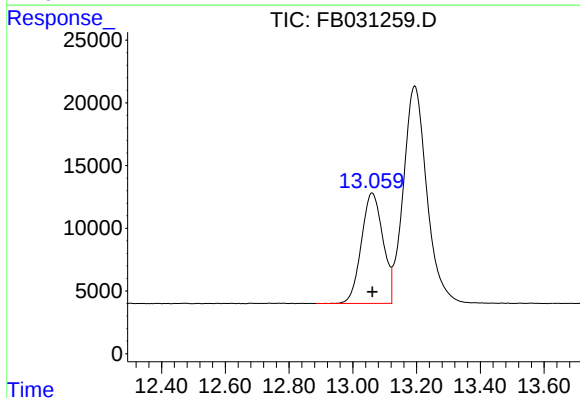


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.000 min
Response: 413631
Conc: 9.43 ng/ml

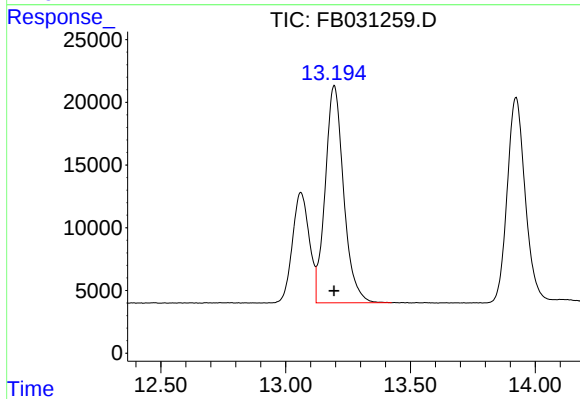

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.000 min
Response: 889972
Conc: 18.88 ng/ml

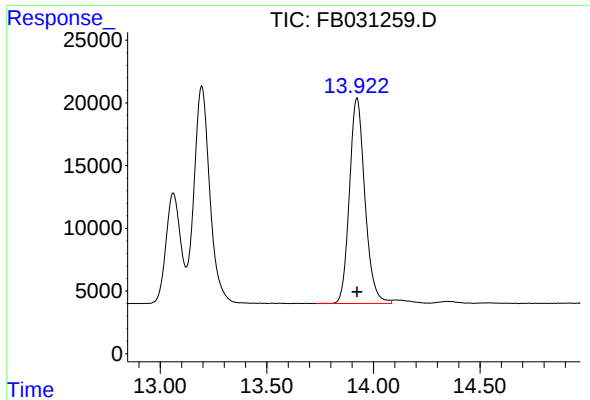

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.000 min
Response: 826587
Conc: 18.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1122S1

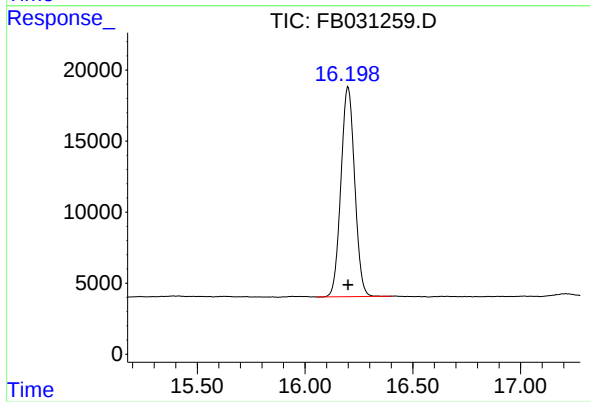

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 655540
Conc: 18.36 ng/ml