

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112224\
 Data File : FB031263.D
 Signal(s) : FID2B.CH
 Acq On : 22 Nov 2024 14:39
 Operator : YP/AJ
 Sample : BSF1122S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1122S2

Integration File: Calibration.e
 Quant Time: Nov 23 00:18:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
 Quant Title :
 QLast Update : Thu Nov 21 12:34:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	595002	21.139 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	1332756	33.794 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	1550533	32.789 ng/ml
3) t n-Heptane	7.756	493557	10.568 ng/ml
4) t Benzene	7.896	564597	10.417 ng/ml
6) t Toluene	10.625	1591425	31.823 ng/ml
7) t Ethylbenzene	13.062	451688	10.296 ng/ml
8) t m-Xylene	13.196	971504	20.606 ng/ml
9) t O-Xylene	13.924	912070	20.941 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	714349	20.012 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112224\
Data File : FB031263.D
Signal(s) : FID2B.CH
Acq On : 22 Nov 2024 14:39
Operator : YP/AJ
Sample : BSF1122S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1122S2

Integration File: Calibration.e
Quant Time: Nov 23 00:18:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

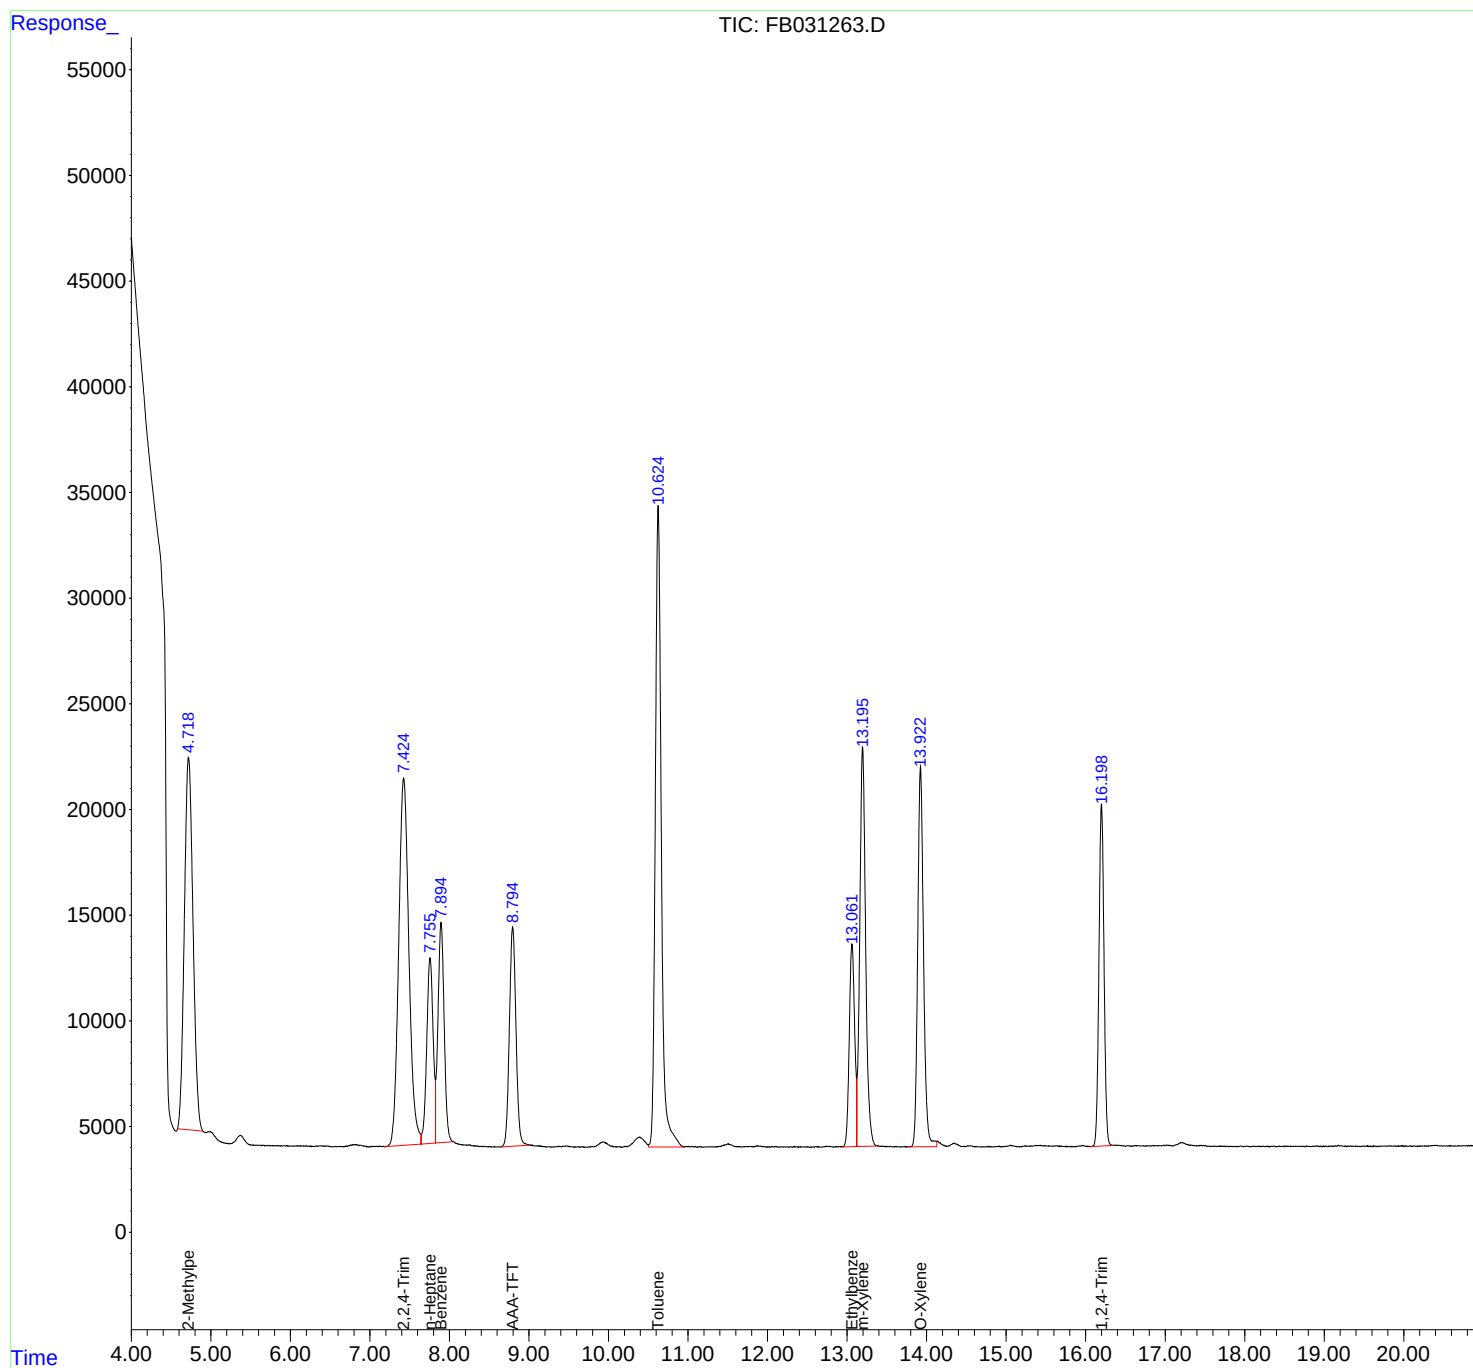


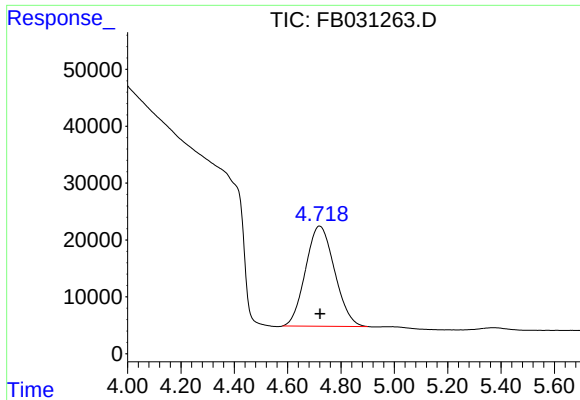

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: -0.003 min
Response: 1332756
Conc: 33.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1122S2

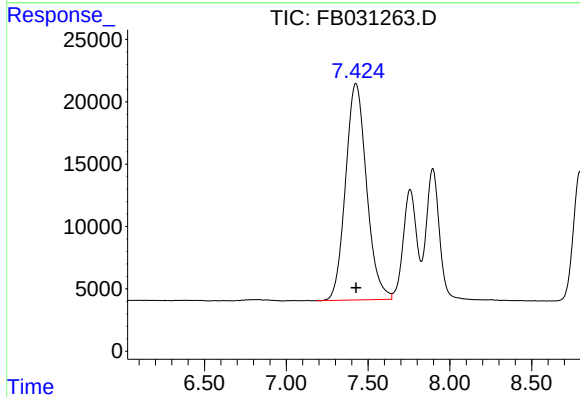


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.002 min
Response: 1550533
Conc: 32.79 ng/ml

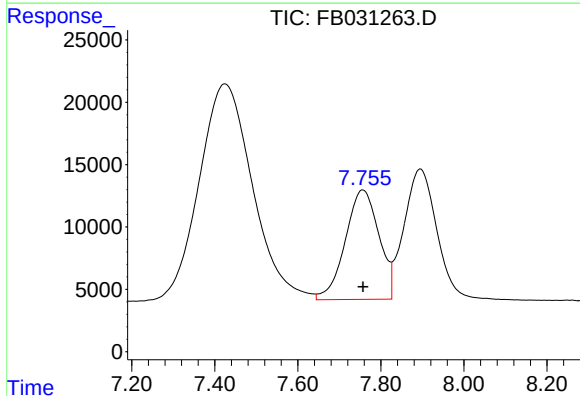


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 493557
Conc: 10.57 ng/ml

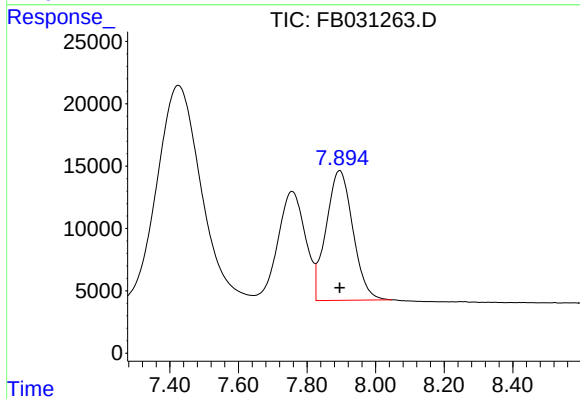

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 564597
Conc: 10.42 ng/ml

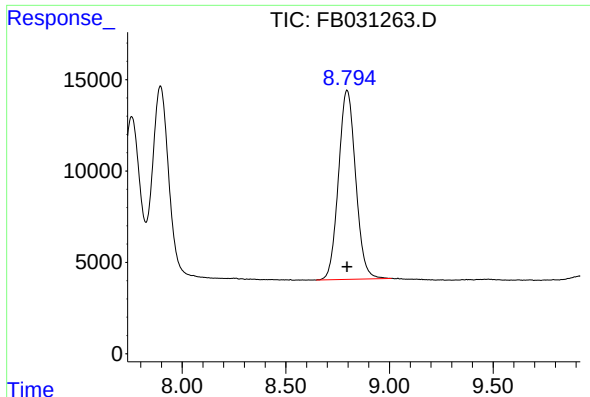

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 595002
Conc: 21.14 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1122S2

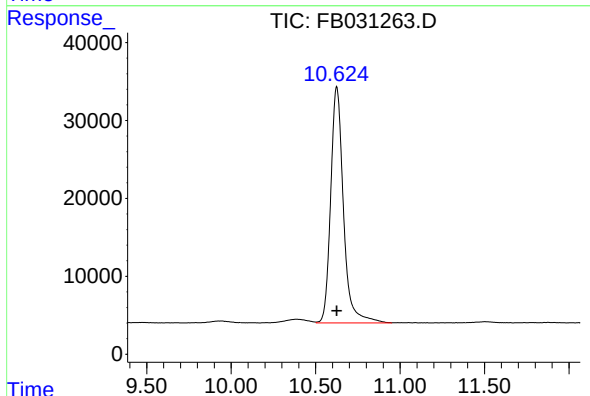


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.000 min
Response: 1591425
Conc: 31.82 ng/ml

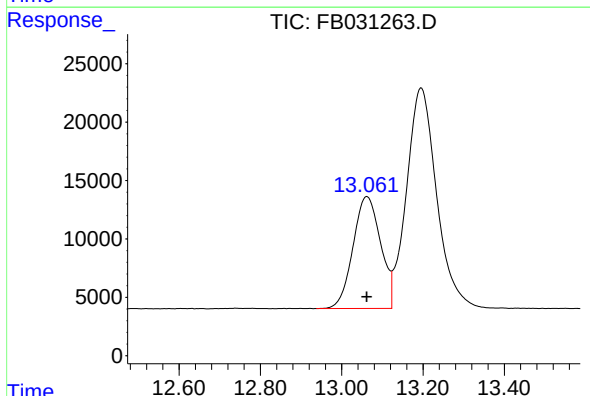


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.000 min
Response: 451688
Conc: 10.30 ng/ml

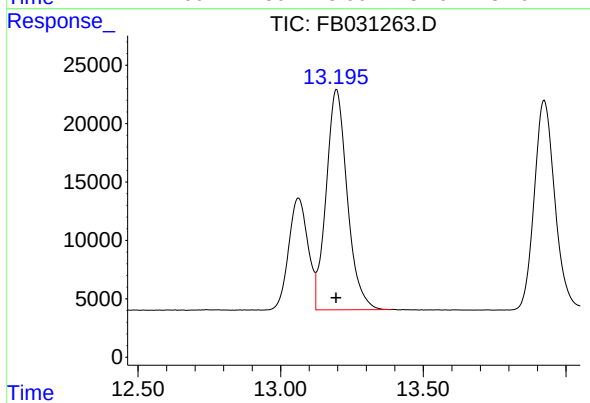

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.001 min
Response: 971504
Conc: 20.61 ng/ml

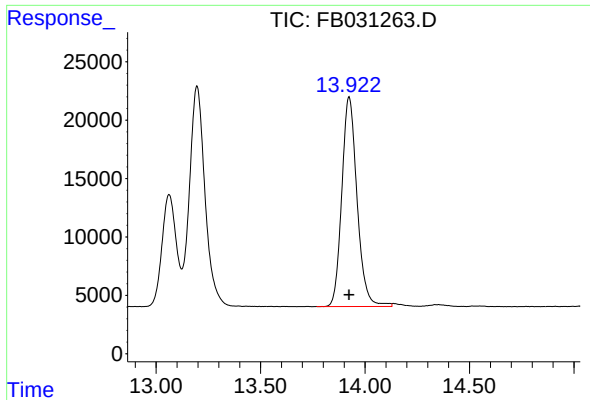

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.001 min
Response: 912070
Conc: 20.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1122S2

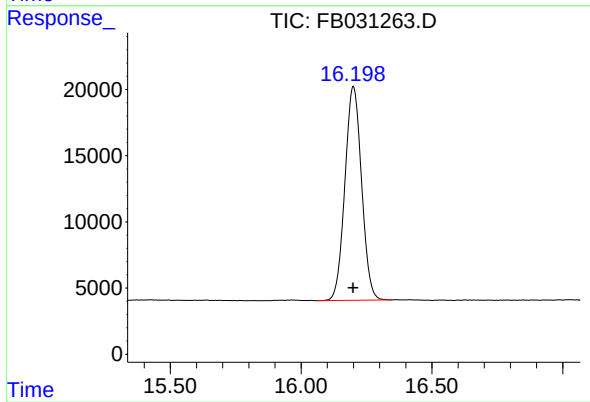

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.000 min
Response: 714349
Conc: 20.01 ng/ml