

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
 Data File : FB025256.D
 Signal(s) : FID2B.CH
 Acq On : 24 Nov 2020 11:57
 Operator : DD/AJ
 Sample : L4800-05MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 25 00:26:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	484021	21.436 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	919923	28.500 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	923011	27.820 ng/ml
3) t n-Heptane	7.757	304535	9.272 ng/ml
4) t Benzene	7.891	397103	9.987 ng/ml
6) t Toluene	10.629	1110543	29.701 ng/ml
7) t Ethylbenzene	13.069	342437	9.972 ng/ml
8) t m-Xylene	13.202	680929	20.167 ng/ml
9) t O-Xylene	13.930	663694	20.299 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	564123	20.502 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
Data File : FB025256.D
Signal(s) : FID2B.CH
Acq On : 24 Nov 2020 11:57
Operator : DD/AJ
Sample : L4800-05MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 25 00:26:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

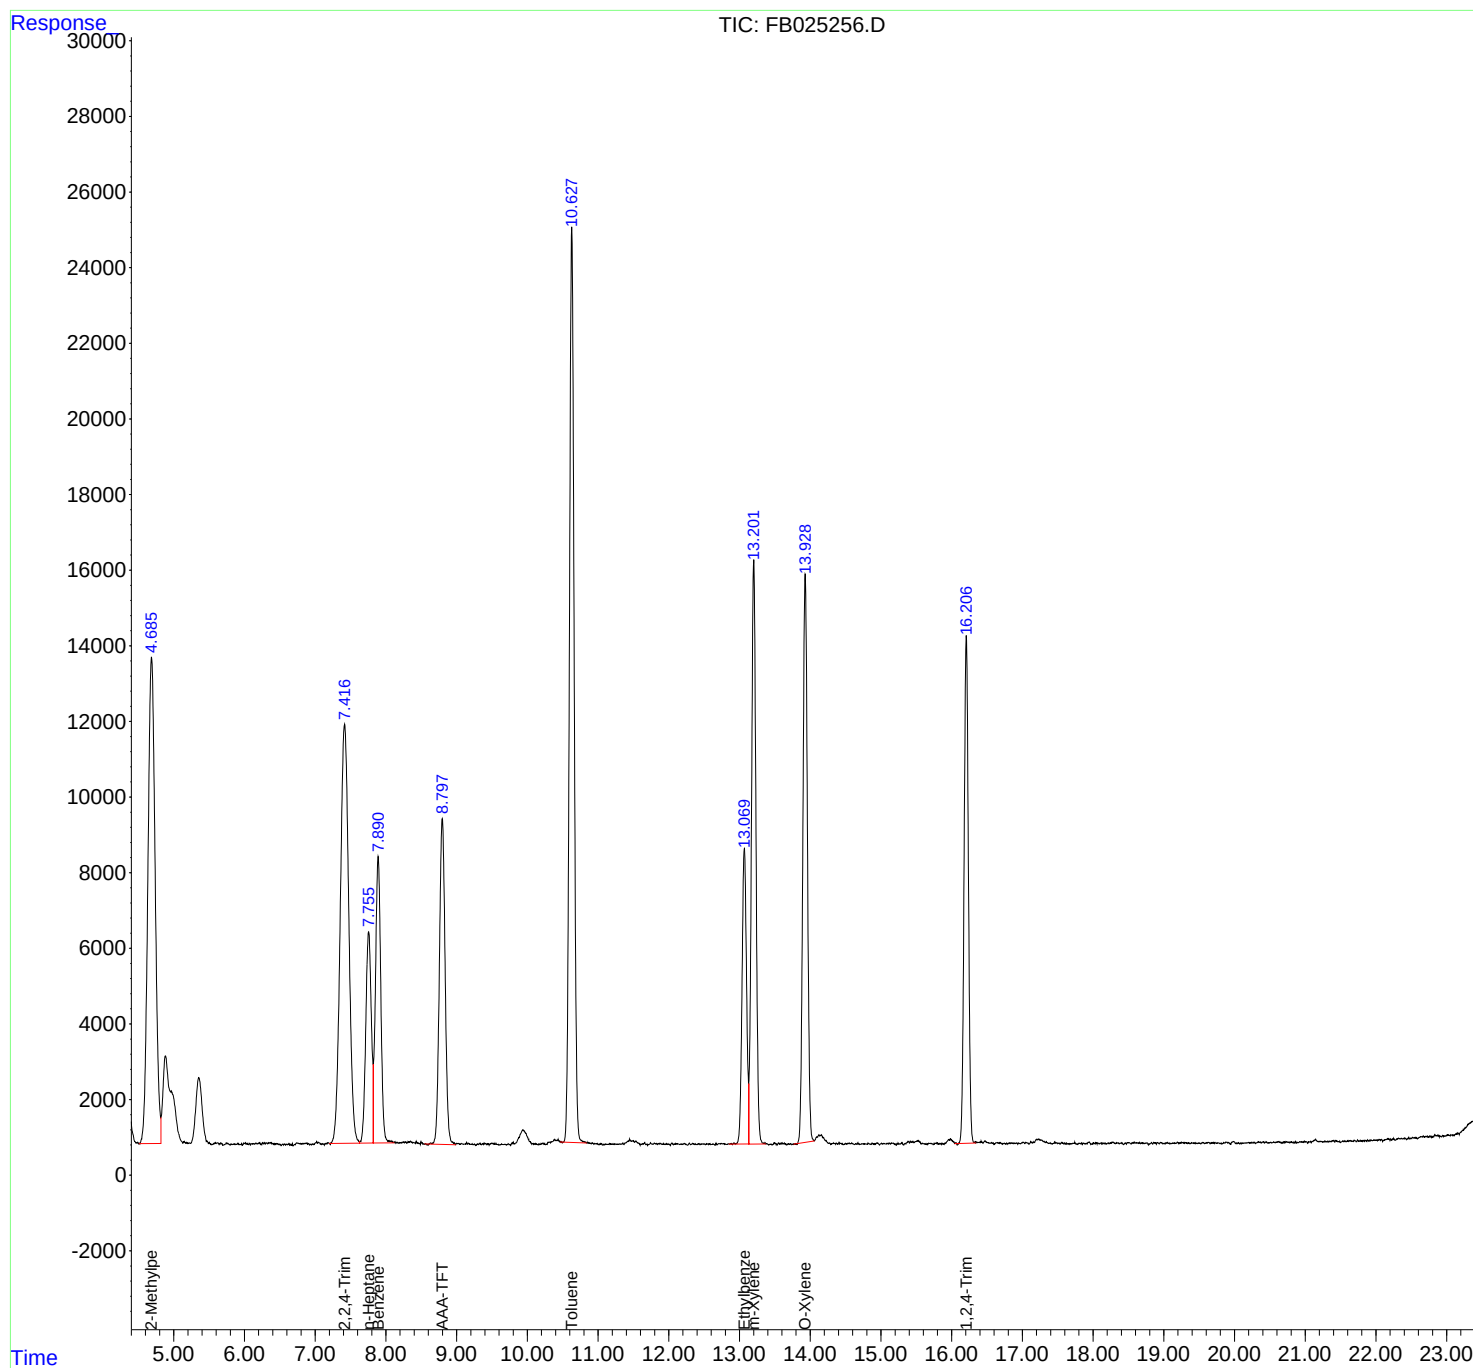


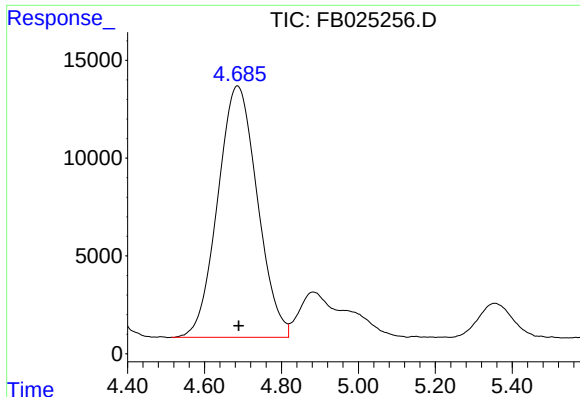

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 919923
Conc: 28.50 ng/ml

Instrument :
FID_B
ClientSampleId :

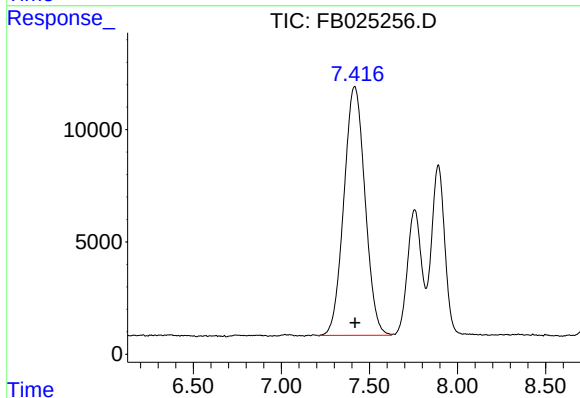


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 923011
Conc: 27.82 ng/ml

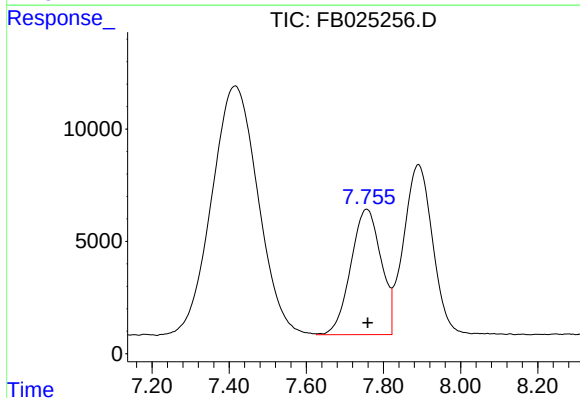


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 304535
Conc: 9.27 ng/ml

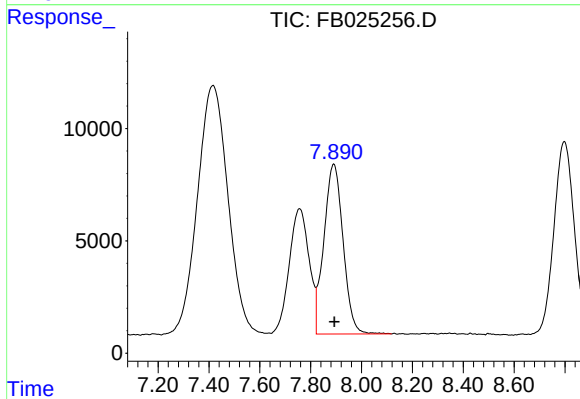

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 397103
Conc: 9.99 ng/ml

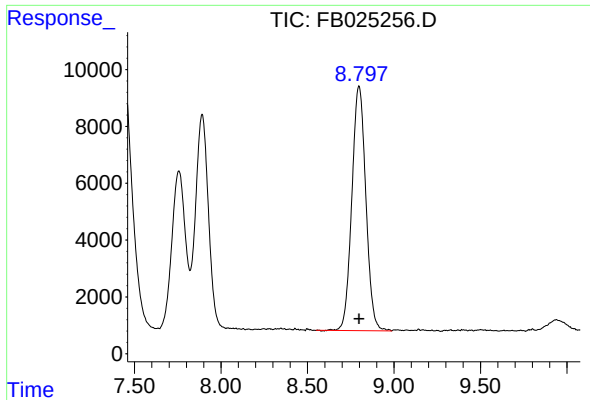

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.001 min
Response: 484021
Conc: 21.44 ng/ml

Instrument :
FID_B
ClientSampleId :

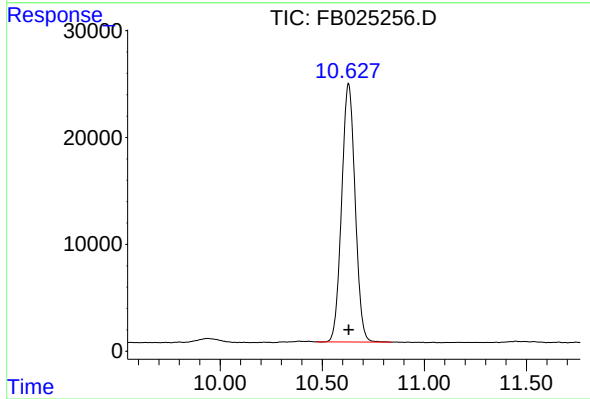


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1110543
Conc: 29.70 ng/ml

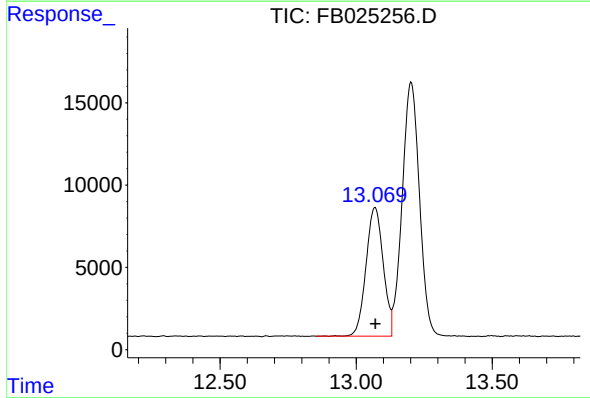


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 342437
Conc: 9.97 ng/ml

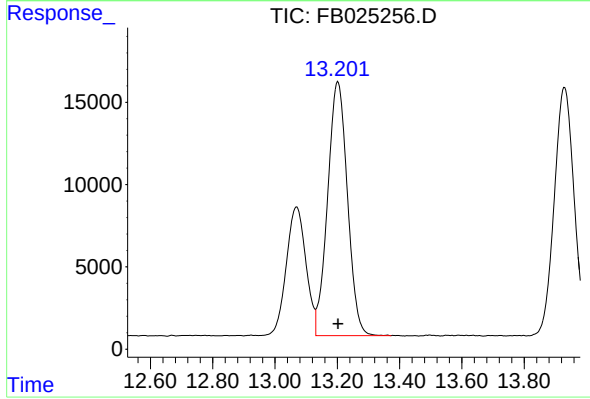

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 680929
Conc: 20.17 ng/ml

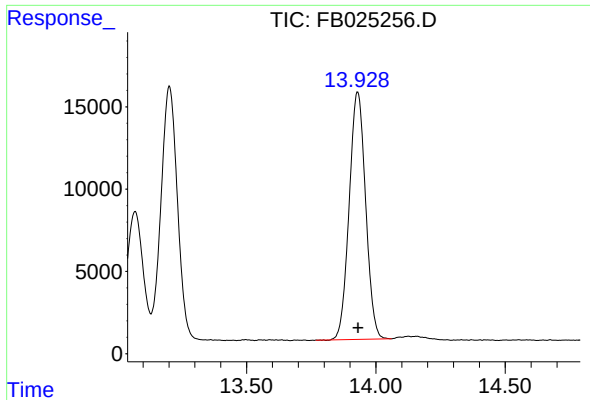

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 663694
Conc: 20.30 ng/ml

Instrument :
FID_B
ClientSampleId :

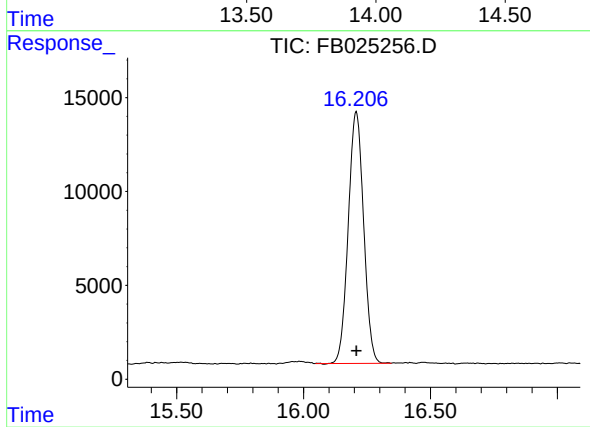

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 564123
Conc: 20.50 ng/ml