

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
 Data File : FB025264.D
 Signal(s) : FID2B.CH
 Acq On : 24 Nov 2020 16:06
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Nov 25 00:27:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	455659	20.180 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	998586	30.937 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1041898	31.403 ng/ml
3) t n-Heptane	7.755	342173	10.418 ng/ml
4) t Benzene	7.890	425865	10.711 ng/ml
6) t Toluene	10.629	1204120	32.204 ng/ml
7) t Ethylbenzene	13.069	364882	10.625 ng/ml
8) t m-Xylene	13.202	732553	21.696 ng/ml
9) t O-Xylene	13.930	711265	21.753 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	629059	22.862 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
Data File : FB025264.D
Signal(s) : FID2B.CH
Acq On : 24 Nov 2020 16:06
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 25 00:27:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

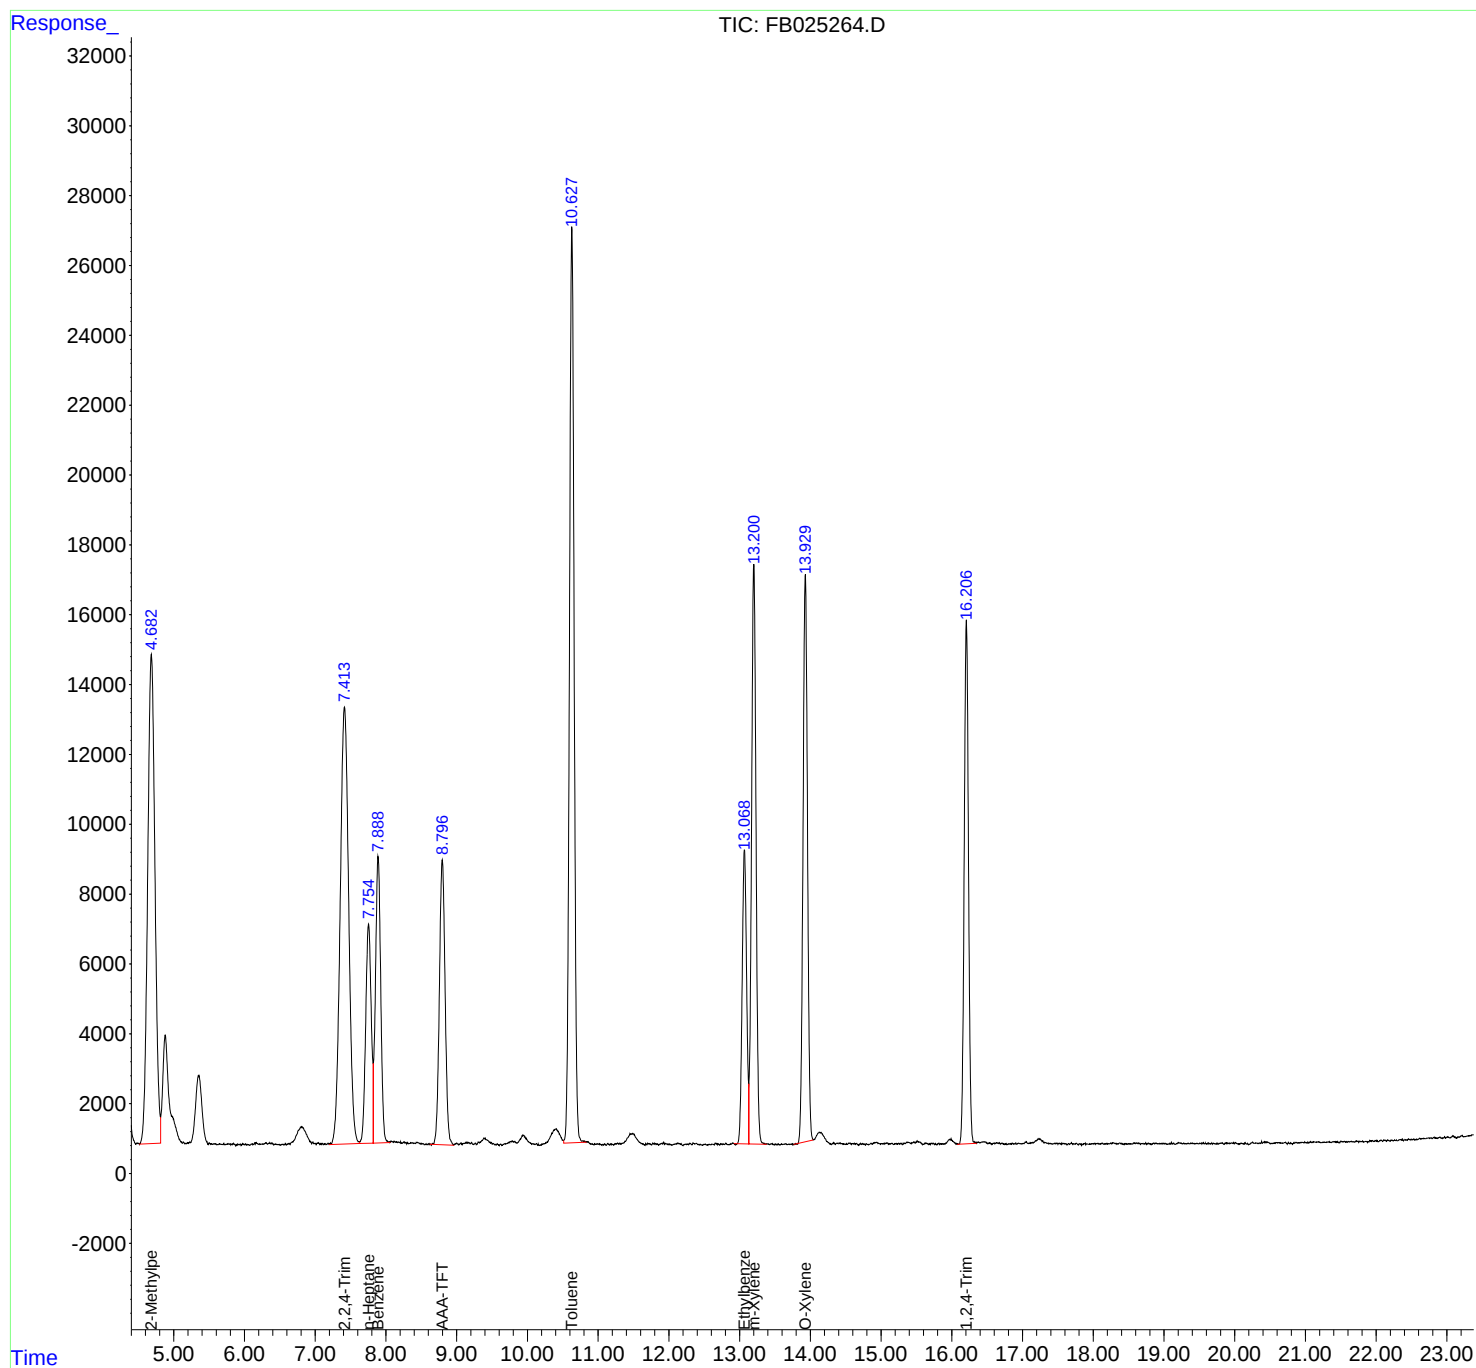


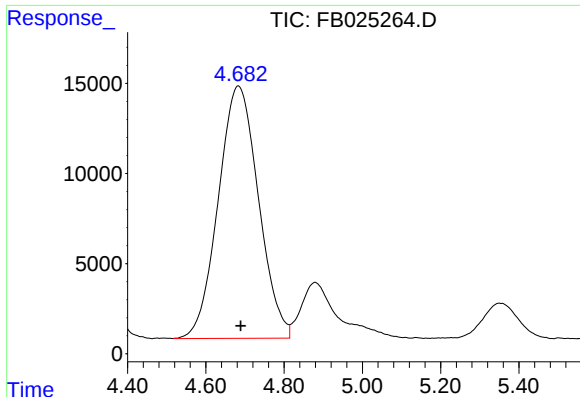

#1 2-Methylpentane


R.T.: 4.684 min
Delta R.T.: -0.005 min
Response: 998586
Conc: 30.94 ng/ml

Instrument :
FID_B
ClientSampleId :

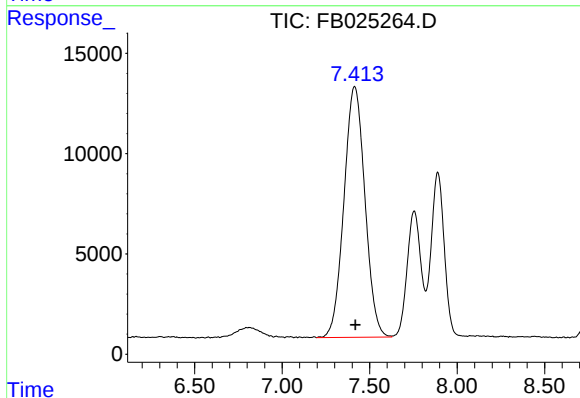


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1041898
Conc: 31.40 ng/ml

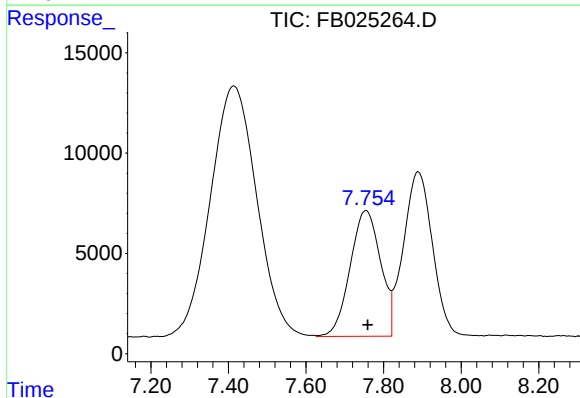


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.004 min
Response: 342173
Conc: 10.42 ng/ml

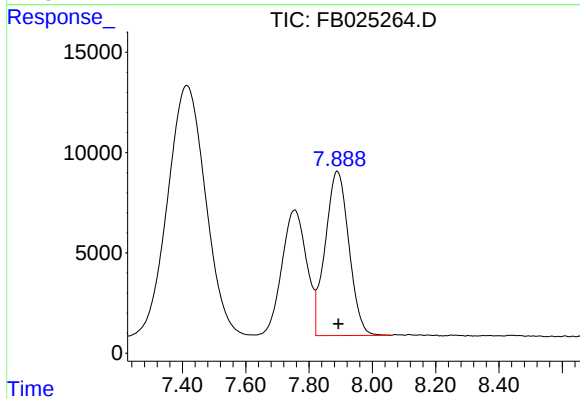

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.004 min
Response: 425865
Conc: 10.71 ng/ml

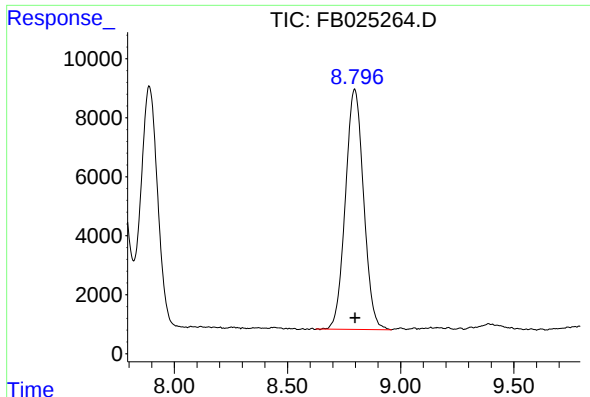

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 455659
Conc: 20.18 ng/ml

Instrument :
FID_B
ClientSampleId :

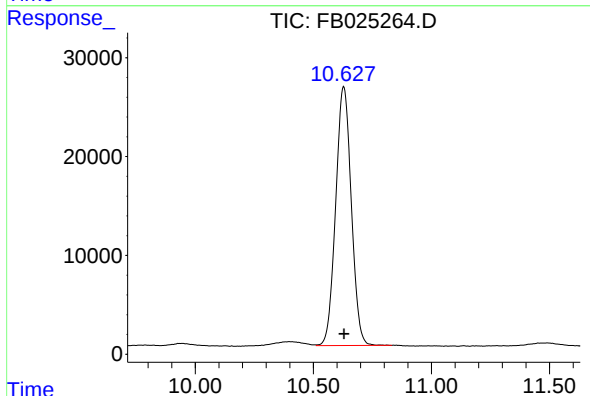


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 1204120
Conc: 32.20 ng/ml

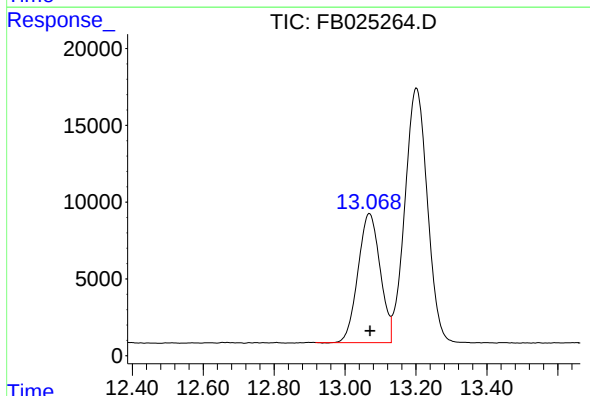


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 364882
Conc: 10.63 ng/ml

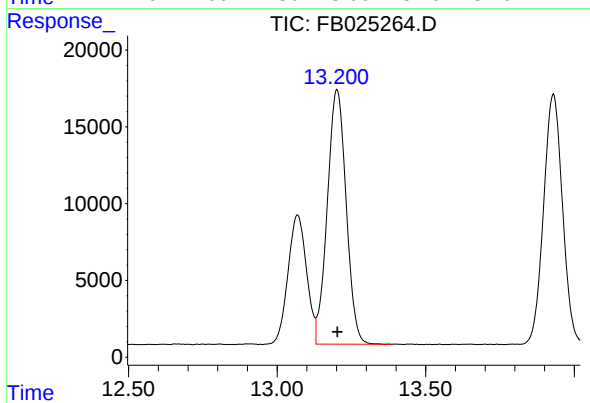

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 732553
Conc: 21.70 ng/ml

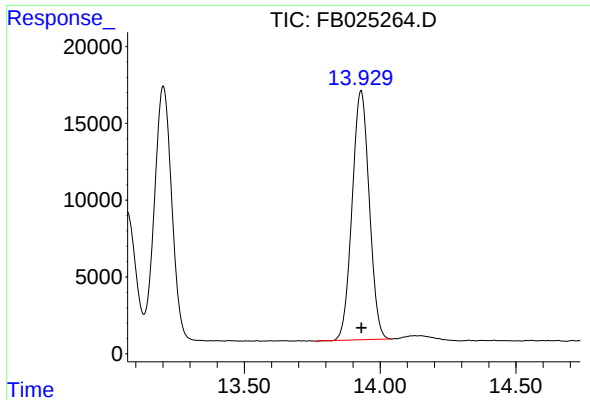

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 711265
Conc: 21.75 ng/ml

Instrument :
FID_B
ClientSampleId :

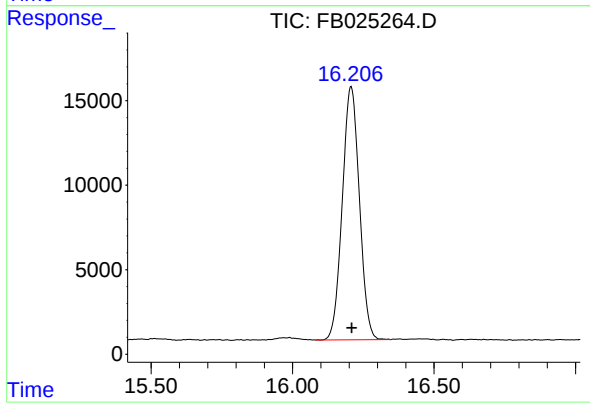

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 629059
Conc: 22.86 ng/ml