

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
 Data File : FB025252.D
 Signal(s) : FID2B.CH
 Acq On : 24 Nov 2020 9:56
 Operator : DD/AJ
 Sample : BSF1124S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1124S1

Integration File: Calibration.e
 Quant Time: Nov 25 00:26:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	449611	19.912 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	1031244	31.949 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1090564	32.870 ng/ml
3) t n-Heptane	7.755	359226	10.937 ng/ml
4) t Benzene	7.890	427933	10.763 ng/ml
6) t Toluene	10.629	1224411	32.746 ng/ml
7) t Ethylbenzene	13.069	372351	10.843 ng/ml
8) t m-Xylene	13.202	743921	22.033 ng/ml
9) t O-Xylene	13.930	731813	22.382 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	628191	22.831 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
Data File : FB025252.D
Signal(s) : FID2B.CH
Acq On : 24 Nov 2020 9:56
Operator : DD/AJ
Sample : BSF1124S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1124S1

Integration File: Calibration.e
Quant Time: Nov 25 00:26:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

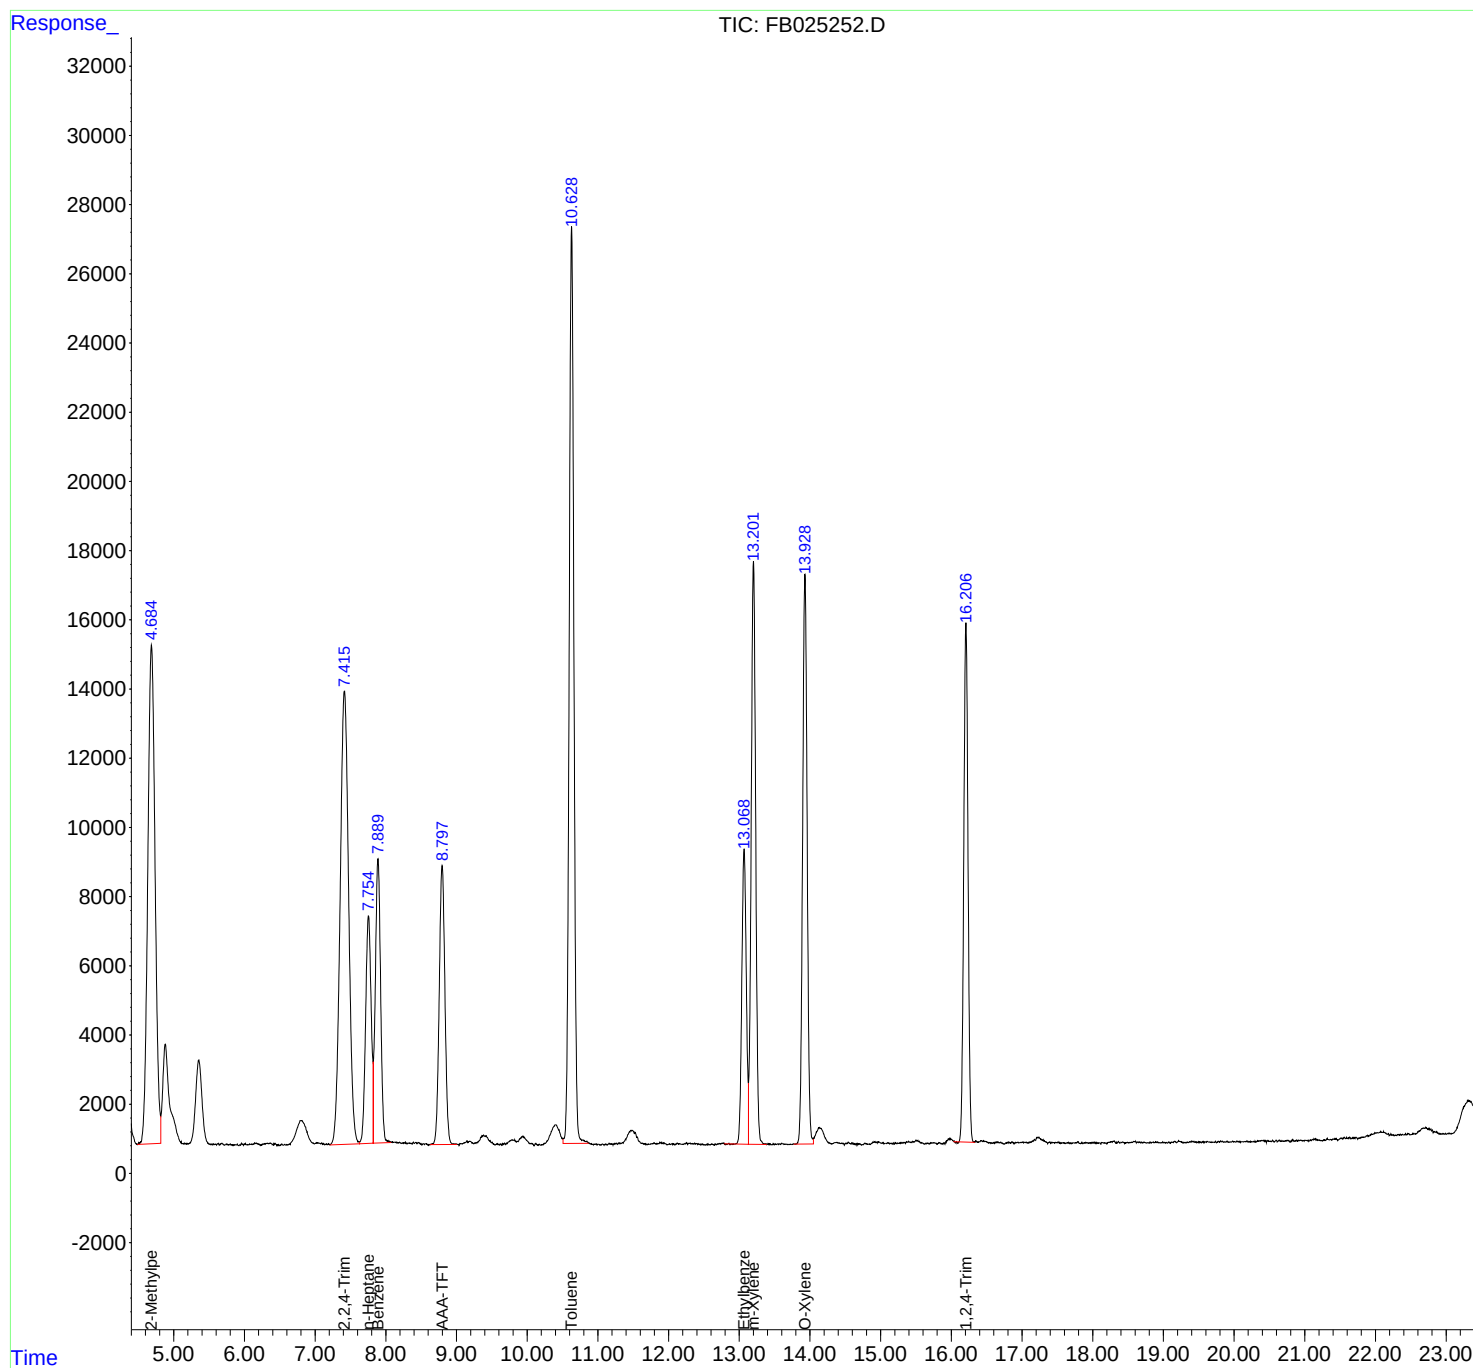


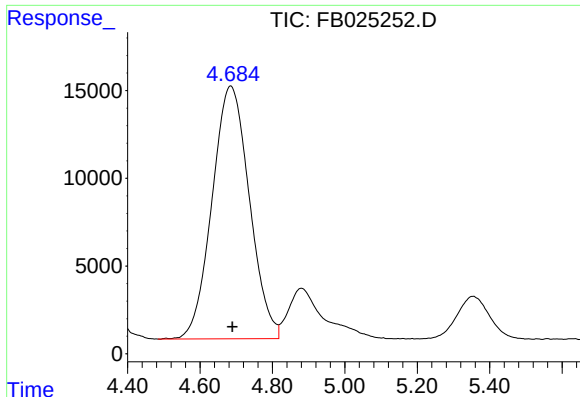

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.004 min
Response: 1031244
Conc: 31.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1124S1

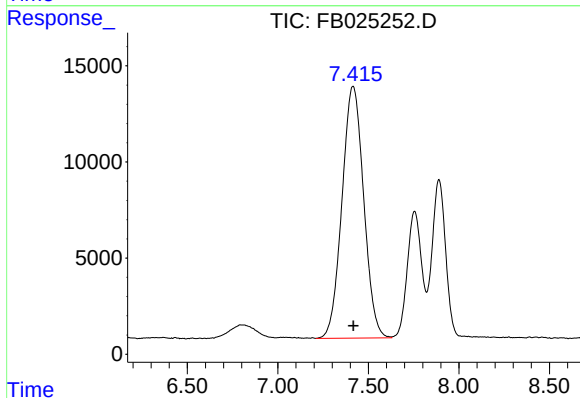


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 1090564
Conc: 32.87 ng/ml

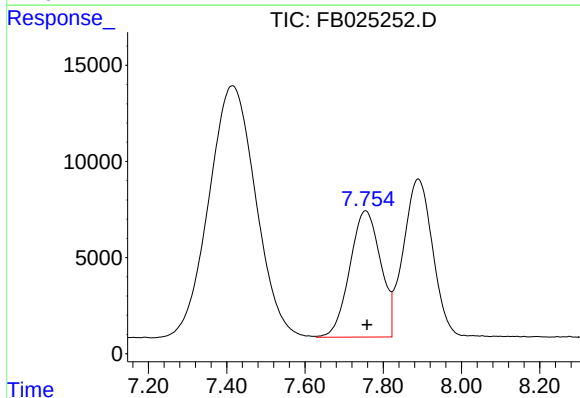


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 359226
Conc: 10.94 ng/ml

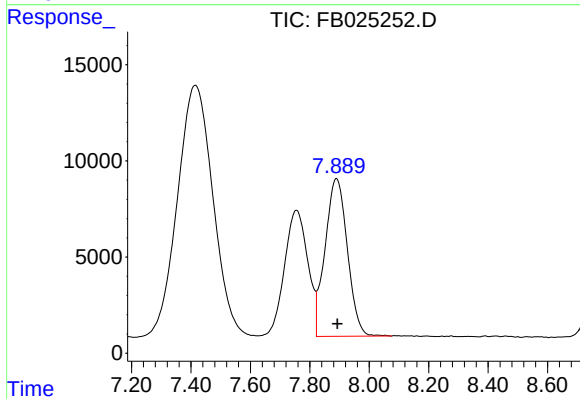

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 427933
Conc: 10.76 ng/ml

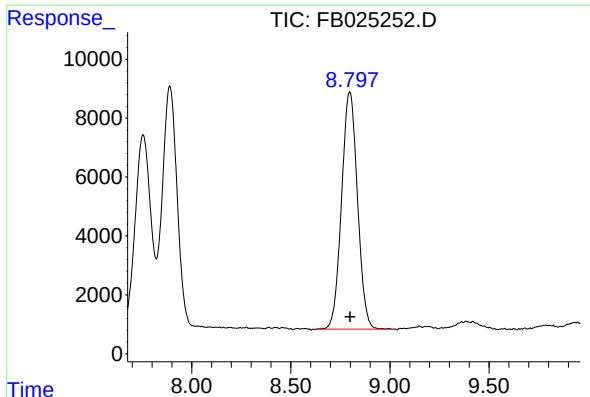

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.001 min
Response: 449611
Conc: 19.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1124S1

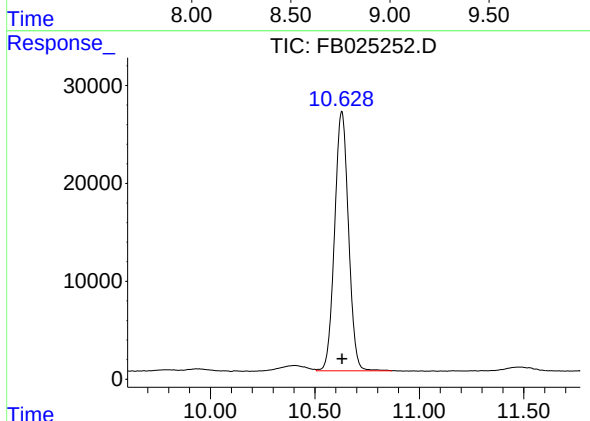


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1224411
Conc: 32.75 ng/ml

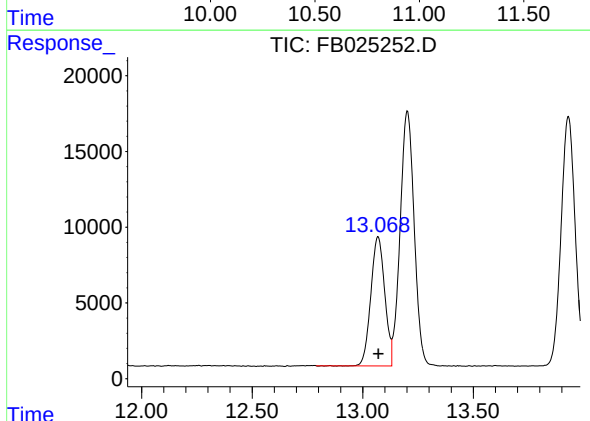


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 372351
Conc: 10.84 ng/ml

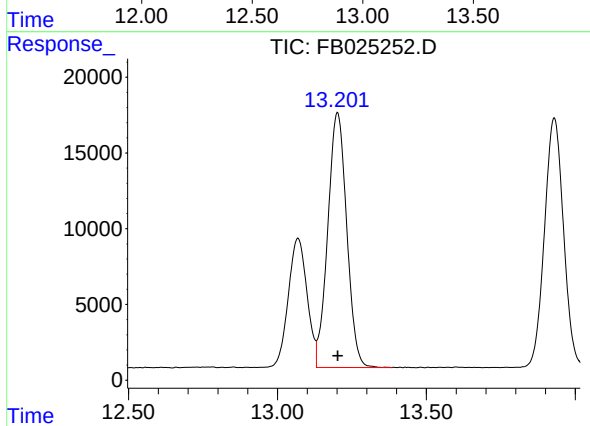

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.001 min
Response: 743921
Conc: 22.03 ng/ml

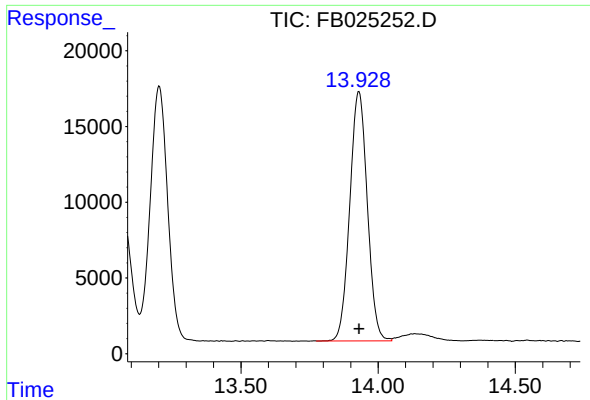

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 731813
Conc: 22.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1124S1

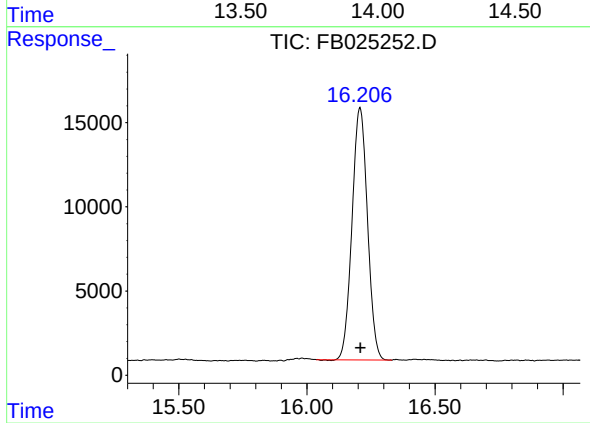

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.001 min
Response: 628191
Conc: 22.83 ng/ml