

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
 Data File : FB025255.D
 Signal(s) : FID2B.CH
 Acq On : 24 Nov 2020 11:27
 Operator : DD/AJ
 Sample : L4800-05MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B1-111820-8-10MS

Integration File: Calibration.e
 Quant Time: Nov 25 00:26:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	202018	8.947 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.696	419193	12.987 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	405035	12.208 ng/ml
3) t n-Heptane	7.760	129873	3.954 ng/ml
4) t Benzene	7.892	166567	4.189 ng/ml
6) t Toluene	10.631	434337	11.616 ng/ml
7) t Ethylbenzene	13.069	130404	3.797 ng/ml
8) t m-Xylene	13.202	248509	7.360 ng/ml
9) t O-Xylene	13.931	231926	7.093 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	164543	5.980 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
Data File : FB025255.D
Signal(s) : FID2B.CH
Acq On : 24 Nov 2020 11:27
Operator : DD/AJ
Sample : L4800-05MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

Integration File: Calibration.e
Quant Time: Nov 25 00:26:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

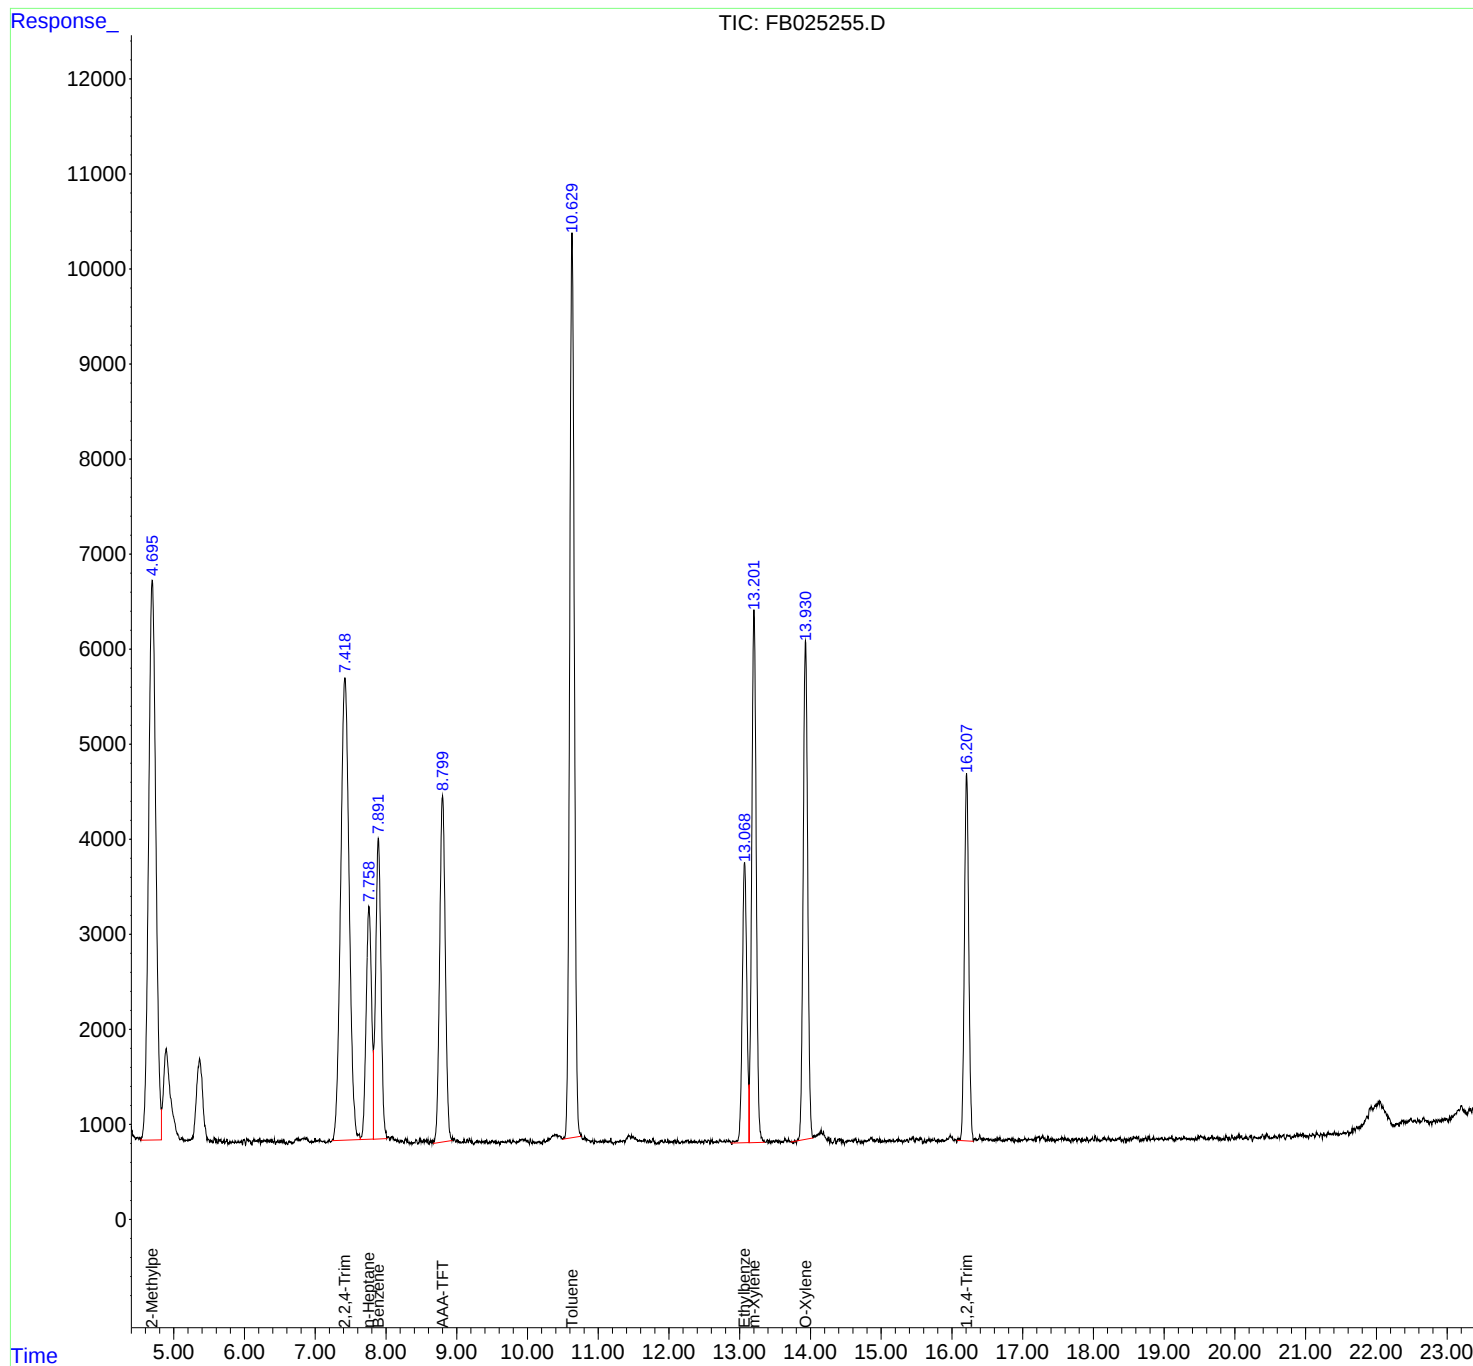


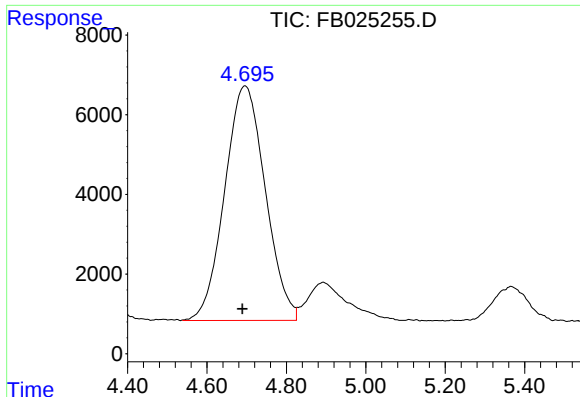

#1 2-Methylpentane


R.T.: 4.696 min
Delta R.T.: 0.007 min
Response: 419193
Conc: 12.99 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

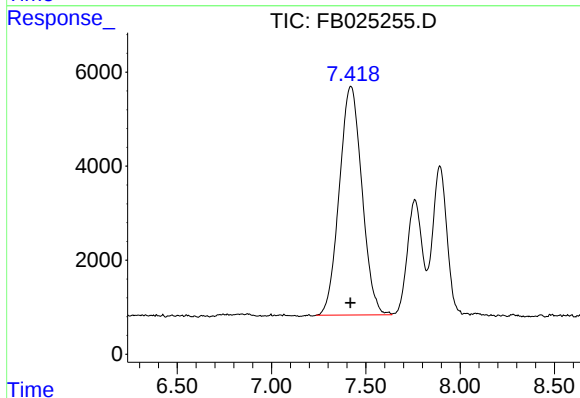


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.002 min
Response: 405035
Conc: 12.21 ng/ml

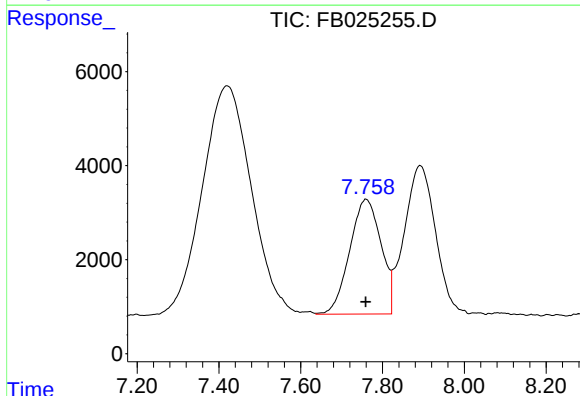


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.001 min
Response: 129873
Conc: 3.95 ng/ml

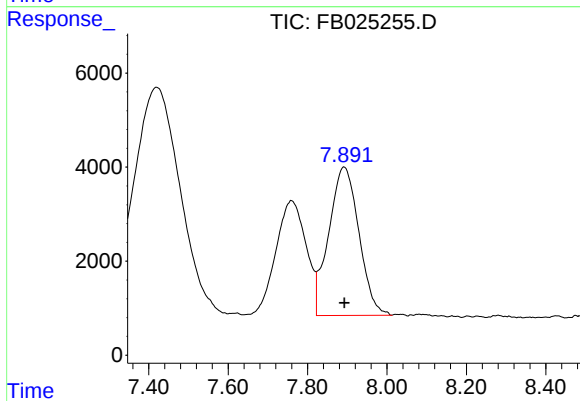

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 166567
Conc: 4.19 ng/ml

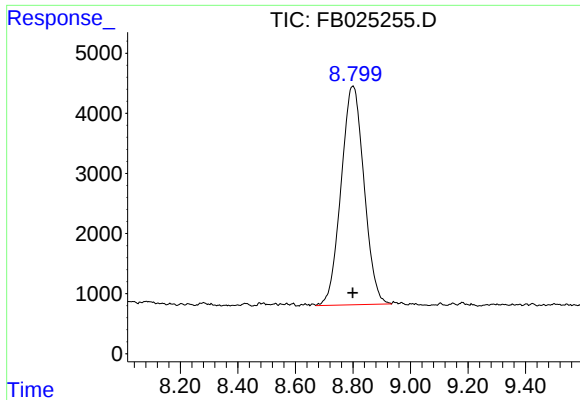

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.001 min
Response: 202018
Conc: 8.95 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

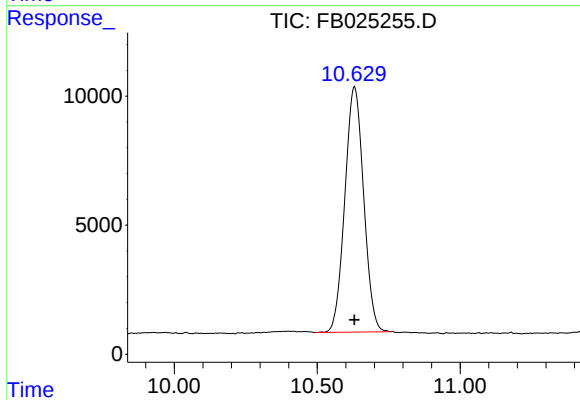


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 434337
Conc: 11.62 ng/ml

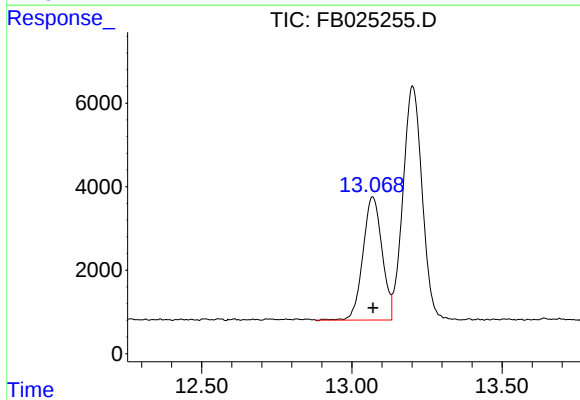


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 130404
Conc: 3.80 ng/ml

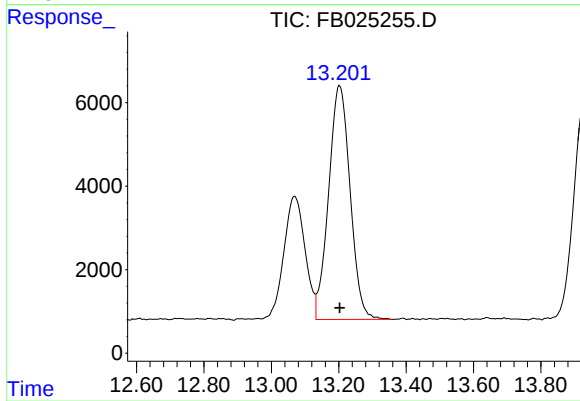

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 248509
Conc: 7.36 ng/ml

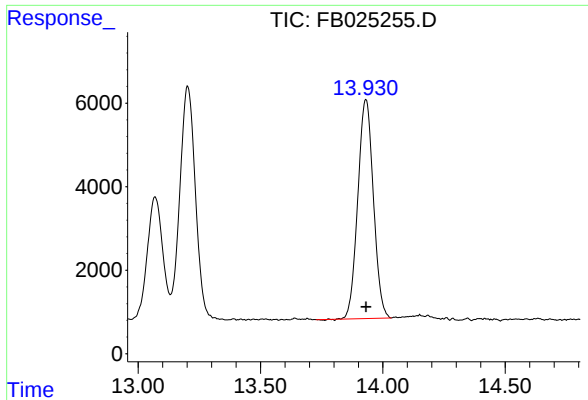

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 231926
Conc: 7.09 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

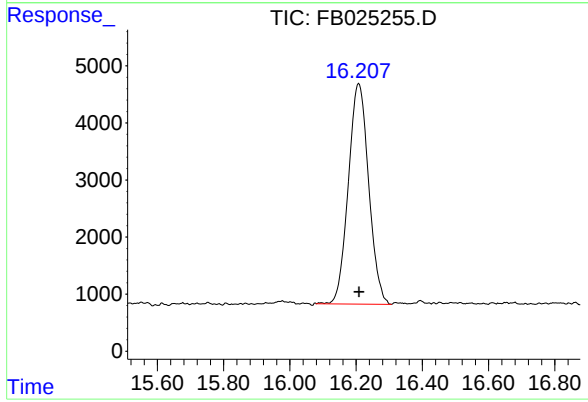

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 164543
Conc: 5.98 ng/ml