

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
 Data File : FB025269.D
 Signal(s) : FID2B.CH
 Acq On : 24 Nov 2020 18:37
 Operator : DD/AJ
 Sample : L4800-05MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B1-111820-8-10MS

Integration File: Calibration.e
 Quant Time: Nov 25 00:28:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
 Quant Title :
 QLast Update : Wed Nov 04 08:05:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	468631	20.755 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	924004	28.627 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	985772	29.712 ng/ml
3) t n-Heptane	7.756	323688	9.855 ng/ml
4) t Benzene	7.890	392298	9.867 ng/ml
6) t Toluene	10.628	1094880	29.282 ng/ml
7) t Ethylbenzene	13.067	333695	9.717 ng/ml
8) t m-Xylene	13.200	673581	19.949 ng/ml
9) t O-Xylene	13.928	647802	19.813 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	570585	20.737 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112420\
Data File : FB025269.D
Signal(s) : FID2B.CH
Acq On : 24 Nov 2020 18:37
Operator : DD/AJ
Sample : L4800-05MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

Integration File: Calibration.e
Quant Time: Nov 25 00:28:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB110320.M
Quant Title :
QLast Update : Wed Nov 04 08:05:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

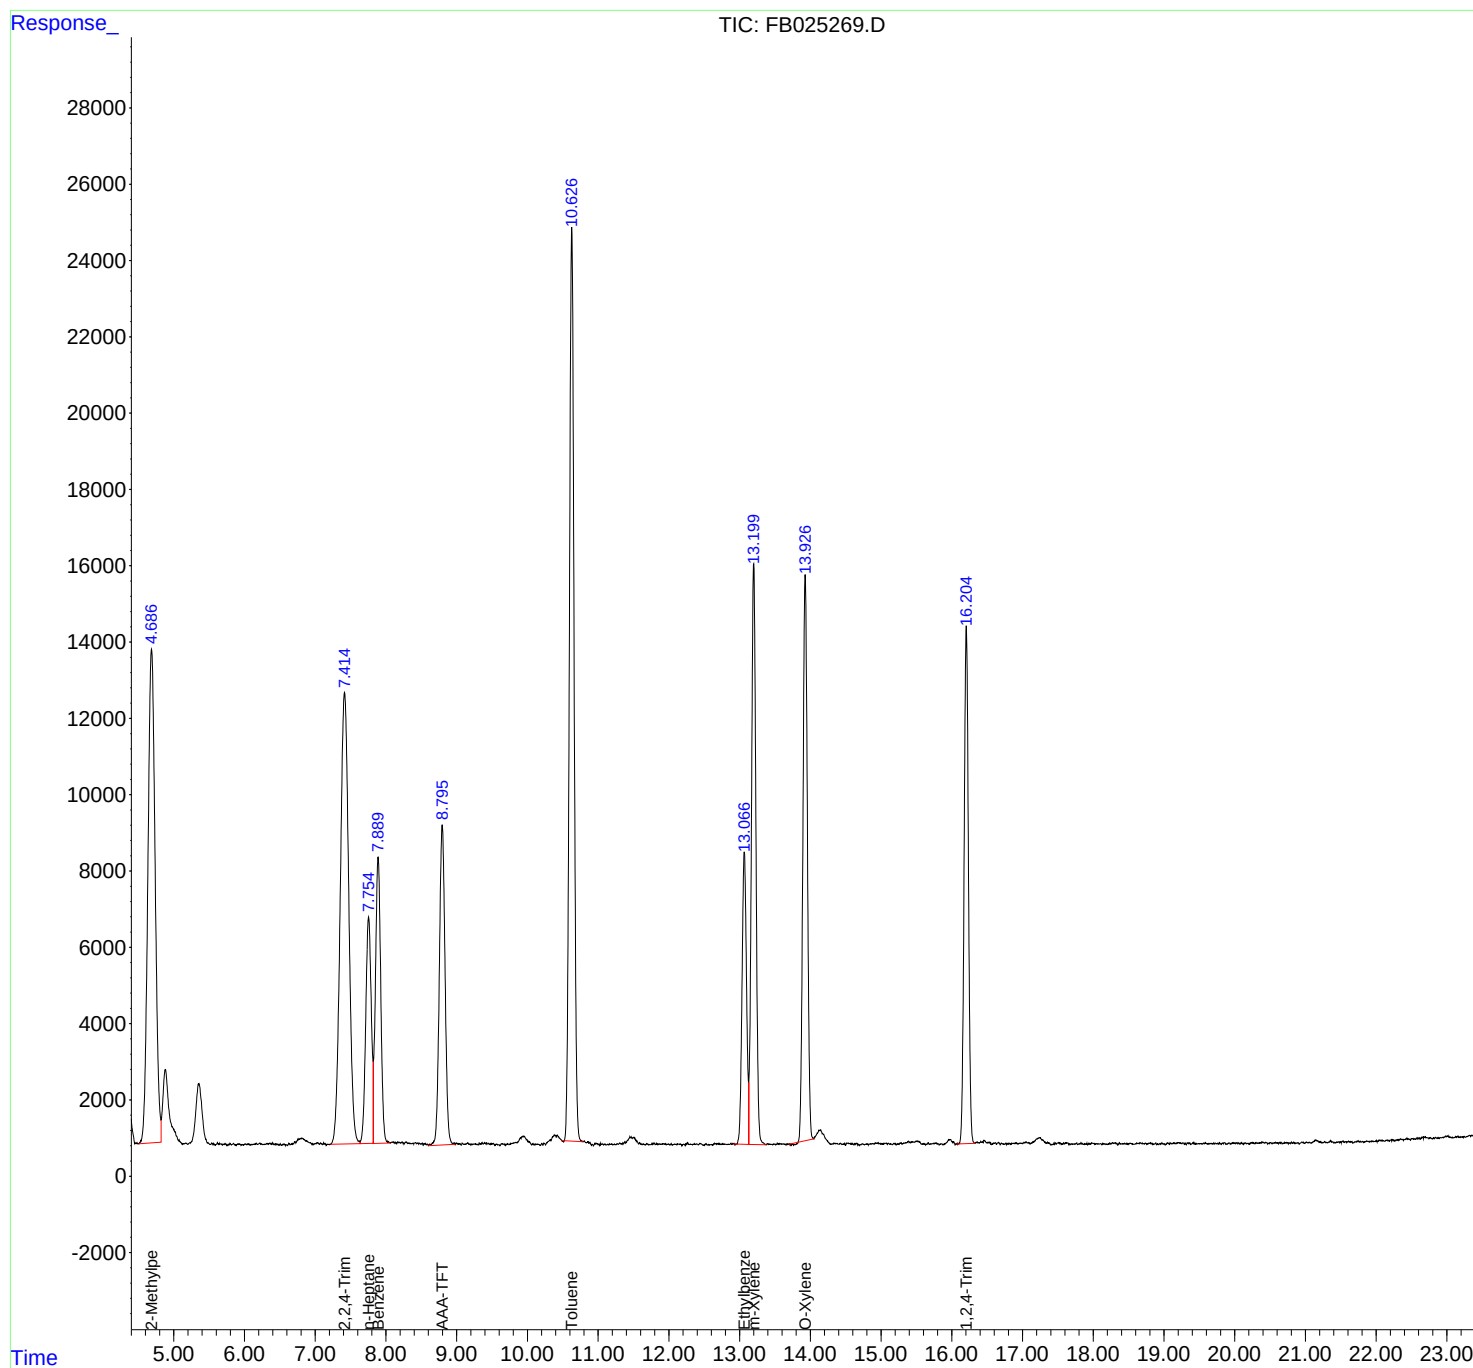


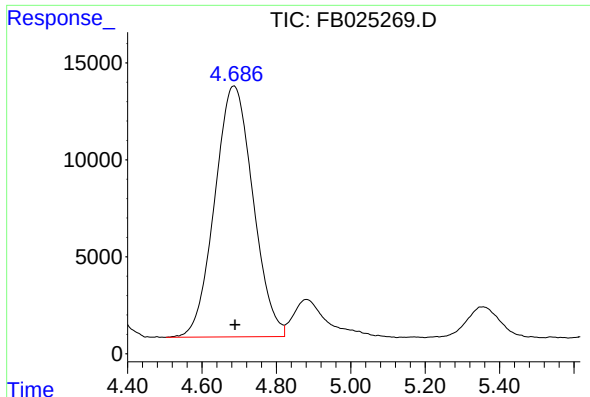

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 924004
Conc: 28.63 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

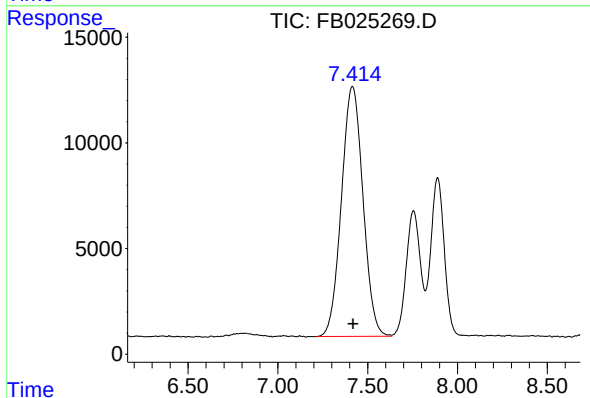


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 985772
Conc: 29.71 ng/ml

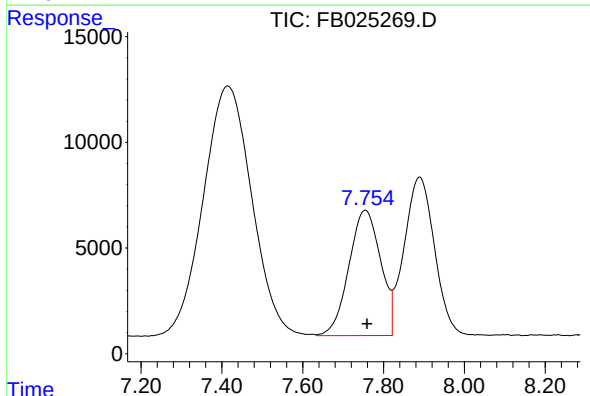


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 323688
Conc: 9.85 ng/ml

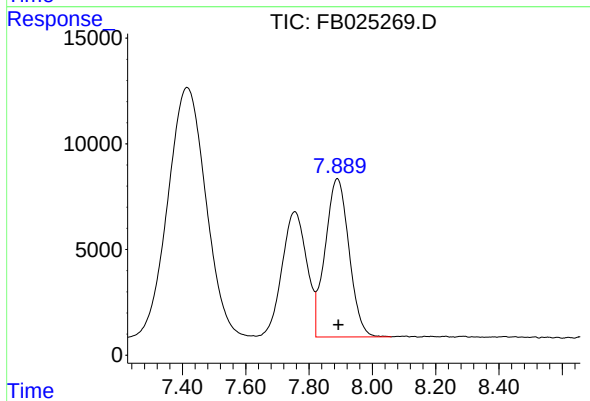

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 392298
Conc: 9.87 ng/ml

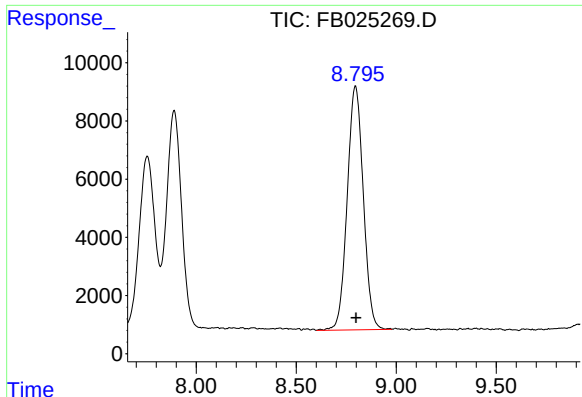

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 468631
Conc: 20.75 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

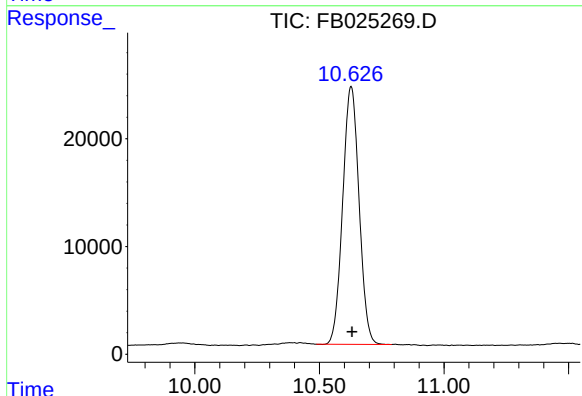


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1094880
Conc: 29.28 ng/ml

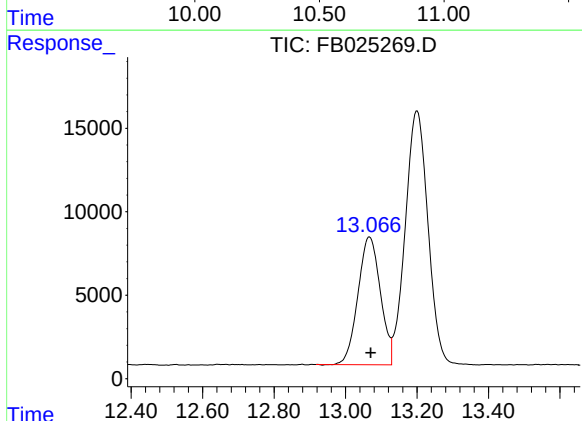


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.003 min
Response: 333695
Conc: 9.72 ng/ml

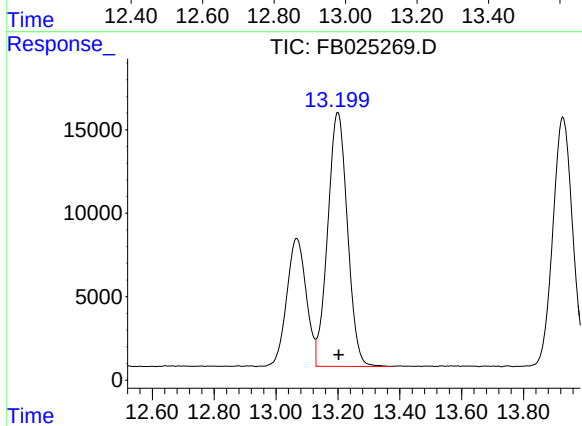

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 673581
Conc: 19.95 ng/ml

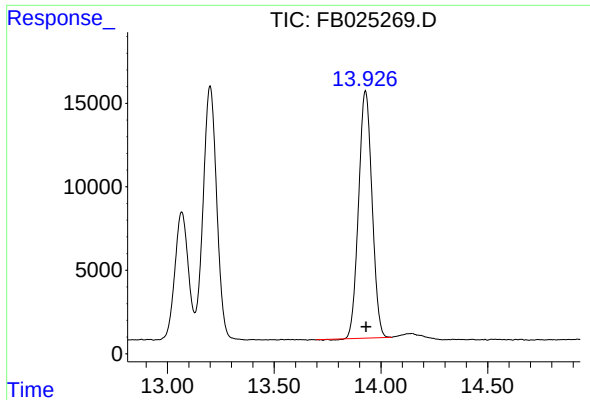

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.003 min
Response: 647802
Conc: 19.81 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B1-111820-8-10MS

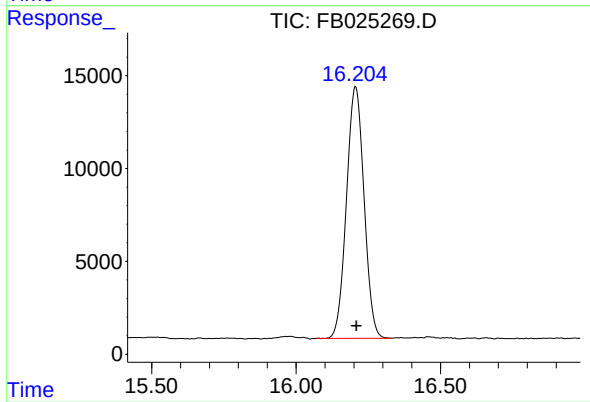

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 570585
Conc: 20.74 ng/ml