

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112519\
Data File : FB023087.D
Signal(s) : FID2B.CH
Acq On : 25 Nov 2019 15:27
Operator : DD/AJ
Sample : K5663-02MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 26 00:25:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	469240	19.103 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	913142	27.943 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	957207	27.450 ng/ml
3) t	n-Heptane	7.756	310807	9.040 ng/ml
4) t	Benzene	7.890	403242	9.678 ng/ml
6) t	Toluene	10.628	1174090	29.145 ng/ml
7) t	Ethylbenzene	13.069	364980	9.458 ng/ml
8) t	m-Xylene	13.202	685308	18.832 ng/ml
9) t	O-Xylene	13.929	654208	18.842 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	515415	18.379 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112519\
Data File : FB023087.D
Signal(s) : FID2B.CH
Acq On : 25 Nov 2019 15:27
Operator : DD/AJ
Sample : K5663-02MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 26 00:25:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

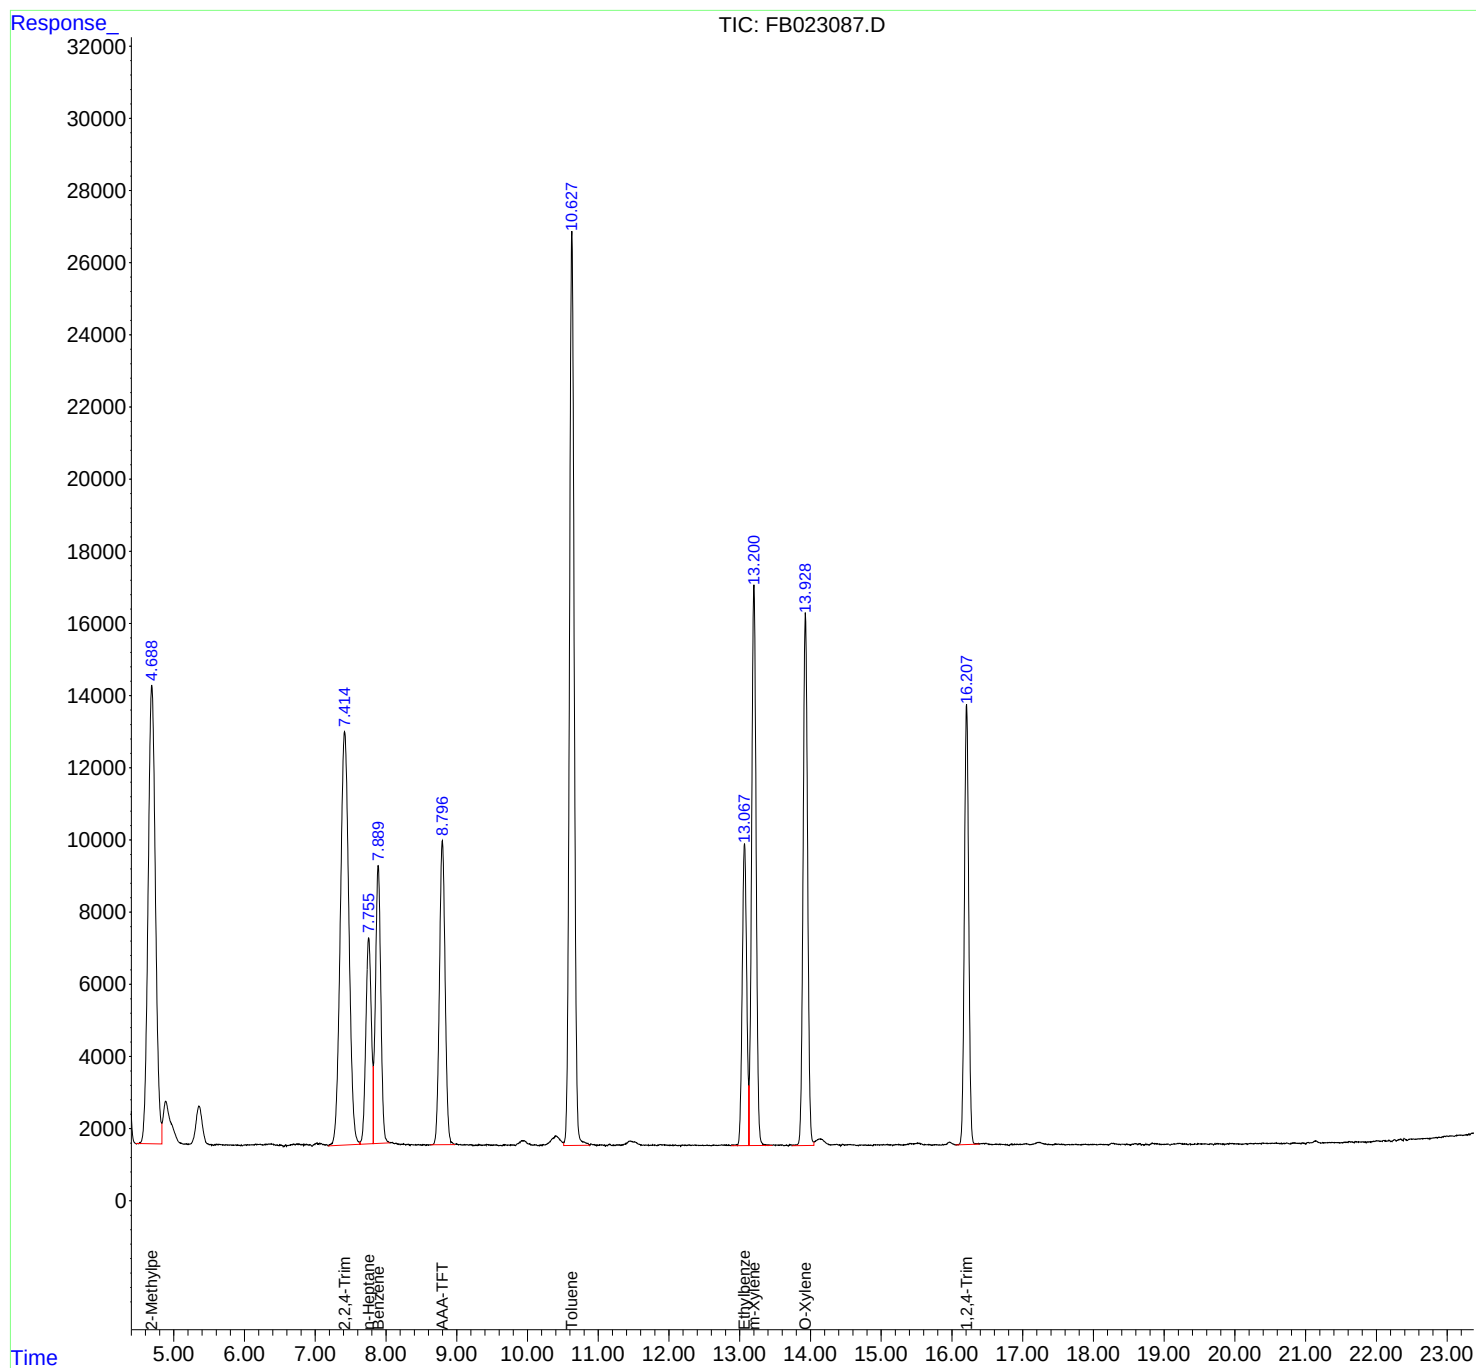

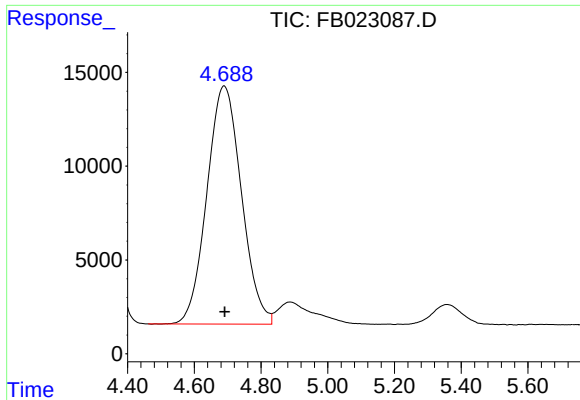


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 913142
Conc: 27.94 ng/ml

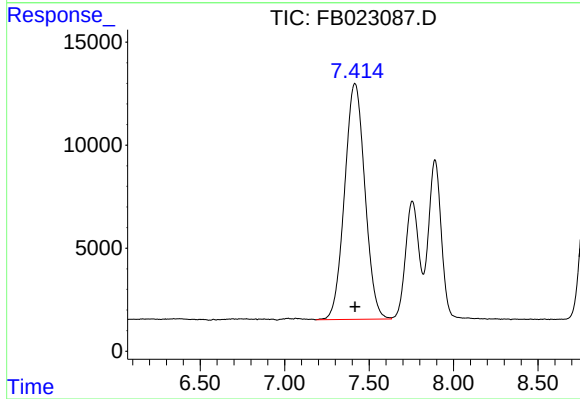


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 957207
Conc: 27.45 ng/ml

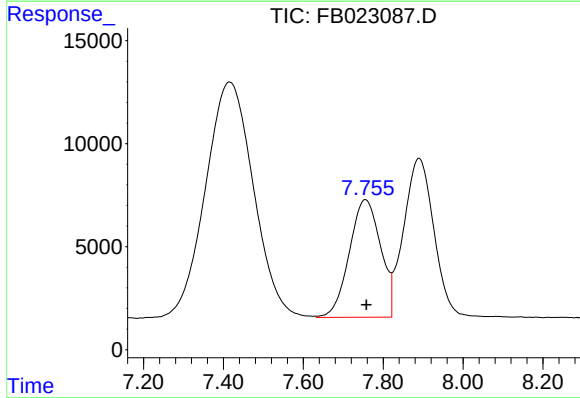


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 310807
Conc: 9.04 ng/ml

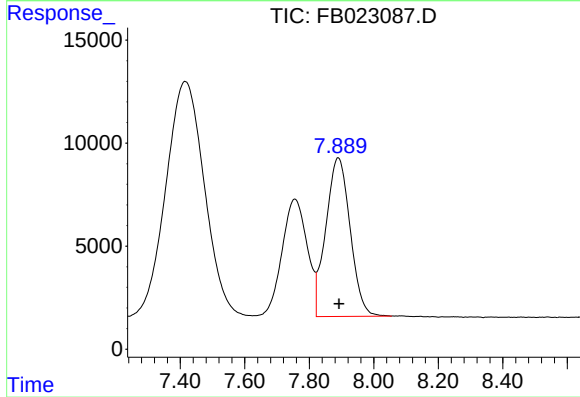


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 403242
Conc: 9.68 ng/ml

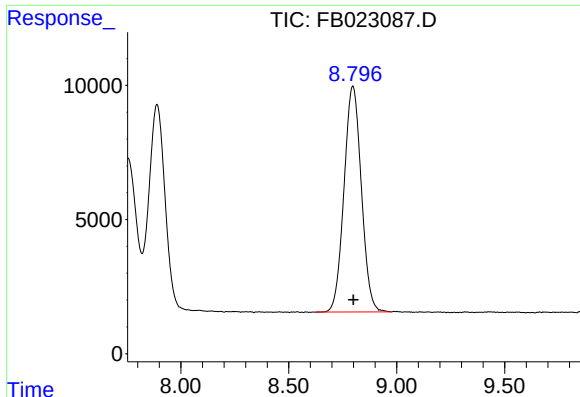


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 469240
Conc: 19.10 ng/ml

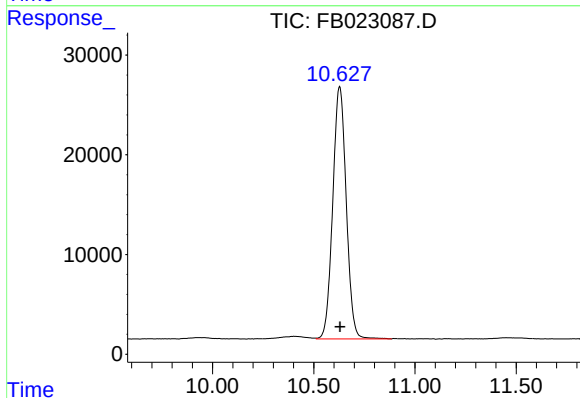


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1174090
Conc: 29.15 ng/ml

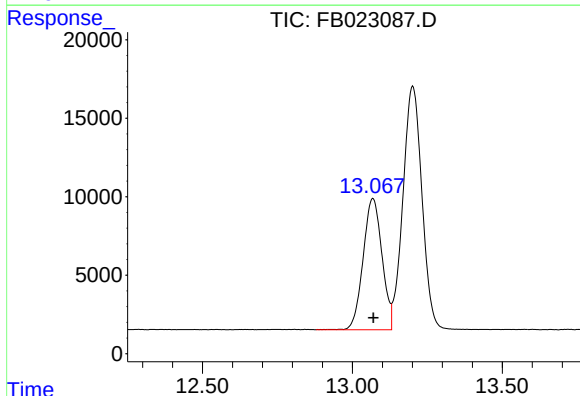


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 364980
Conc: 9.46 ng/ml

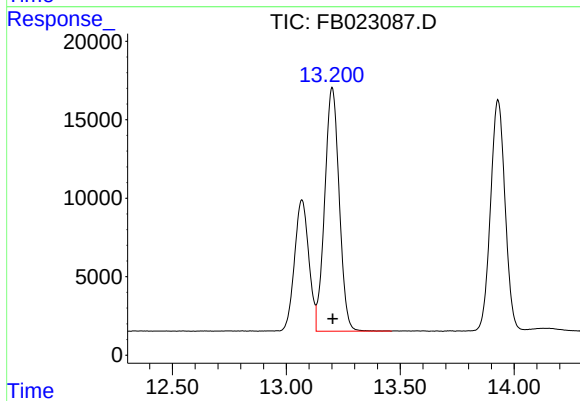


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 685308
Conc: 18.83 ng/ml

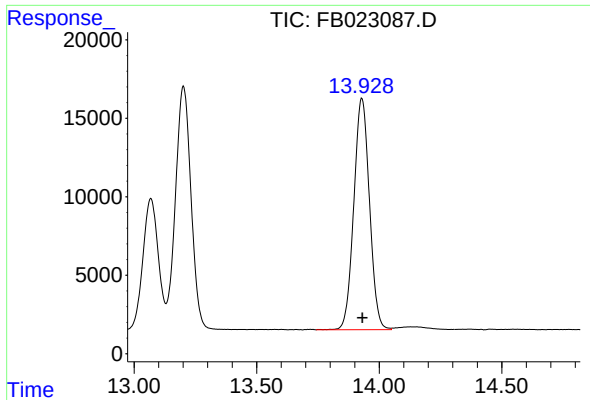

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 654208
Conc: 18.84 ng/ml

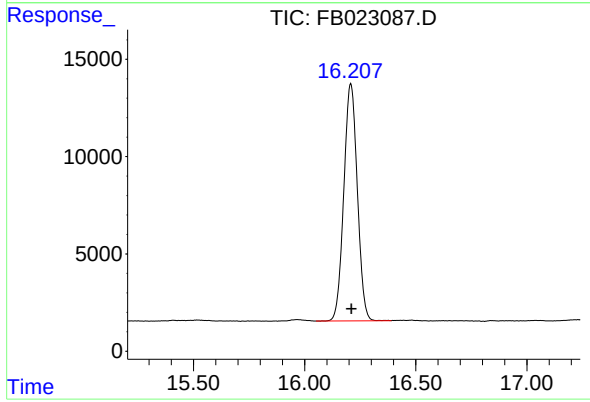

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 515415
Conc: 18.38 ng/ml