

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112519\
 Data File : FB023088.D
 Signal(s) : FID2B.CH
 Acq On : 25 Nov 2019 16:13
 Operator : DD/AJ
 Sample : K5663-02MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Nov 26 00:25:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	542638	22.091 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	1041575	31.874 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1153189	33.071 ng/ml
3) t n-Heptane	7.755	379211	11.029 ng/ml
4) t Benzene	7.889	450348	10.809 ng/ml
6) t Toluene	10.628	1308453	32.481 ng/ml
7) t Ethylbenzene	13.068	408001	10.573 ng/ml
8) t m-Xylene	13.201	769638	21.150 ng/ml
9) t O-Xylene	13.929	734864	21.165 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	607818	21.674 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112519\
Data File : FB023088.D
Signal(s) : FID2B.CH
Acq On : 25 Nov 2019 16:13
Operator : DD/AJ
Sample : K5663-02MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Nov 26 00:25:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

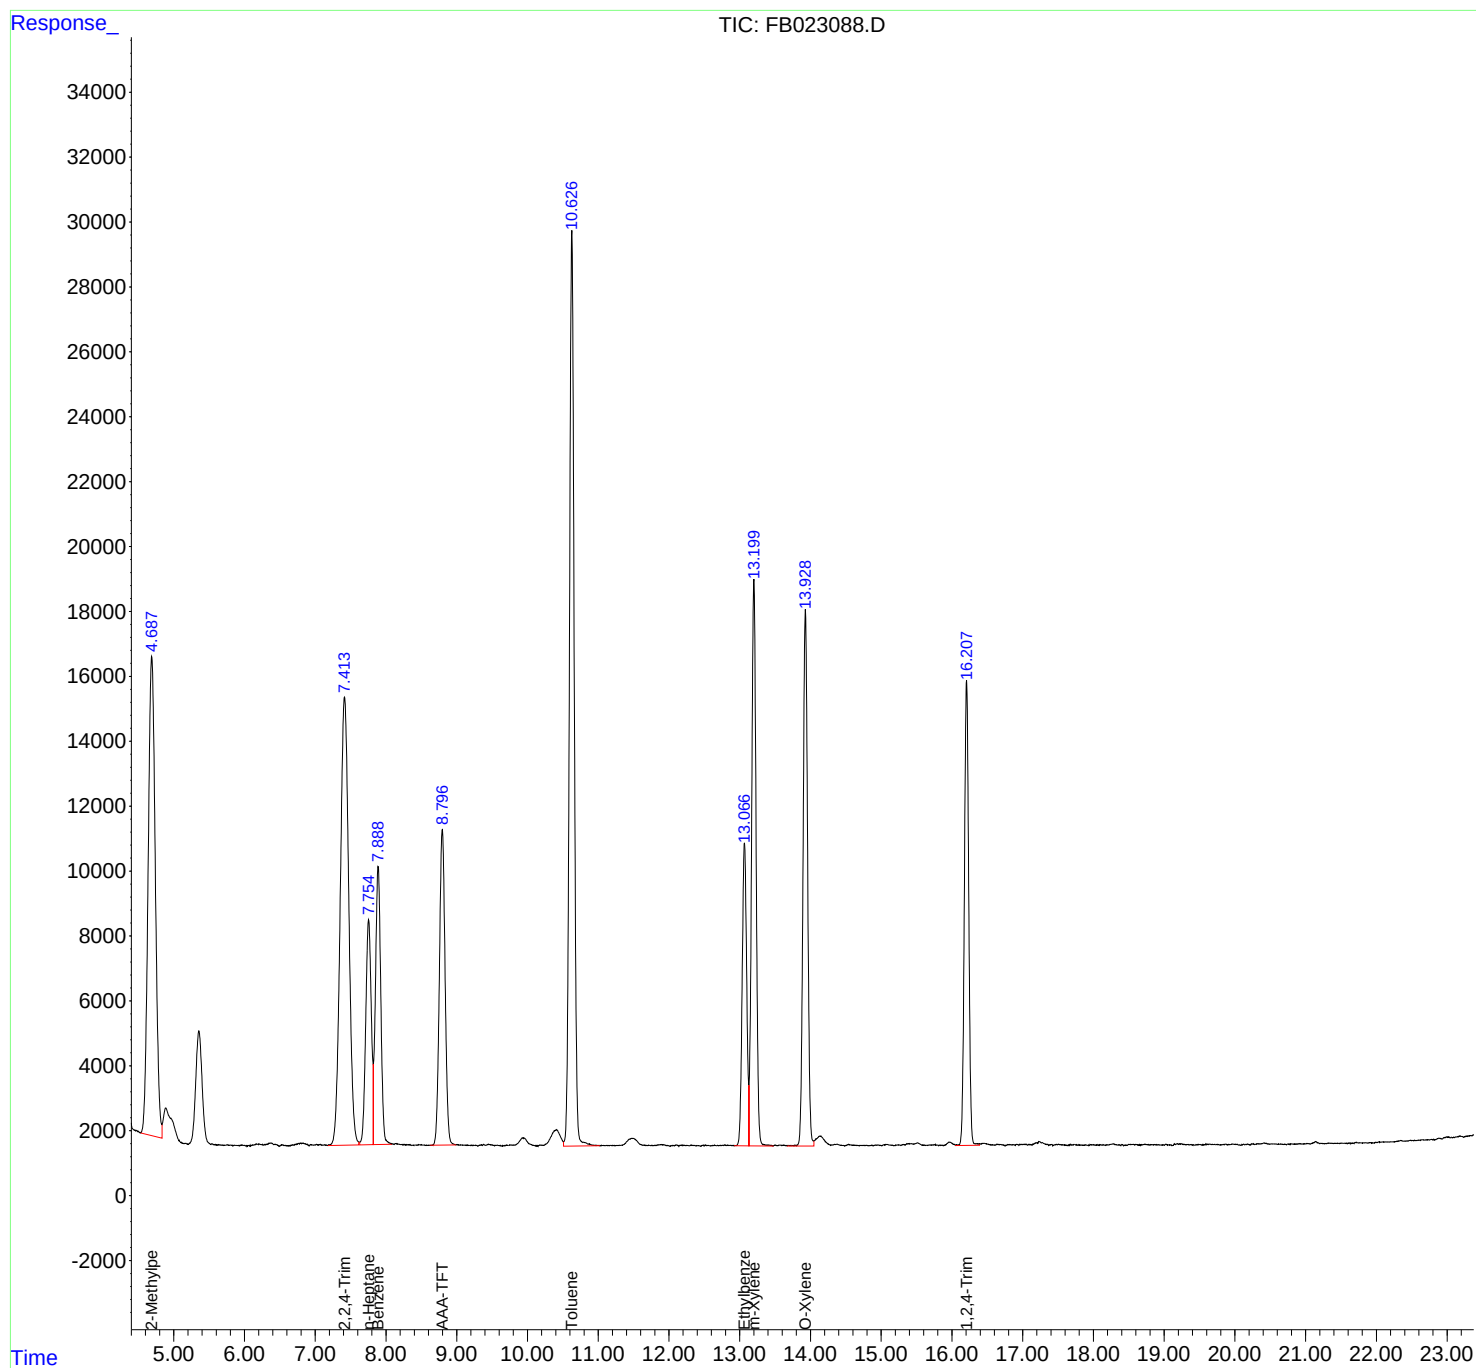

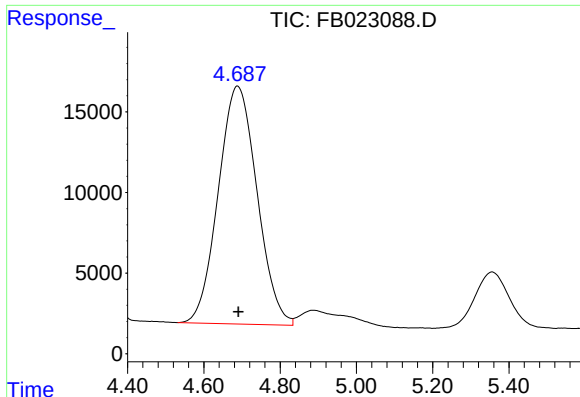


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 1041575
Conc: 31.87 ng/ml

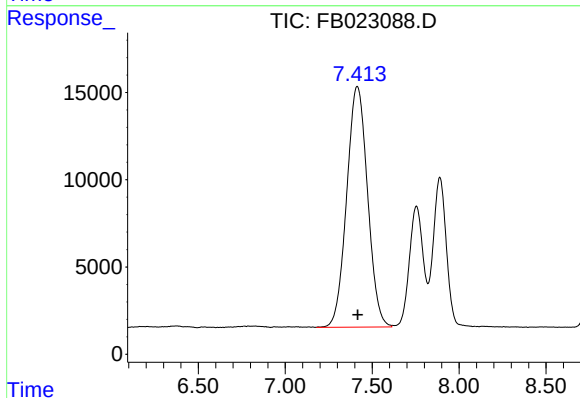


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 1153189
Conc: 33.07 ng/ml

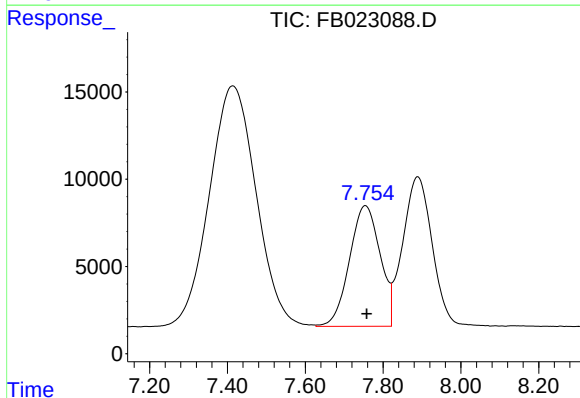


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 379211
Conc: 11.03 ng/ml

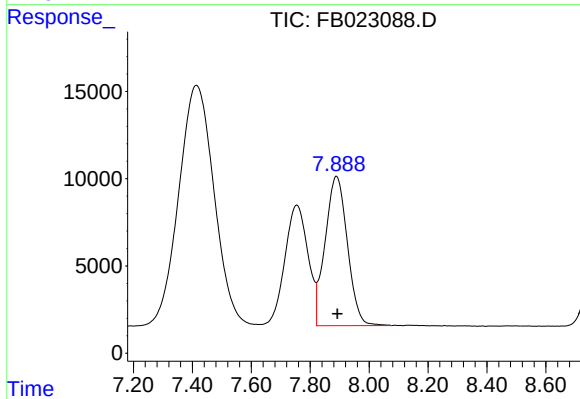


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 450348
Conc: 10.81 ng/ml

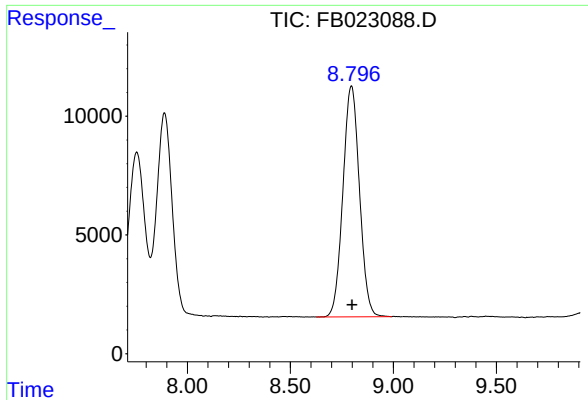


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 542638
Conc: 22.09 ng/ml

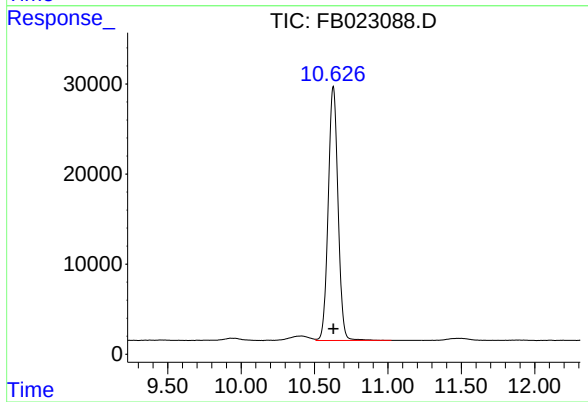


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1308453
Conc: 32.48 ng/ml

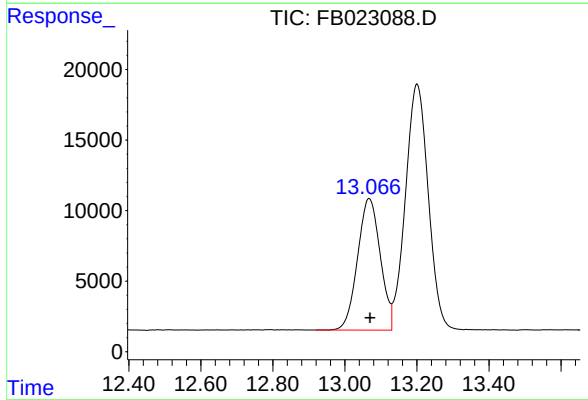


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 408001
Conc: 10.57 ng/ml

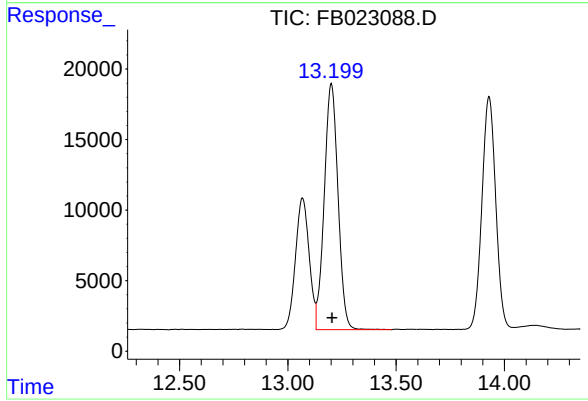


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 769638
Conc: 21.15 ng/ml

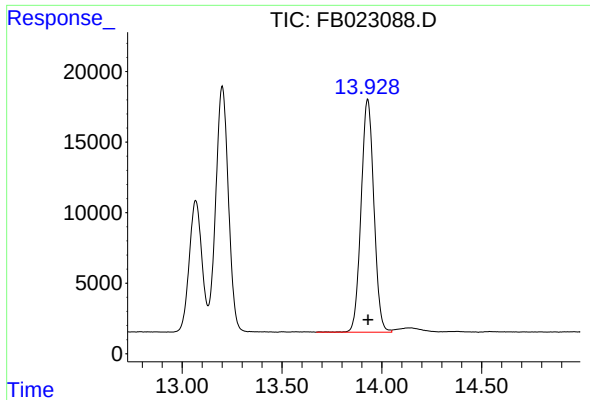

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 734864
Conc: 21.16 ng/ml

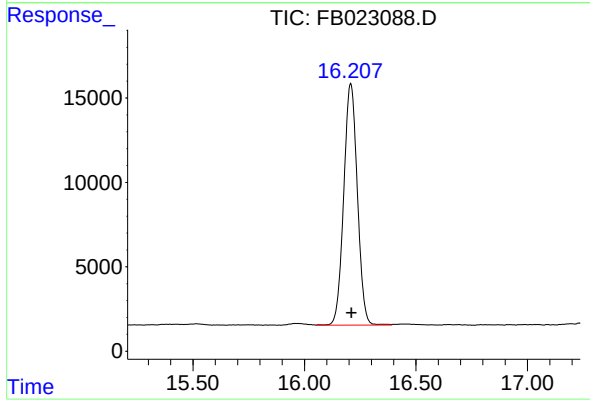

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 607818
Conc: 21.67 ng/ml